

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061423\
 Data File : BF133749.D
 Acq On : 14 Jun 2023 13:10
 Operator : CG\JU
 Sample : PB153411BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153411BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133749.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.140	6	9	20	rVB	30965	51014	1.35%	0.208%
2	5.069	504	507	514	rVB	50229	68161	1.80%	0.277%
3	5.457	567	573	576	rBV	3070513	3131841	82.83%	12.742%
4	6.463	738	744	747	rBV	2812666	3193741	84.46%	12.994%
5	6.828	803	806	810	rBV	969355	832098	22.01%	3.385%
6	7.398	897	903	906	rBV	2262515	2092150	55.33%	8.512%
7	8.116	1021	1025	1028	rBV	1320032	1083633	28.66%	4.409%
8	9.192	1204	1208	1211	rBV	4419499	3669353	97.04%	14.929%
9	9.869	1319	1323	1327	rBV	1429819	1207889	31.95%	4.914%
10	10.663	1453	1458	1461	rBV	2623696	2452207	64.85%	9.977%
11	11.357	1572	1576	1580	rBV	1415534	1291328	34.15%	5.254%
12	12.951	1842	1847	1850	rBV	4047039	3781148	100.00%	15.384%
13	14.004	2022	2026	2030	rBV	1108588	969352	25.64%	3.944%
14	15.468	2269	2275	2284	rBV	571228	754448	19.95%	3.070%




Sum of corrected areas: 24578363

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061423\
Data File : BF133749.D
Acq On : 14 Jun 2023 13:10
Operator : CG\JU
Sample : PB153411BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153411BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

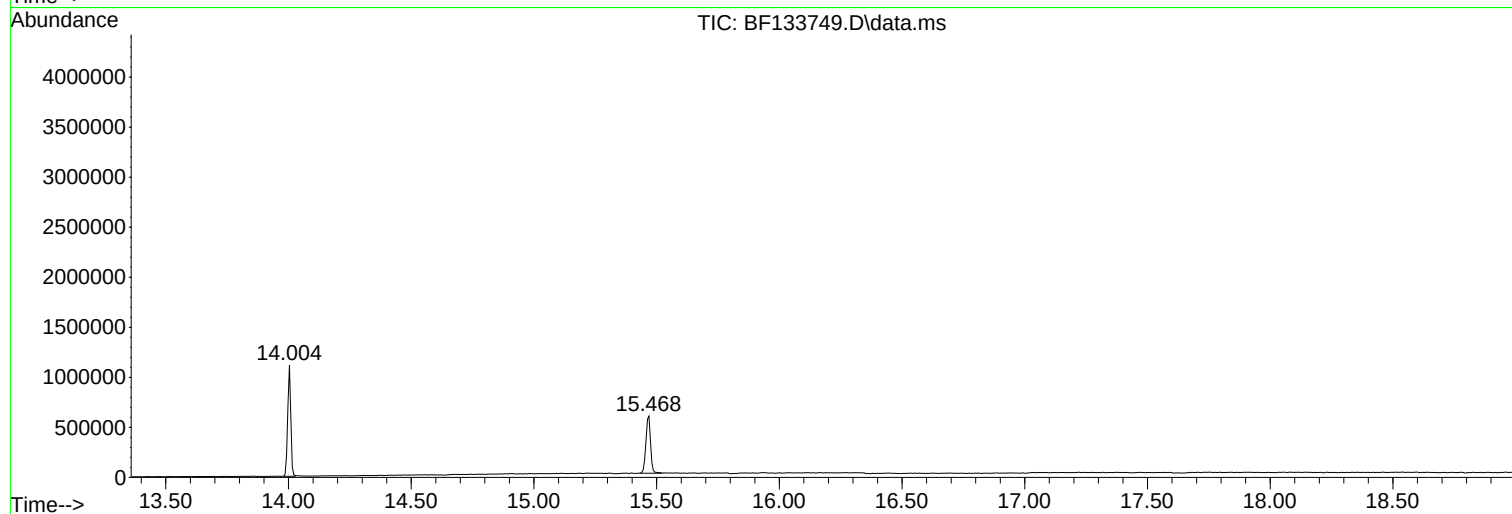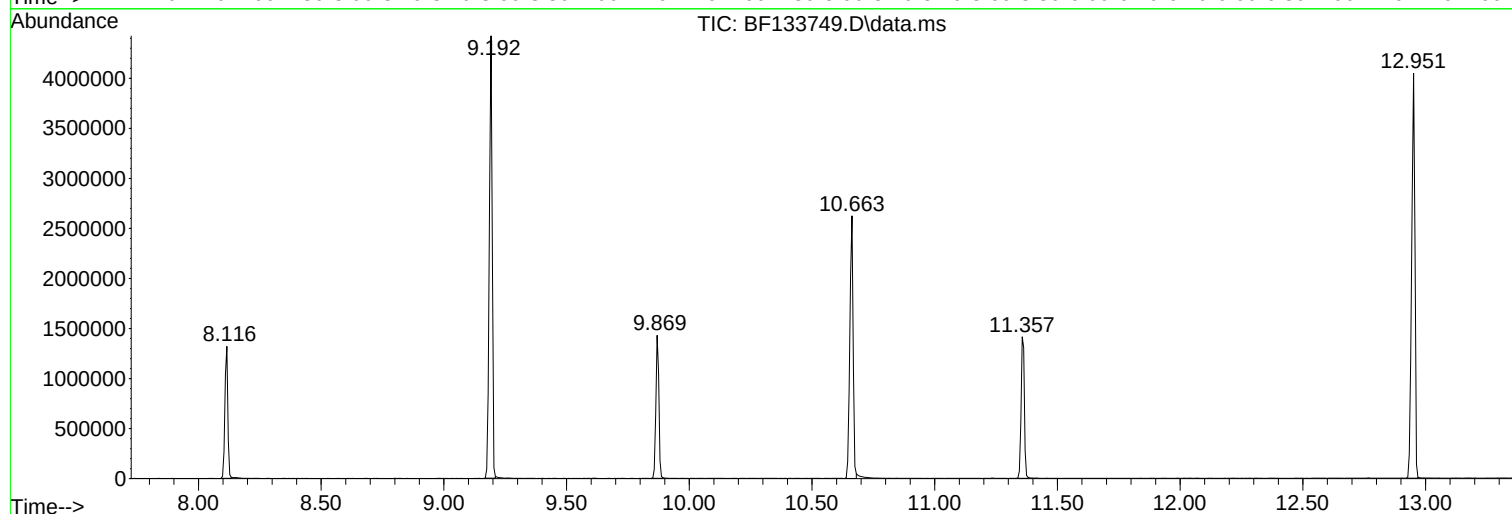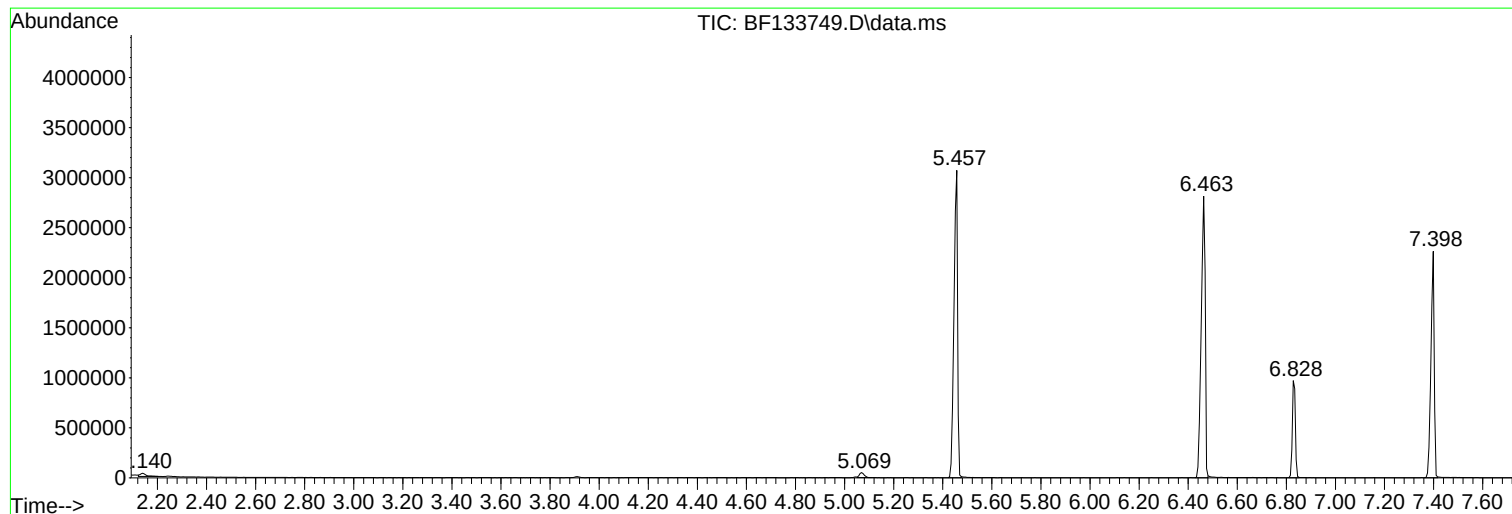

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061423\
Data File : BF133749.D
Acq On : 14 Jun 2023 13:10
Operator : CG\JU
Sample : PB153411BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153411BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061423\
Data File : BF133749.D
Acq On : 14 Jun 2023 13:10
Operator : CG\JU
Sample : PB153411BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153411BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------