
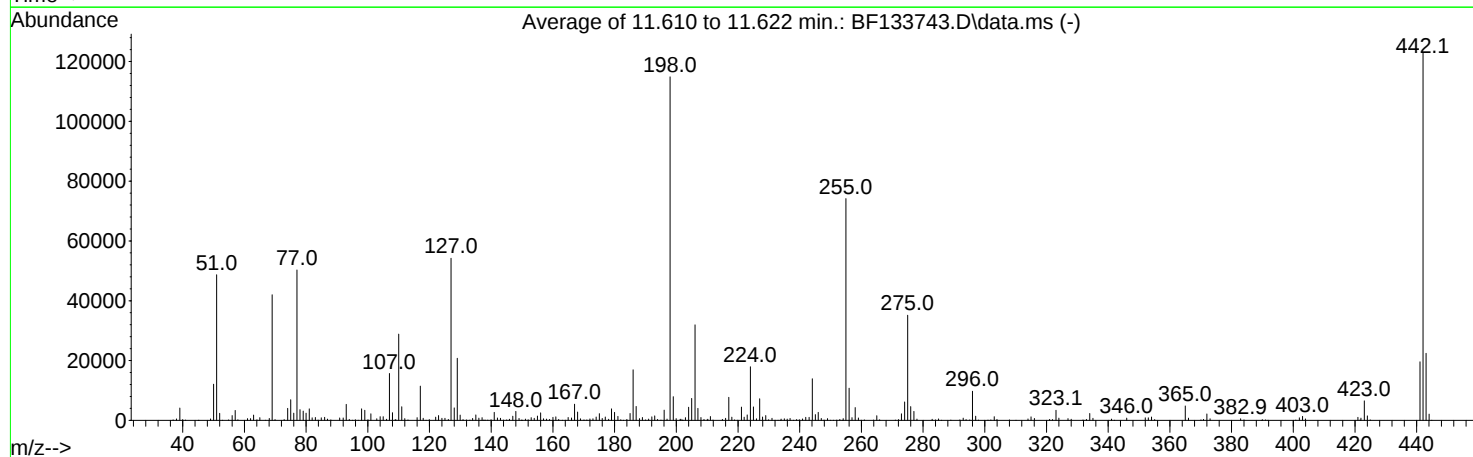


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061423\
 Data File : BF133743.D
 Acq On : 14 Jun 2023 09:58
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 14 16:27:59 2023

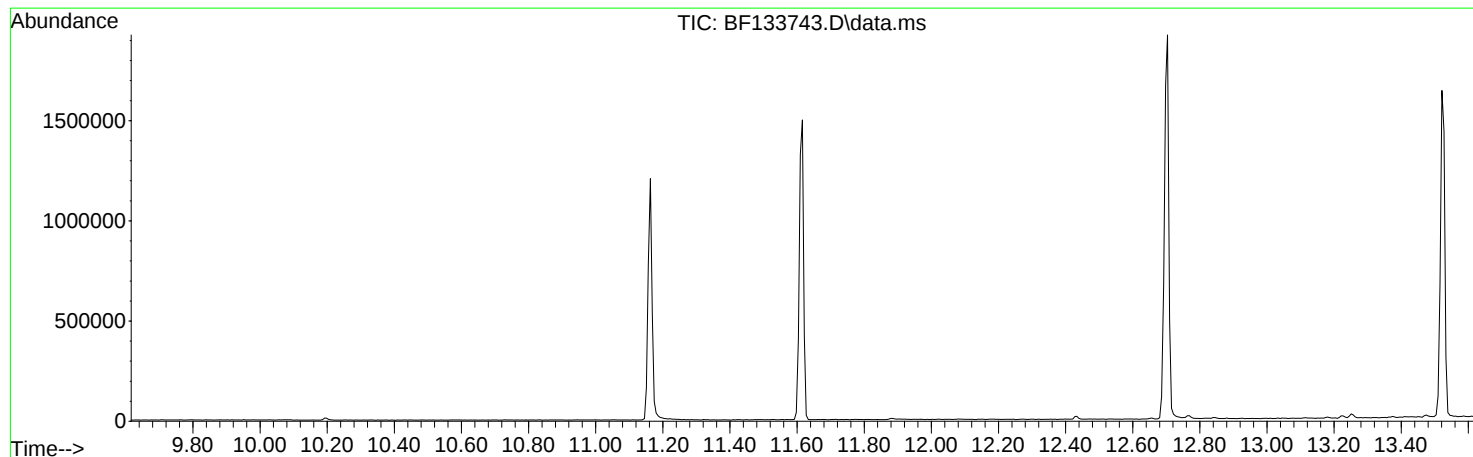

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	48713	PASS
68	69	0.00	2	1.5	630	PASS
69	198	0.00	100	36.6	42020	PASS
70	69	0.00	2	0.7	275	PASS
127	198	10	80	47.2	54202	PASS
197	198	0.00	2	0.4	423	PASS
198	198	100	100	100.0	114899	PASS
199	198	5	9	6.9	7928	PASS
275	198	10	60	30.6	35134	PASS
365	198	1	100	4.2	4805	PASS
441	198	0.01	100	17.0	19590	PASS
442	442	50	100	100.0	123024	PASS
443	442	15	24	18.2	22405	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/14/2023	BNA_F	<u>BF133743.D</u>
Compound Name	Response	Retention Time
DDT	284554	13.521
DDD	6016	13.251
DDE	199	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6215	290769	2.14

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061423\
Data File : BF133743.D
Acq On : 14 Jun 2023 09:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 14 10:23:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 11:26:55 2023
Response via : Initial Calibration

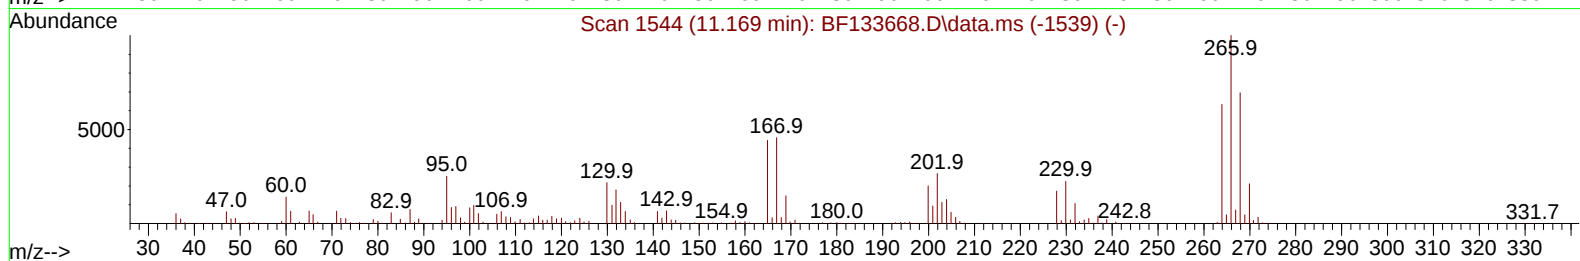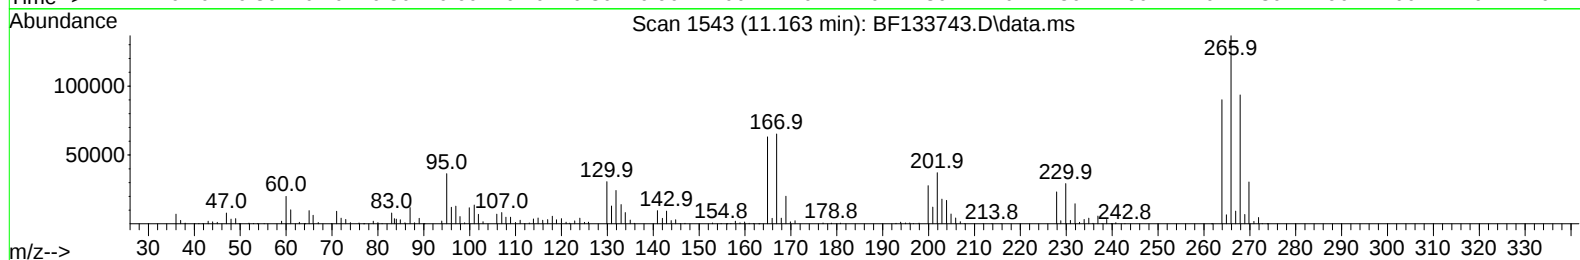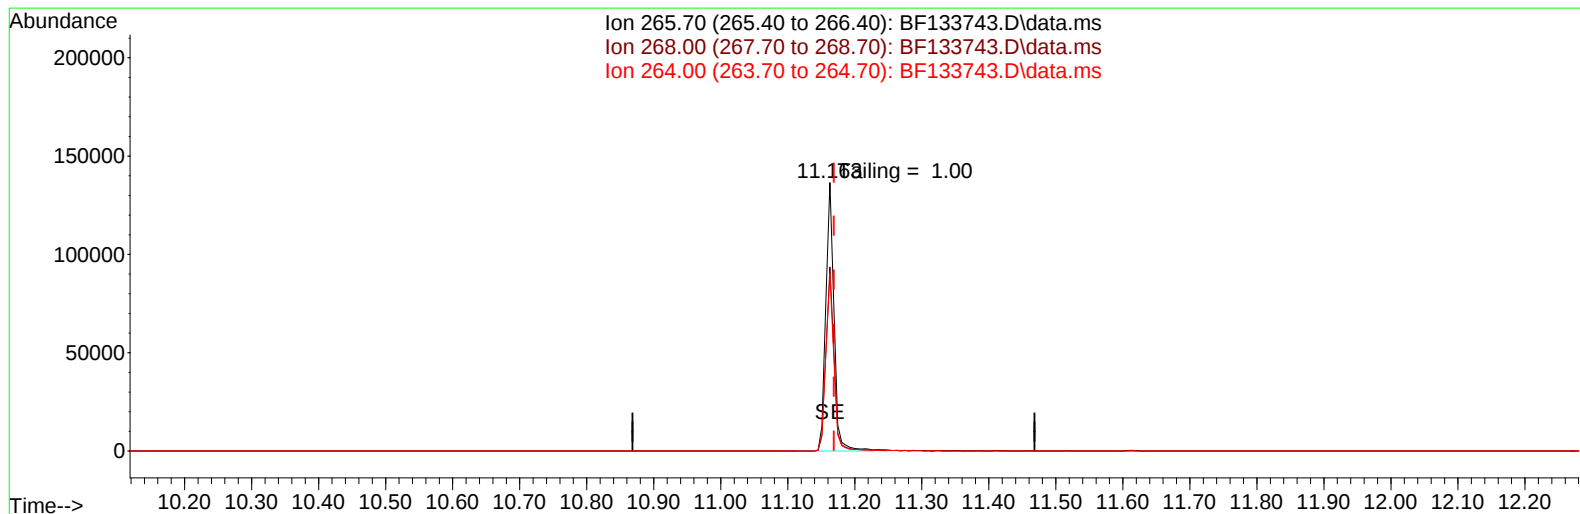

TIC: BF133743.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 26512.57 ng




response 117764

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	68.53
264.00	63.40	66.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061423\
Data File : BF133743.D
Acq On : 14 Jun 2023 09:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 14 10:23:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 13 11:26:55 2023
Response via : Initial Calibration

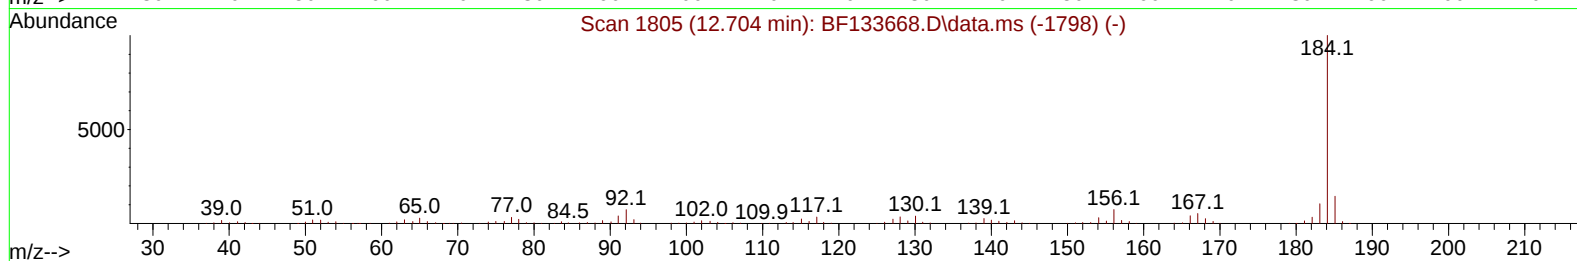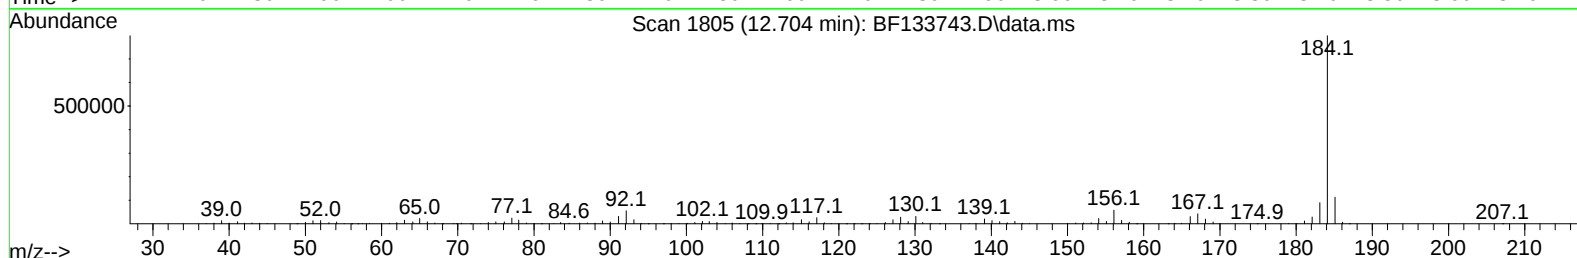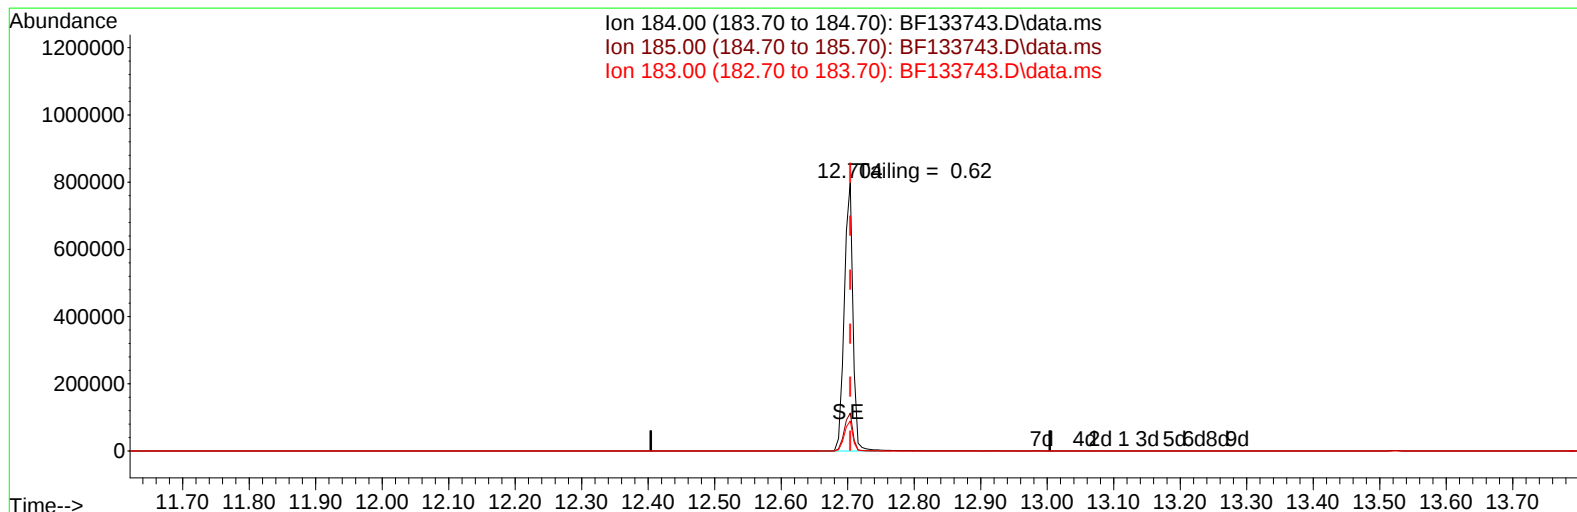

TIC: BF133743.D\data.ms

(77) Benzidine

12.704min (+ 0.000) 391202.01 ng m

response 721994

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.14
183.00	10.50	11.24
0.00	0.00	0.00