
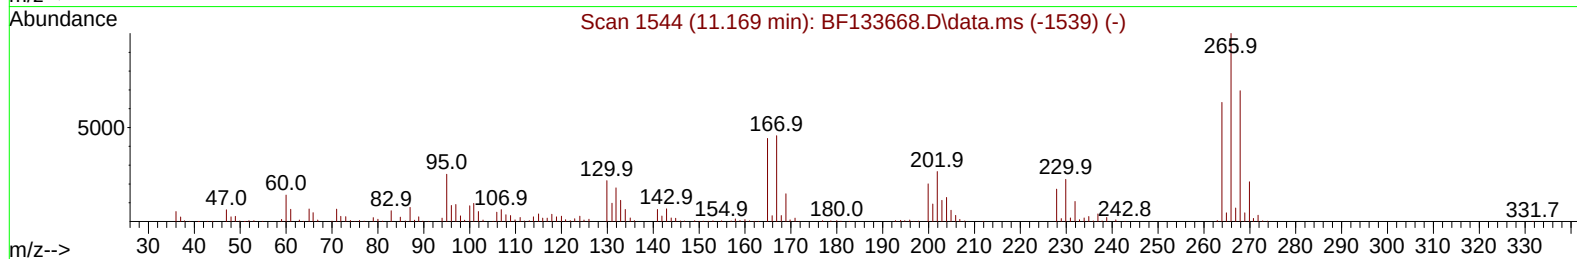
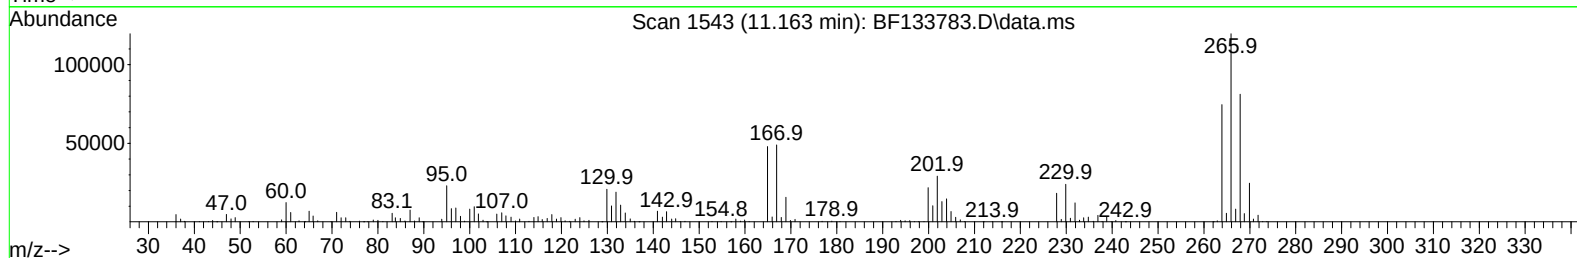


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133783.D
Acq On : 15 Jun 2023 19:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 04:29:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 15:12:57 2023
Response via : Initial Calibration

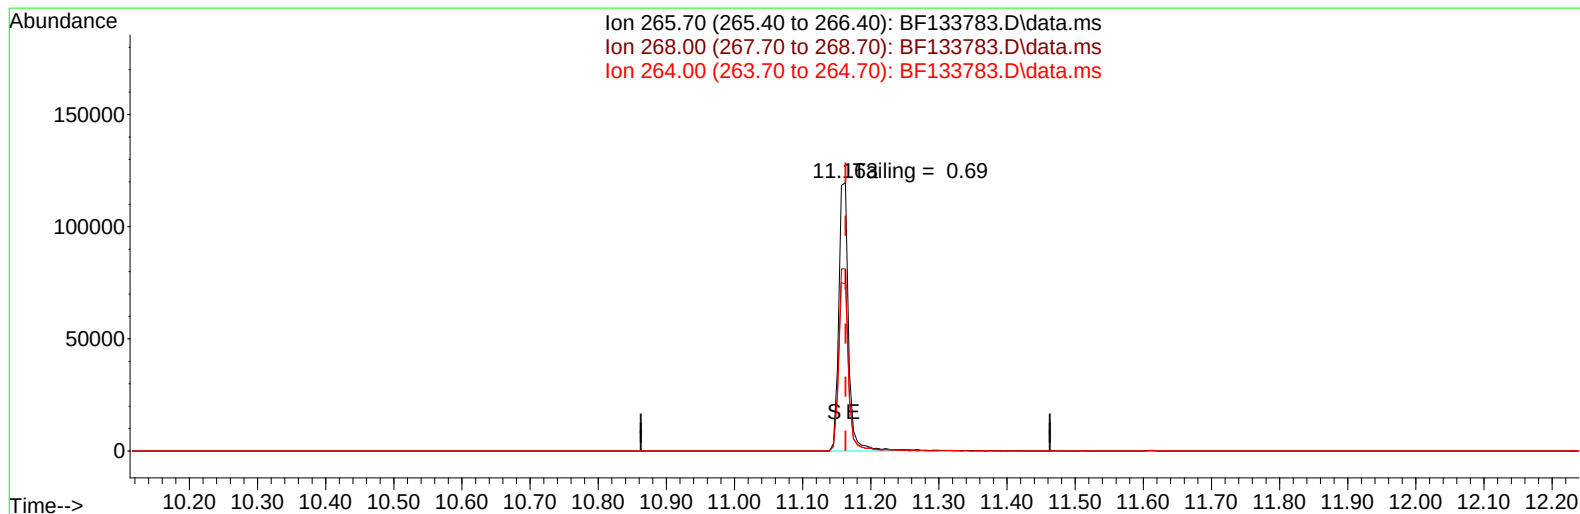

TIC: BF133783.D\data.ms

(70) Pentachlorophenol (C)




11.163min (-0.000) 40797.66 ng

response 119568

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	67.86
264.00	63.40	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133783.D
Acq On : 15 Jun 2023 19:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 04:29:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 15:12:57 2023
Response via : Initial Calibration

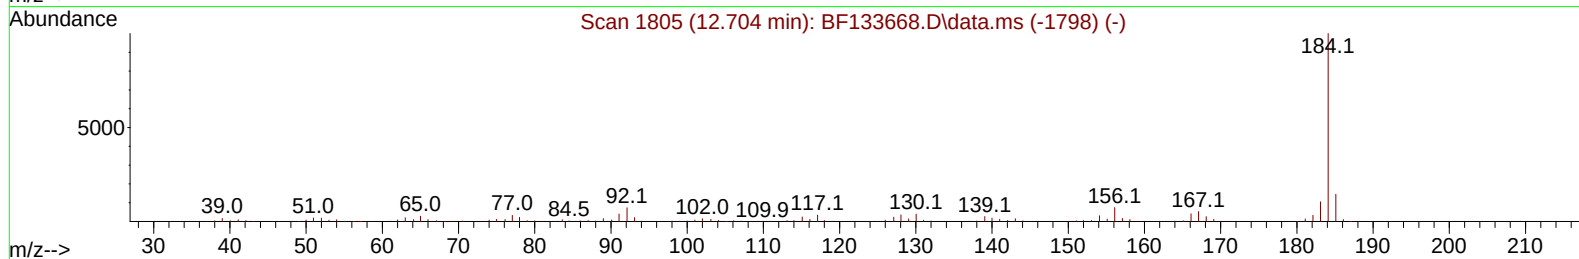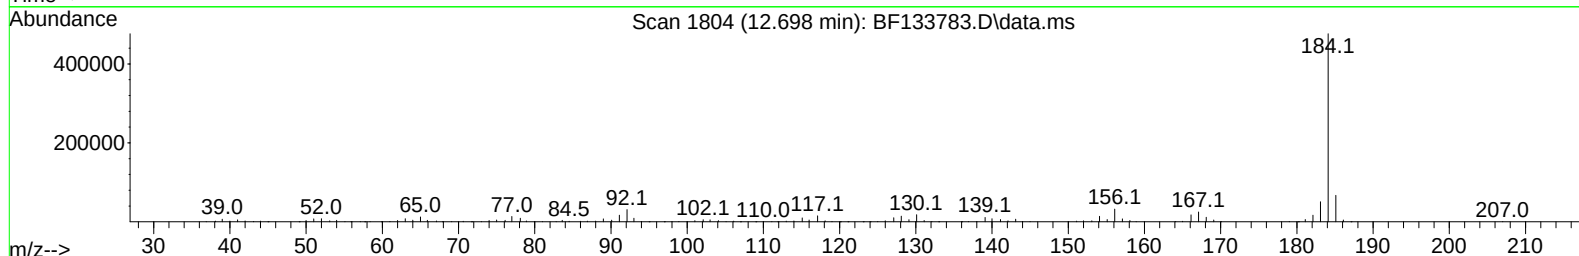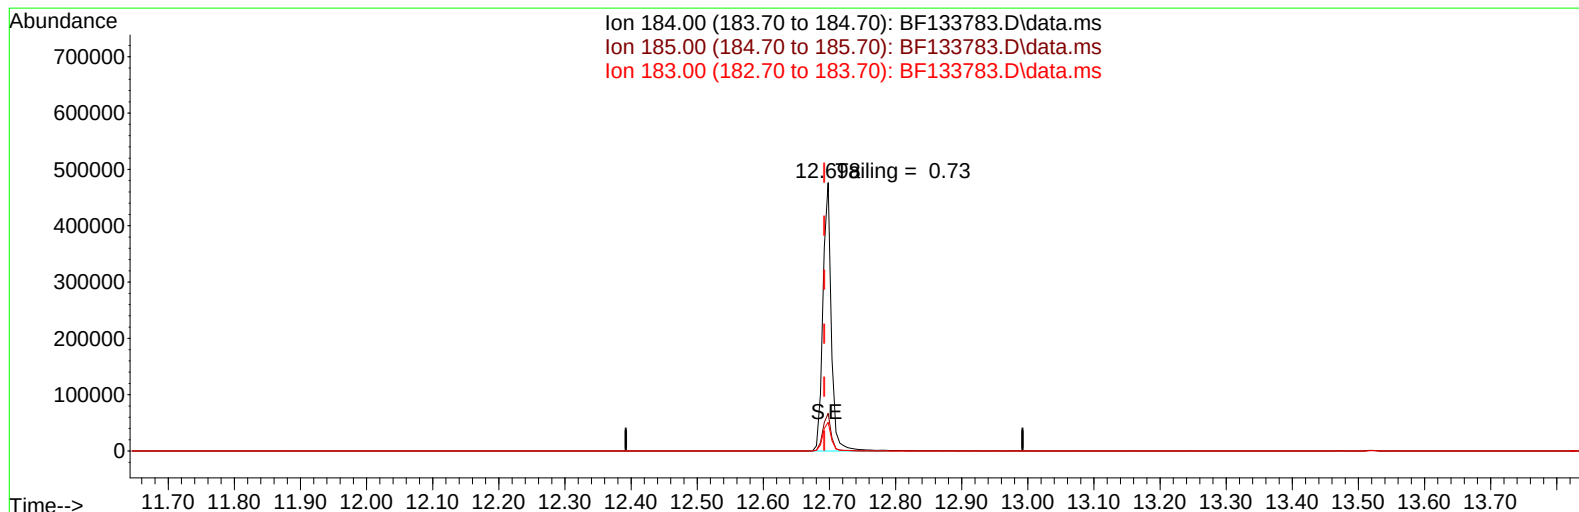

TIC: BF133783.D\data.ms

(77) Benzidine

12.698min (+ 0.006) 234600.84 ng

response 425102

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.04
183.00	10.50	10.69
0.00	0.00	0.00