

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
 Data File : BF133767.D
 Acq On : 15 Jun 2023 10:42
 Operator : CG\JU
 Sample : PB153397BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153397BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.134	3	8	13	rVB	87396	120341	2.39%	0.392%
2	4.392	388	392	401	rBV	80765	97859	1.94%	0.319%
3	4.839	464	468	477	rBV	81350	84410	1.68%	0.275%
4	5.063	498	506	515	rVB	39671	55743	1.11%	0.182%
5	5.451	566	572	575	rBV	3285492	3263695	64.82%	10.644%
6	6.463	738	744	747	rBV	2997012	3289035	65.32%	10.726%
7	6.828	802	806	810	rBV	1274878	1034745	20.55%	3.375%
8	6.981	829	832	836	rBV	938353	842913	16.74%	2.749%
9	7.398	897	903	906	rBV	2796665	2734150	54.30%	8.917%
10	8.110	1021	1024	1028	rBV	1524005	1349198	26.80%	4.400%
11	9.192	1203	1208	1211	rBV	5273872	4671936	92.79%	15.236%
12	9.869	1319	1323	1326	rBV	1936880	1549493	30.77%	5.053%
13	10.663	1453	1458	1461	rBV	2560826	2558484	50.81%	8.344%
14	11.357	1572	1576	1579	rBV	1986098	1648248	32.74%	5.375%
15	12.951	1842	1847	1850	rBV	5027984	5034999	100.00%	16.420%
16	13.998	2021	2025	2029	rBV	1312413	1281190	25.45%	4.178%
17	15.462	2268	2274	2283	rBV	821409	1046596	20.79%	3.413%




Sum of corrected areas: 30663035

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133767.D
Acq On : 15 Jun 2023 10:42
Operator : CG\JU
Sample : PB153397BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153397BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

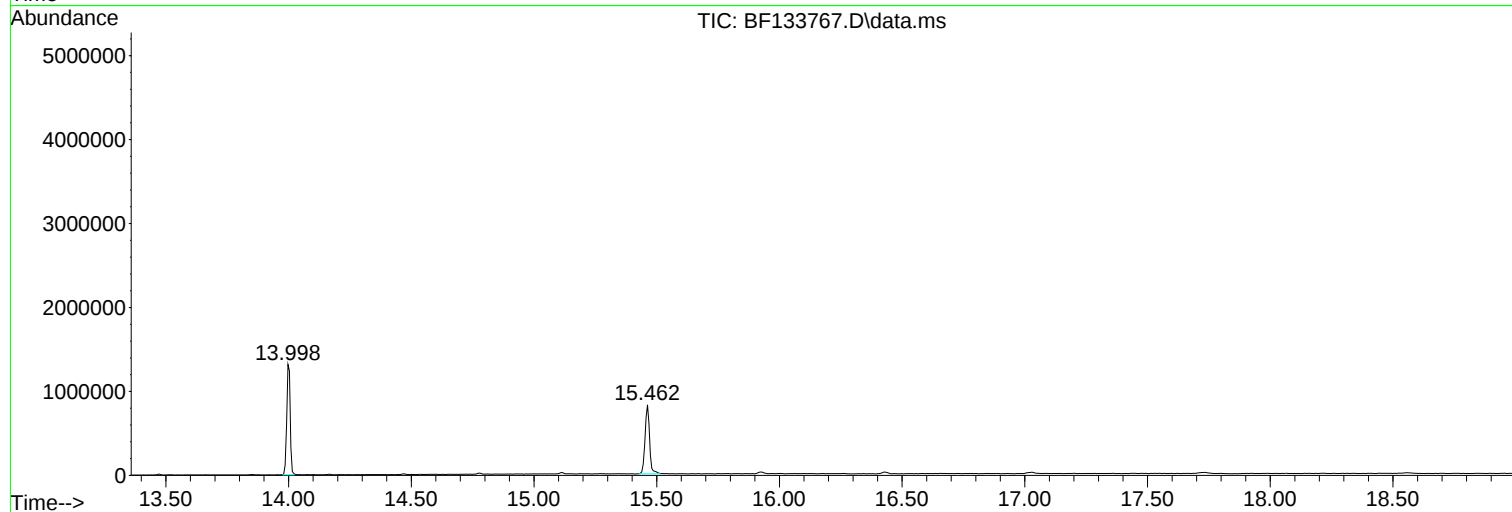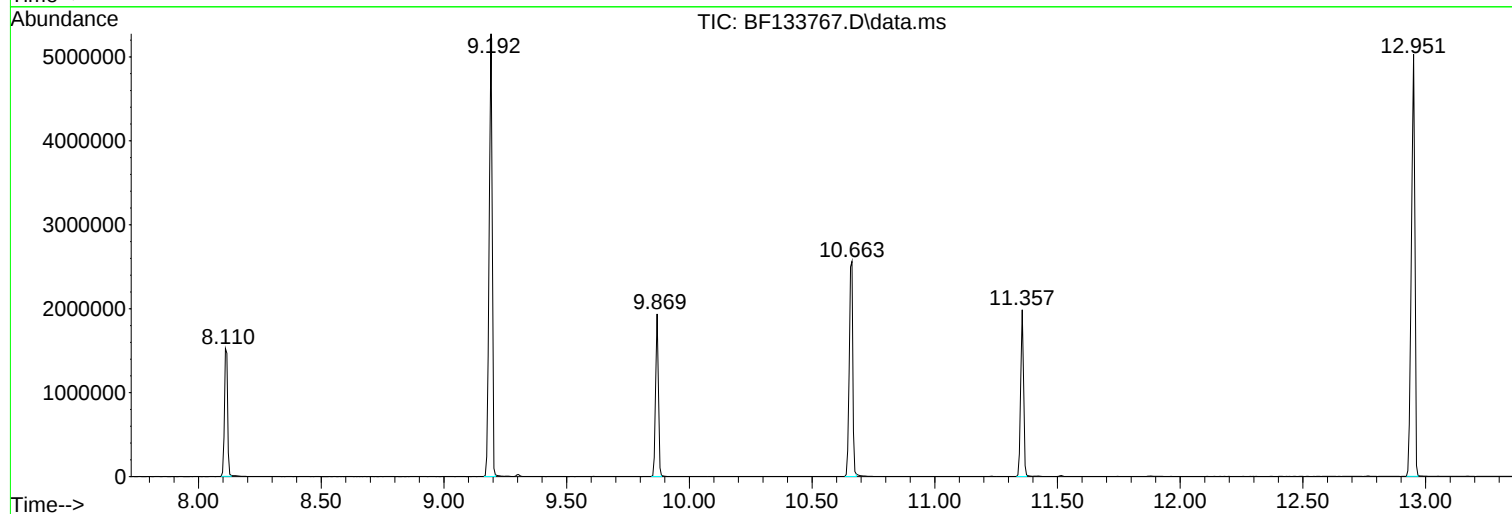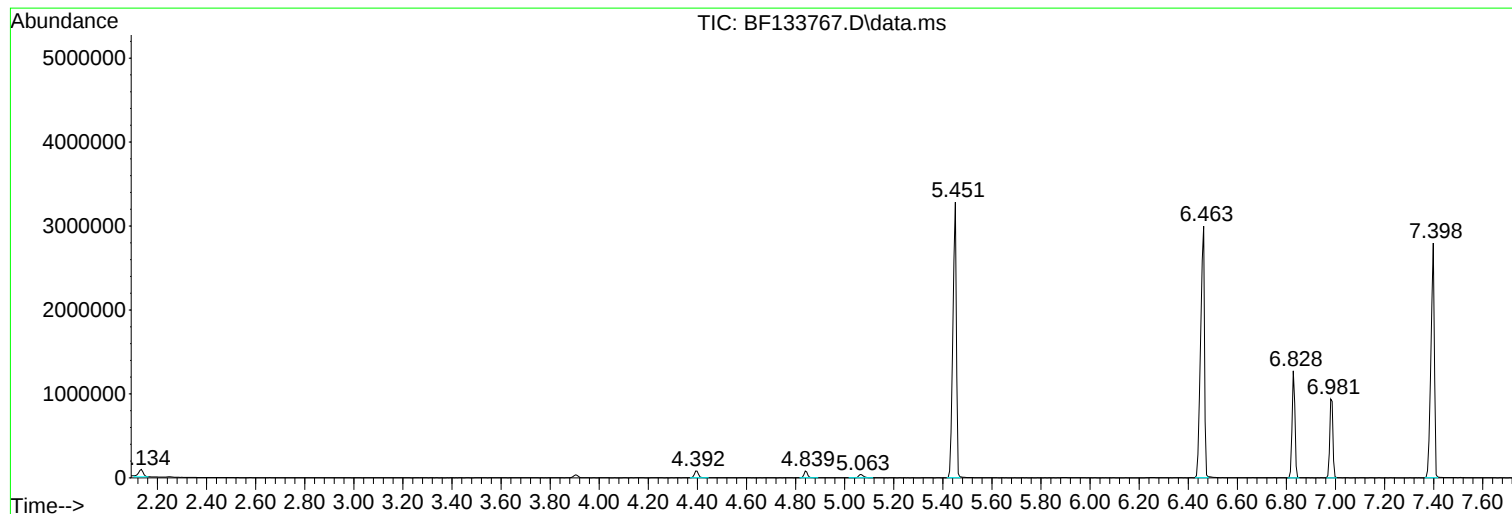

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133767.D
Acq On : 15 Jun 2023 10:42
Operator : CG\JU
Sample : PB153397BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153397BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.134	2.33 ng	120341	1,4-Dichlorobenzene-d4	6.828

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	38
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	35
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
5			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	23

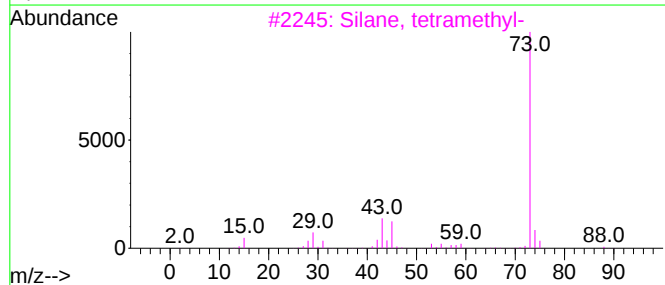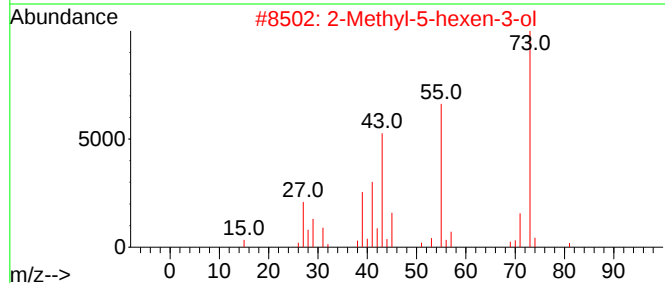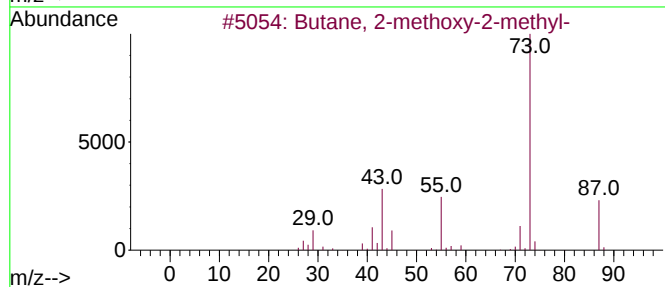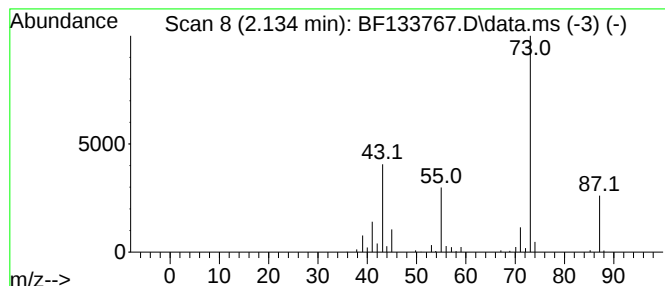

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133767.D
Acq On : 15 Jun 2023 10:42
Operator : CG\JU
Sample : PB153397BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153397BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.134	2.3	ng	120341	1	6.828	1034750	20.0