

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
 Data File : BF133785.D
 Acq On : 15 Jun 2023 20:48
 Operator : CG\JU
 Sample : PB153350BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153350BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.128	3	7	12	rVB	68738	88647	1.64%	0.337%
2	5.451	567	572	575	rBV	2805053	2780146	51.32%	10.575%
3	6.463	738	744	747	rBV	2691312	2795065	51.60%	10.632%
4	6.828	803	806	810	rBV	765224	598955	11.06%	2.278%
5	6.987	829	833	836	rBV	1073123	907368	16.75%	3.451%
6	7.398	897	903	906	rBV	2534336	2623455	48.43%	9.979%
7	8.110	1021	1024	1028	rBV	880082	758897	14.01%	2.887%
8	9.192	1203	1208	1211	rBV	5129313	4814474	88.88%	18.313%
9	9.869	1319	1323	1326	rBV	1126331	912857	16.85%	3.472%
10	10.663	1453	1458	1461	rBV	2416420	2404475	44.39%	9.146%
11	11.357	1572	1576	1579	rBV	1251325	1014726	18.73%	3.860%
12	12.951	1842	1847	1850	rBV	4982054	5417022	100.00%	20.605%
13	13.998	2021	2025	2032	rBV	638110	627748	11.59%	2.388%
14	15.463	2269	2274	2284	rVB	424896	545641	10.07%	2.076%




Sum of corrected areas: 26289476

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133785.D
Acq On : 15 Jun 2023 20:48
Operator : CG\JU
Sample : PB153350BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153350BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

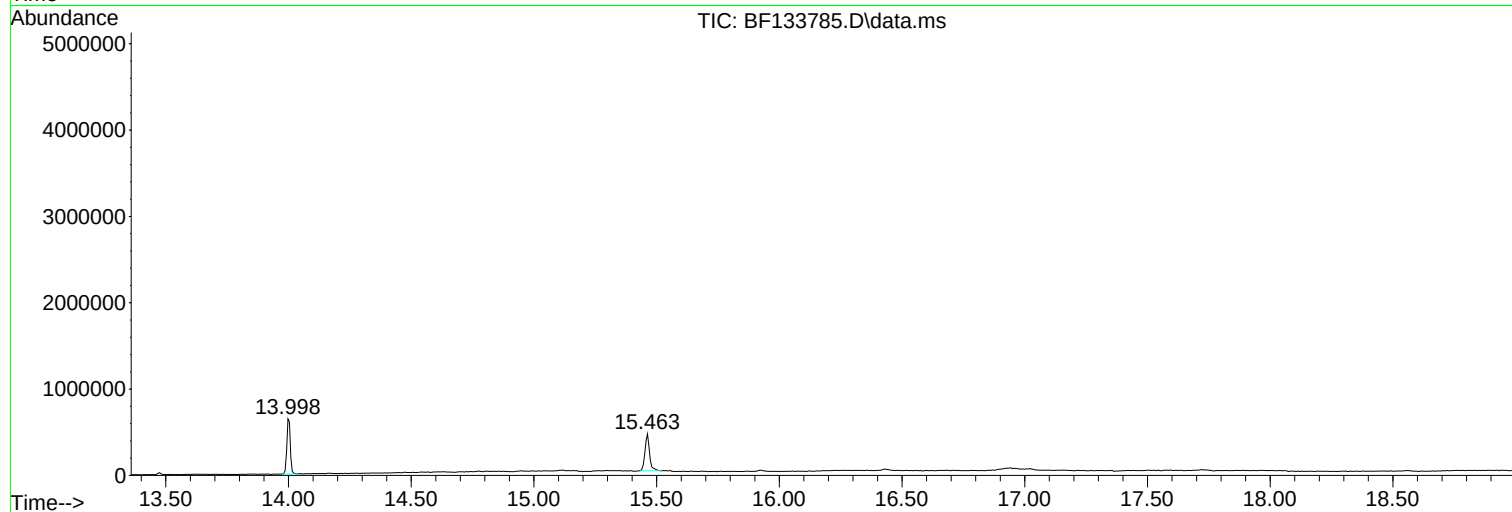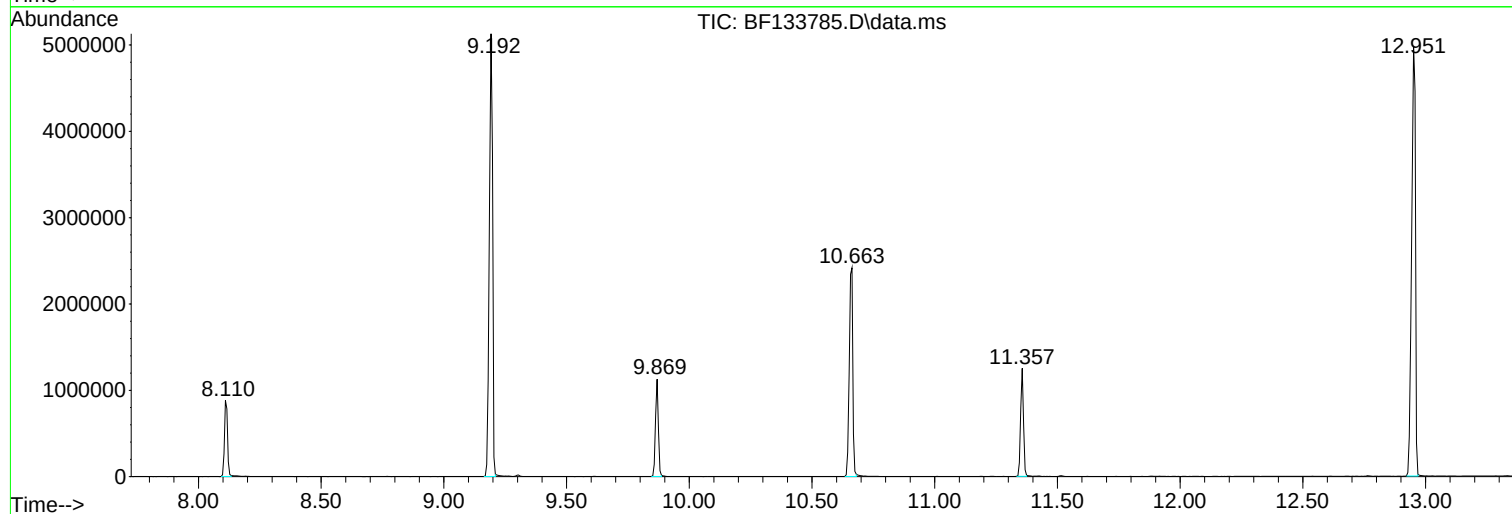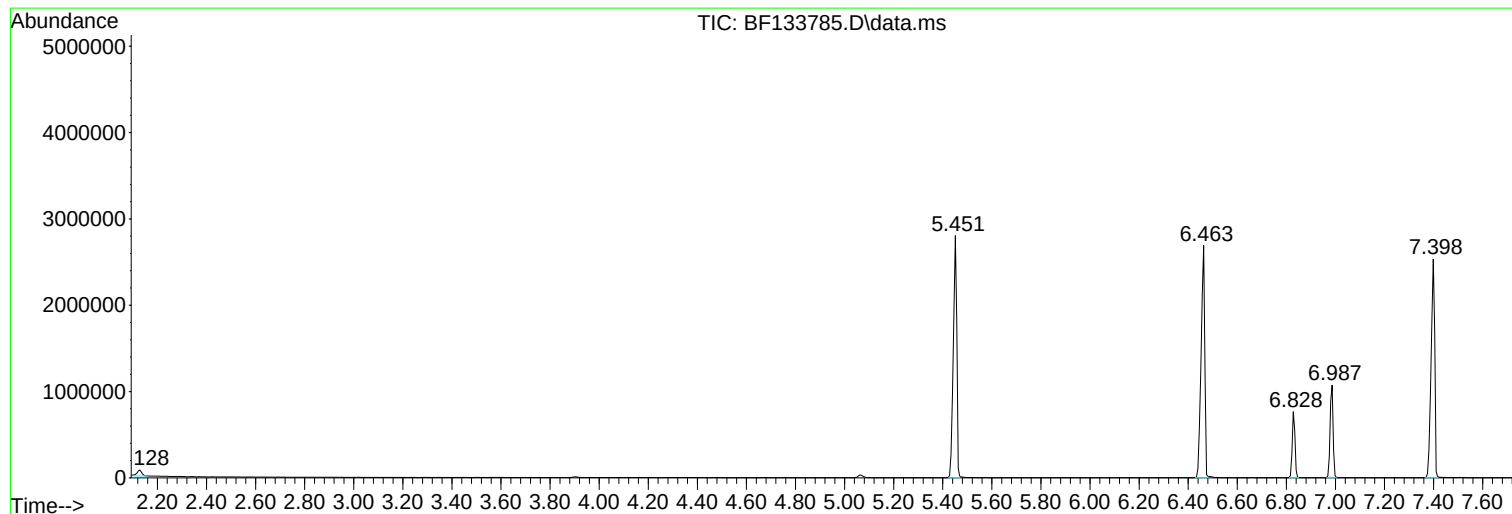

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133785.D
Acq On : 15 Jun 2023 20:48
Operator : CG\JU
Sample : PB153350BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153350BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.128	2.96 ng	88647	1,4-Dichlorobenzene-d4	6.828

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2		Silane, tetramethyl-	88	C4H12Si	000075-76-3	43
3		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	38
4		3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	38
5		Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	33

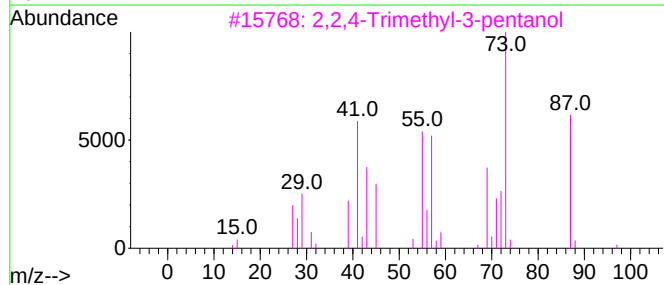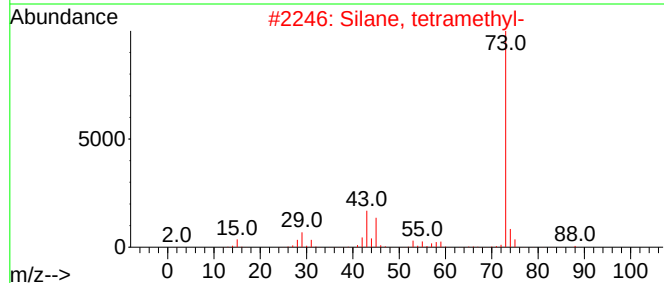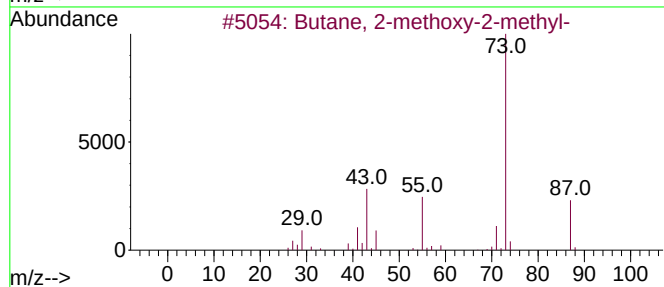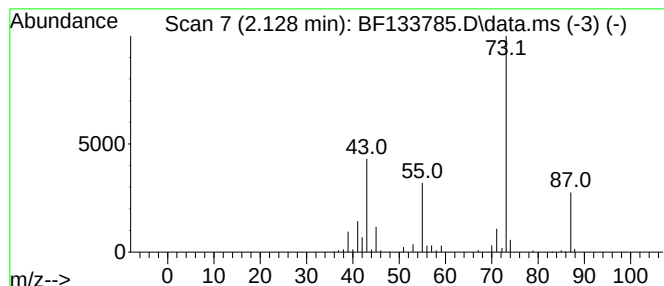

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133785.D
Acq On : 15 Jun 2023 20:48
Operator : CG\JU
Sample : PB153350BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153350BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.128	3.0	ng	88647	1	6.828	598955	20.0