


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133765.D
Acq On : 15 Jun 2023 08:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 15 15:12:57 2023

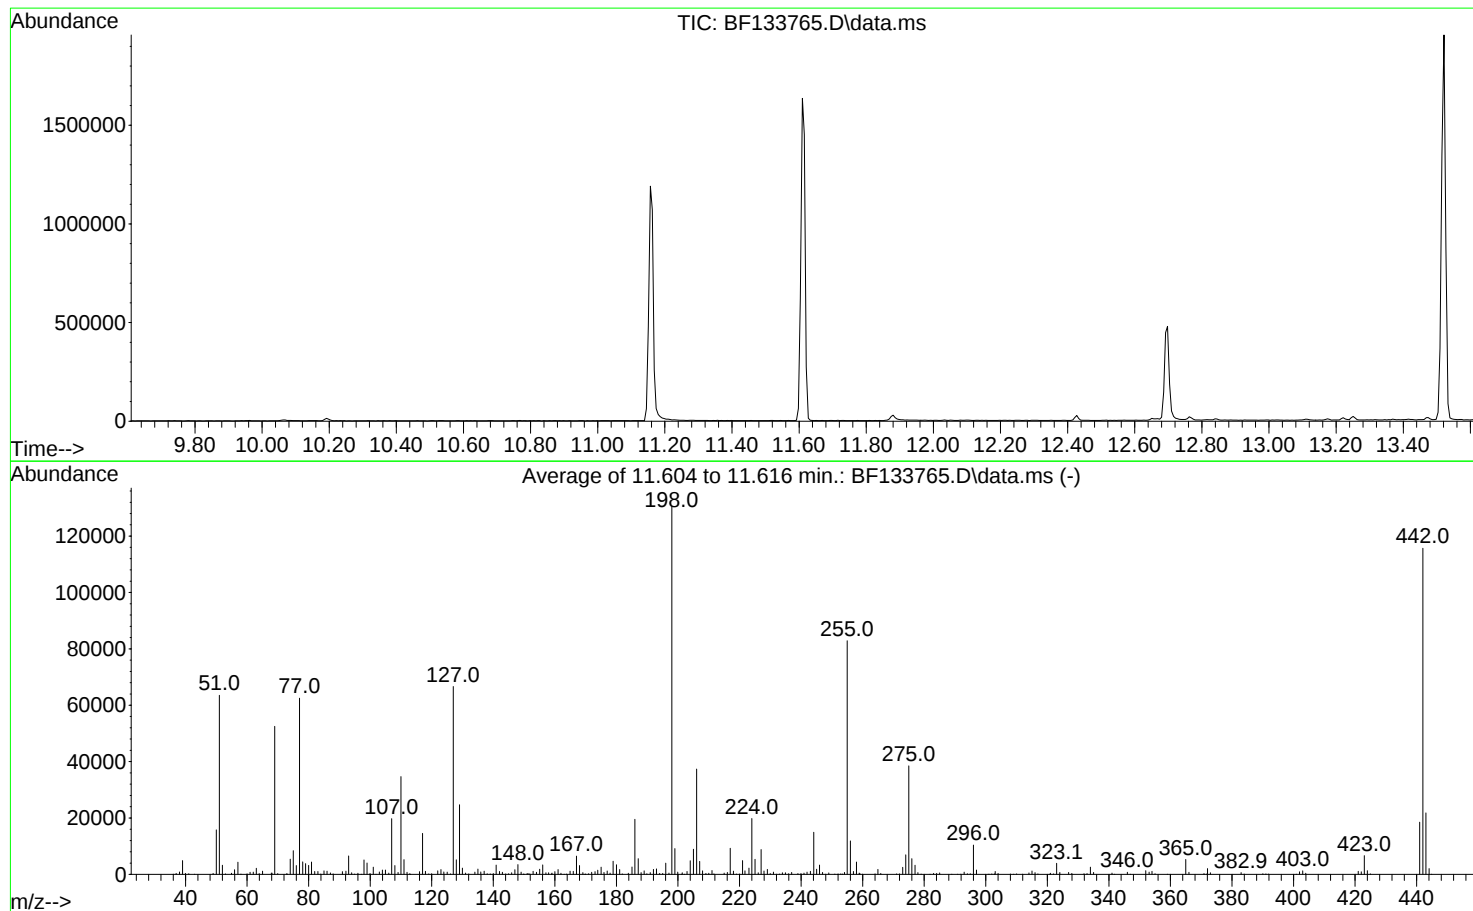

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.7	63528	PASS
68	69	0.00	2	0.9	482	PASS
69	198	0.00	100	40.2	52520	PASS
70	69	0.00	2	0.6	290	PASS
127	198	10	80	51.1	66659	PASS
197	198	0.00	2	0.4	486	PASS
198	198	100	100	100.0	130504	PASS
199	198	5	9	7.0	9146	PASS
275	198	10	60	29.5	38500	PASS
365	198	1	100	4.1	5301	PASS
441	198	0.01	100	14.2	18521	PASS
442	442	50	100	100.0	115693	PASS
443	442	15	24	18.9	21823	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/15/2023	BNA_F	<u>BF133765.D</u>
Compound Name	Response	Retention Time
DDT	317566	13.521
DDD	5661	13.251
DDE	175	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5836	323402	1.80

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133765.D
Acq On : 15 Jun 2023 08:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 15 09:04:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 16:27:59 2023
Response via : Initial Calibration

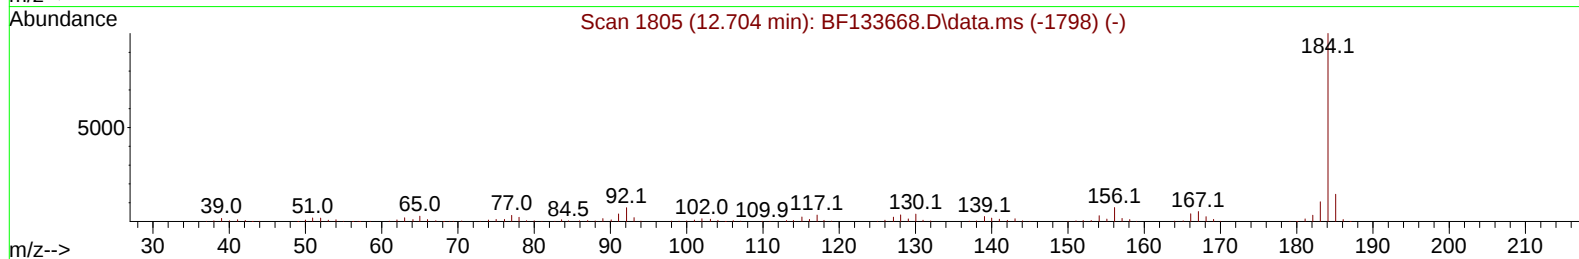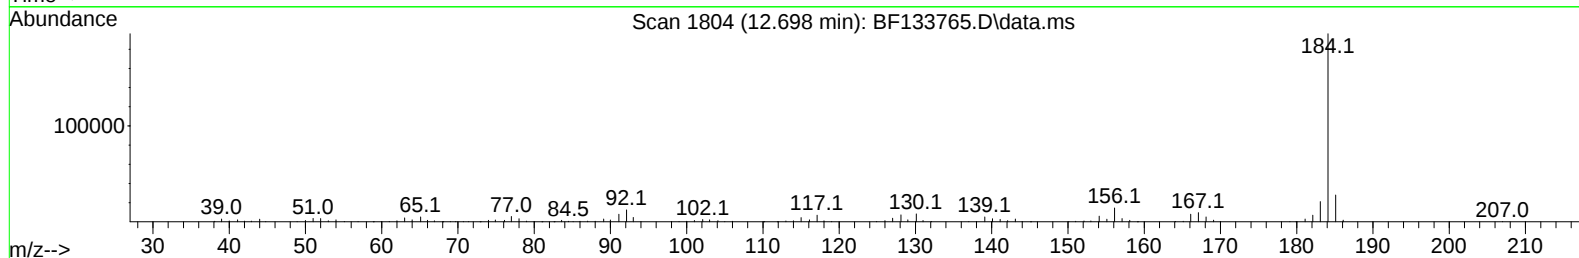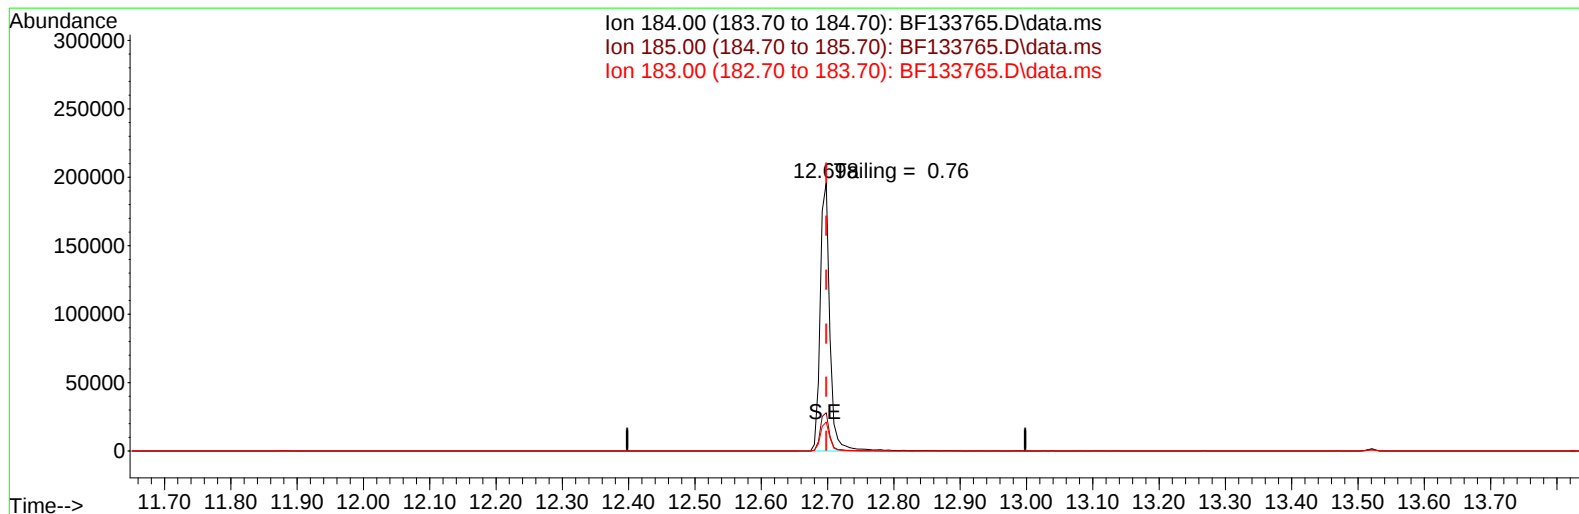

TIC: BF133765.D\data.ms

(77) Benzidine

12.698min (-0.000) 0.00 ng

response 198071

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.28
183.00	10.50	10.82
0.00	0.00	0.00