


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133783.D
Acq On : 15 Jun 2023 19:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 15 15:12:57 2023

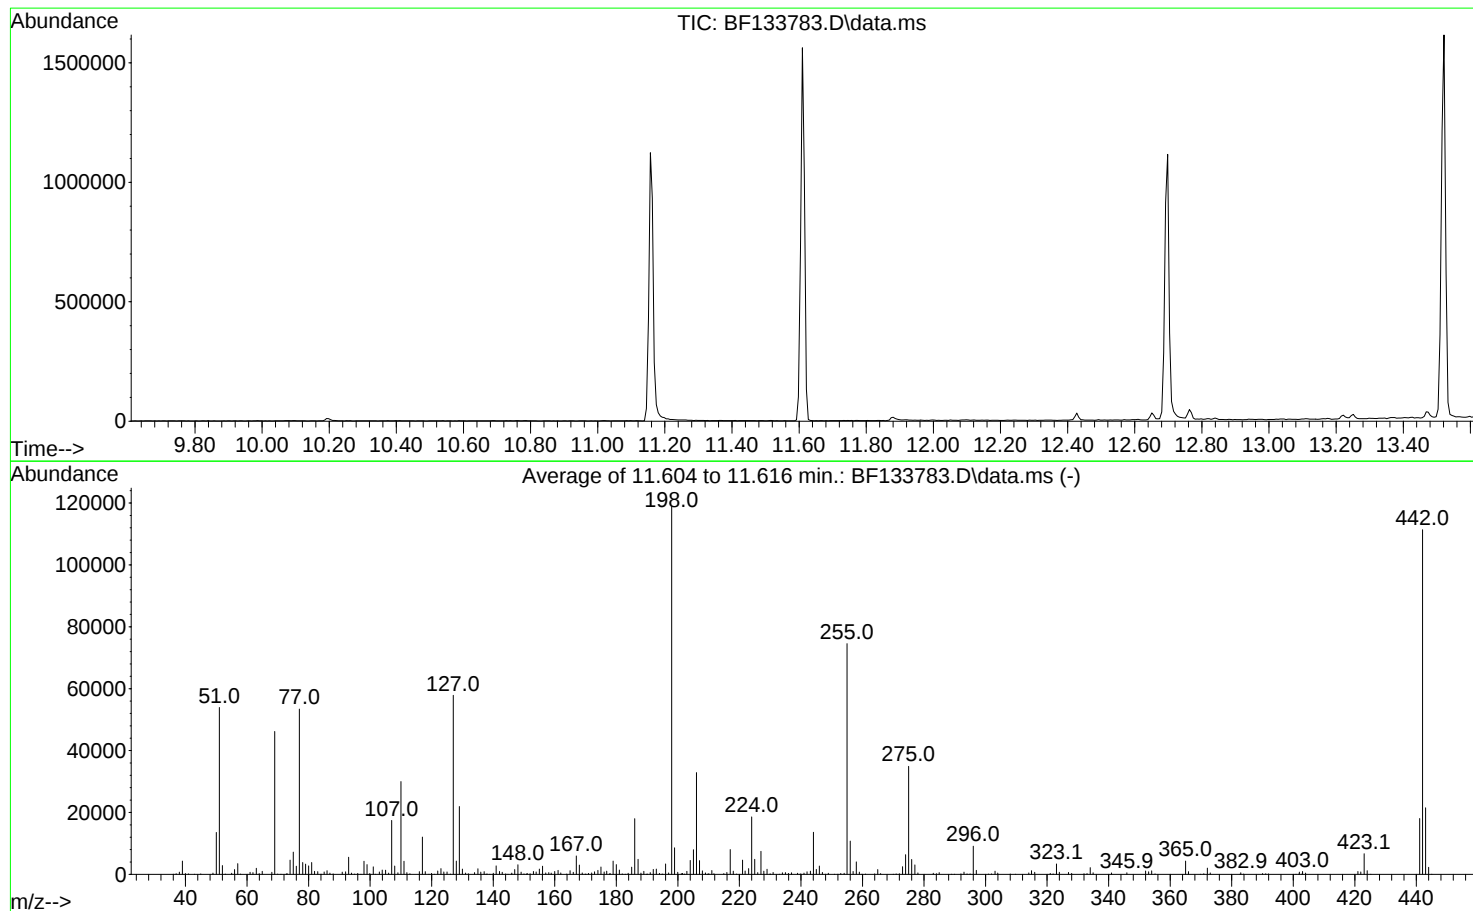

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	53928	PASS
68	69	0.00	2	1.5	673	PASS
69	198	0.00	100	38.9	46192	PASS
70	69	0.00	2	0.2	115	PASS
127	198	10	80	48.7	57853	PASS
197	198	0.00	2	0.4	480	PASS
198	198	100	100	100.0	118872	PASS
199	198	5	9	7.2	8599	PASS
275	198	10	60	29.4	34931	PASS
365	198	1	100	3.6	4309	PASS
441	198	0.01	100	15.2	18056	PASS
442	442	50	100	100.0	111387	PASS
443	442	15	24	19.3	21488	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/15/2023	BNA_F	<u>BF133783.D</u>
Compound Name	Response	Retention Time
DDT	266992	13.521
DDD	6296	13.251
DDE	120	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6416	273408	2.35

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133783.D
Acq On : 15 Jun 2023 19:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 16 04:29:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 15:12:57 2023
Response via : Initial Calibration

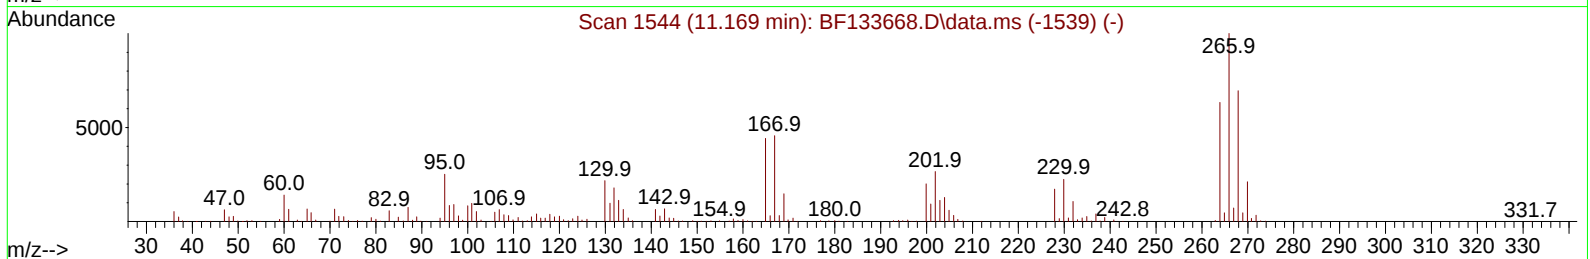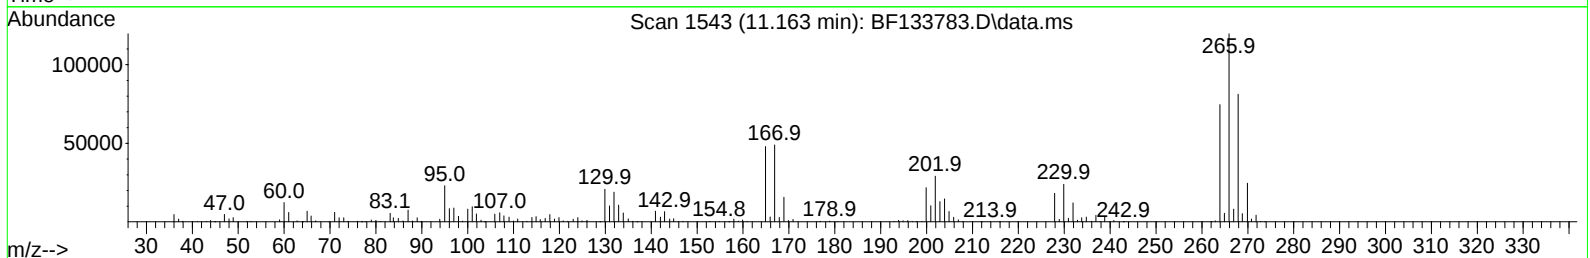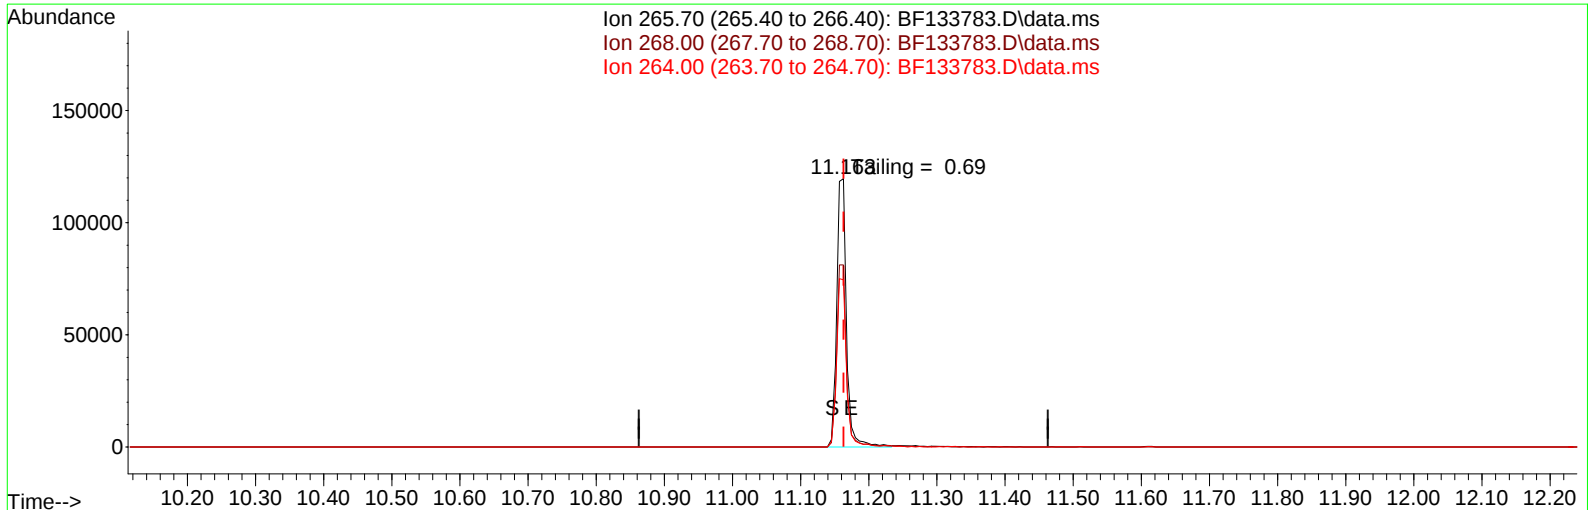

TIC: BF133783.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.000) 40797.66 ng




response 119568

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	67.86
264.00	63.40	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061523\
Data File : BF133783.D
Acq On : 15 Jun 2023 19:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 16 04:29:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 15:12:57 2023
Response via : Initial Calibration

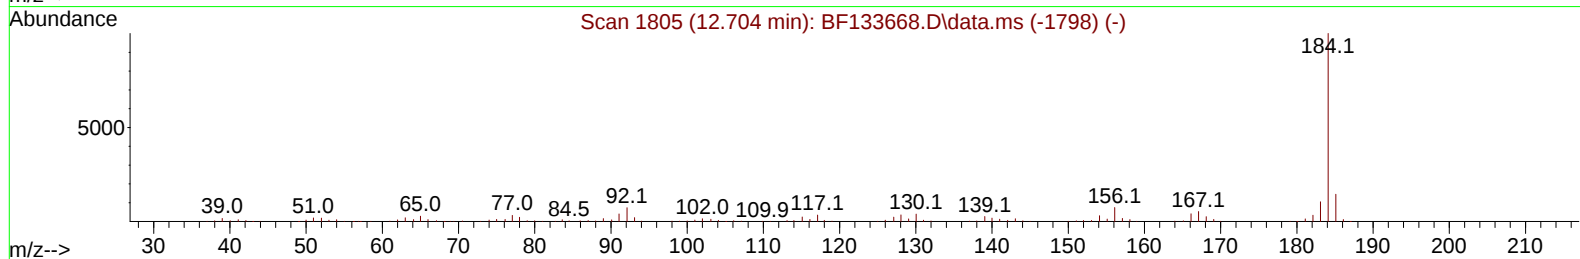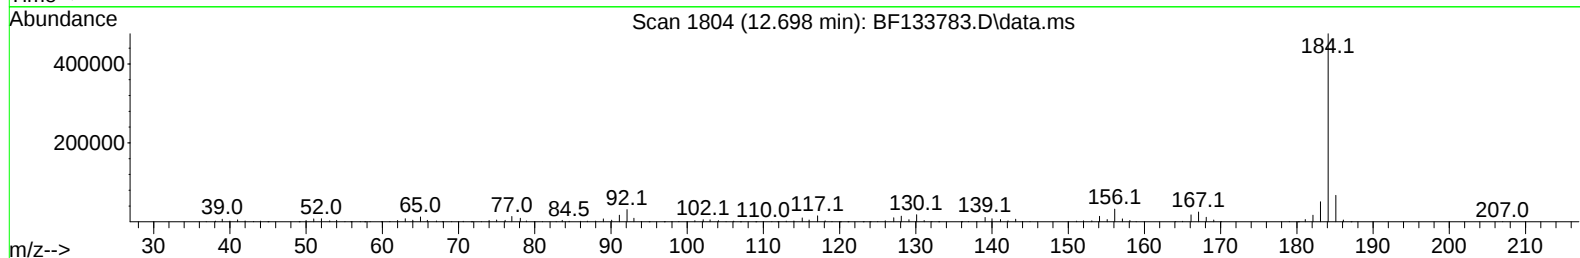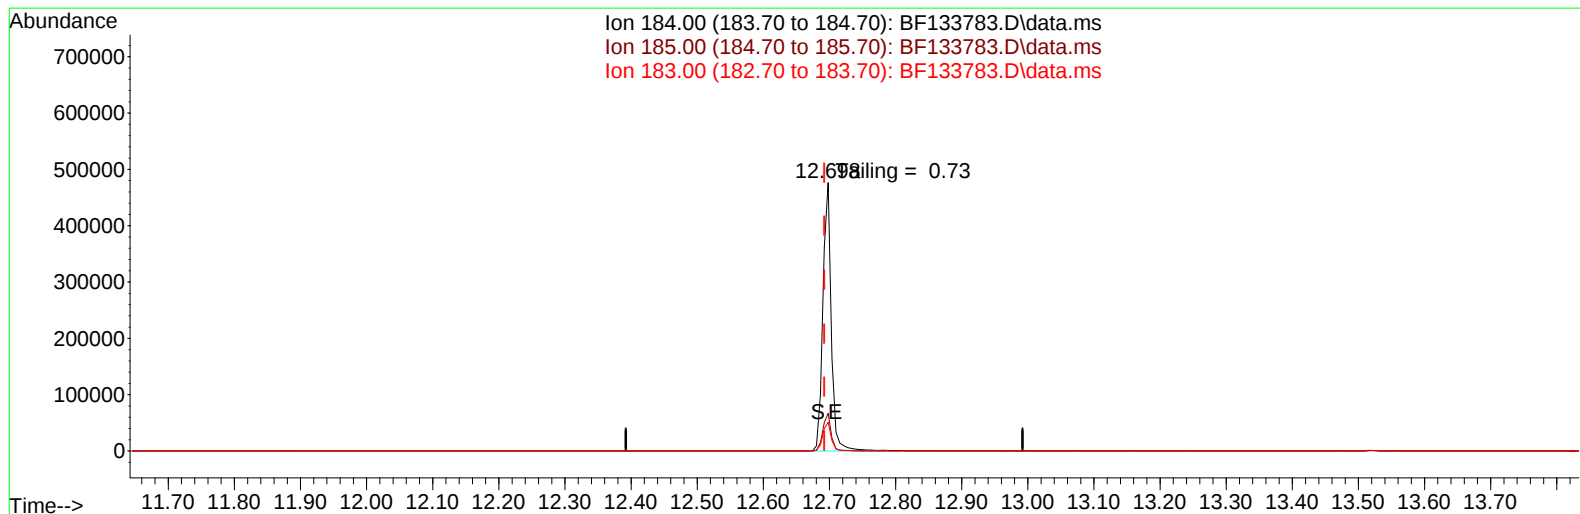

TIC: BF133783.D\data.ms

(77) Benzidine

12.698min (+ 0.006) 234600.84 ng

response 425102

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.04
183.00	10.50	10.69
0.00	0.00	0.00