
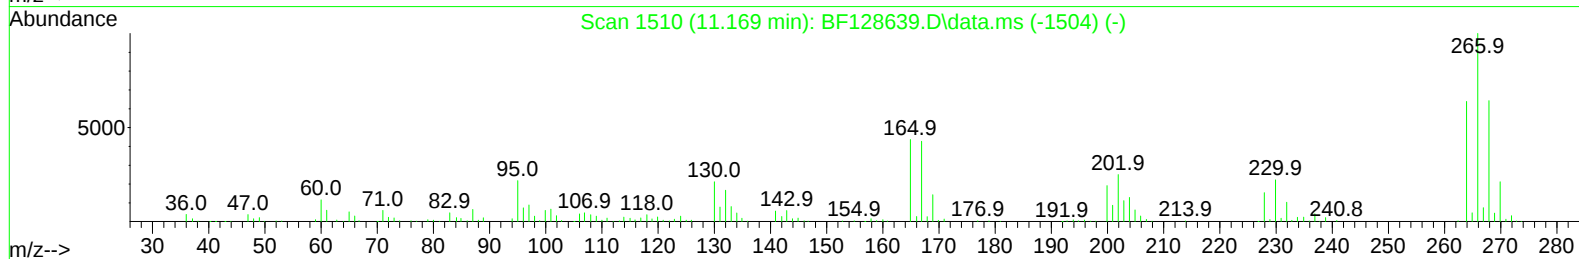
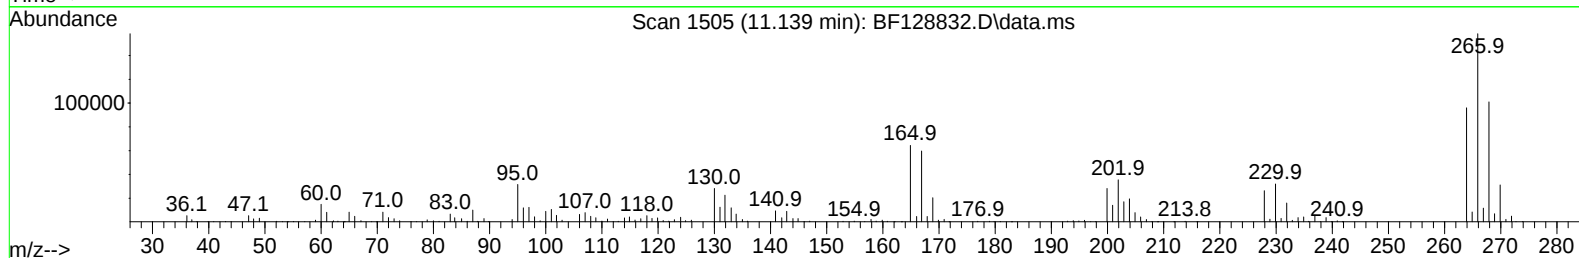


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\
Data File : BF128832.D
Acq On : 16 Jun 2022 11:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 02:28:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 14 14:53:53 2022
Response via : Initial Calibration

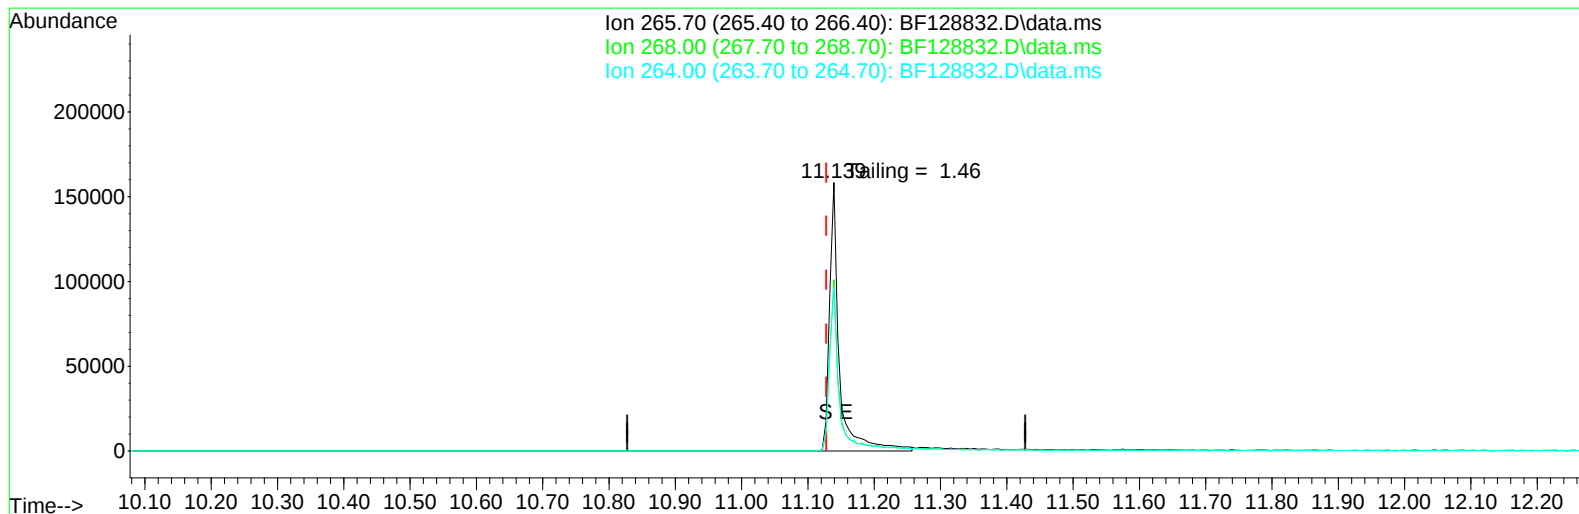

TIC: BF128832.D\data.ms

(70) Pentachlorophenol (C)




11.139min (+ 0.012) 26300.22 ng

response 164220

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.77
264.00	61.80	60.60
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\  
Data File : BF128832.D  
Acq On    : 16 Jun 2022  11:22  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jun 17 02:28:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 14 14:53:53 2022
Response via : Initial Calibration

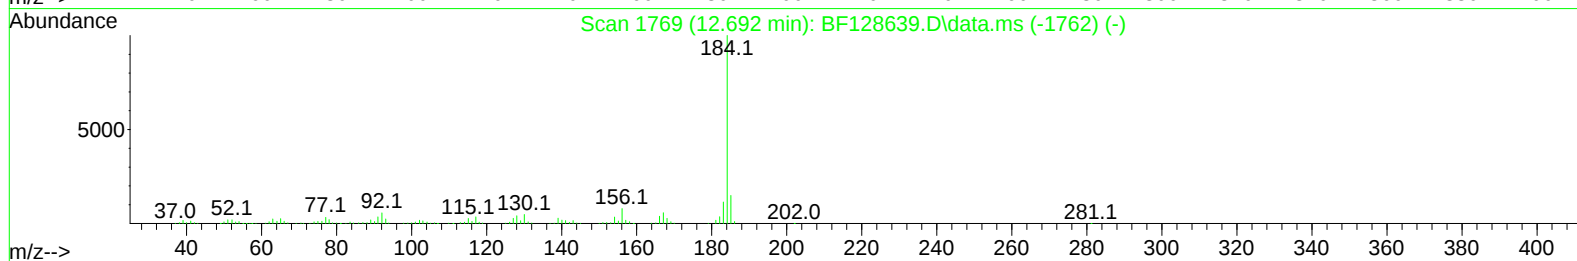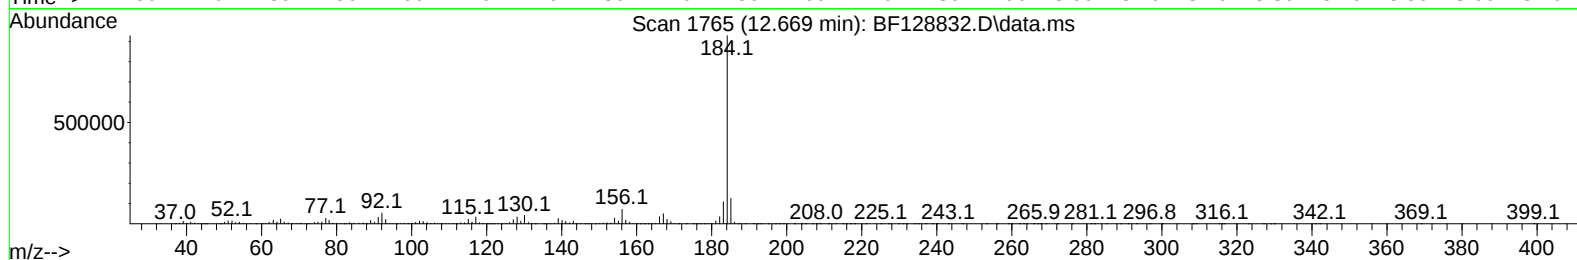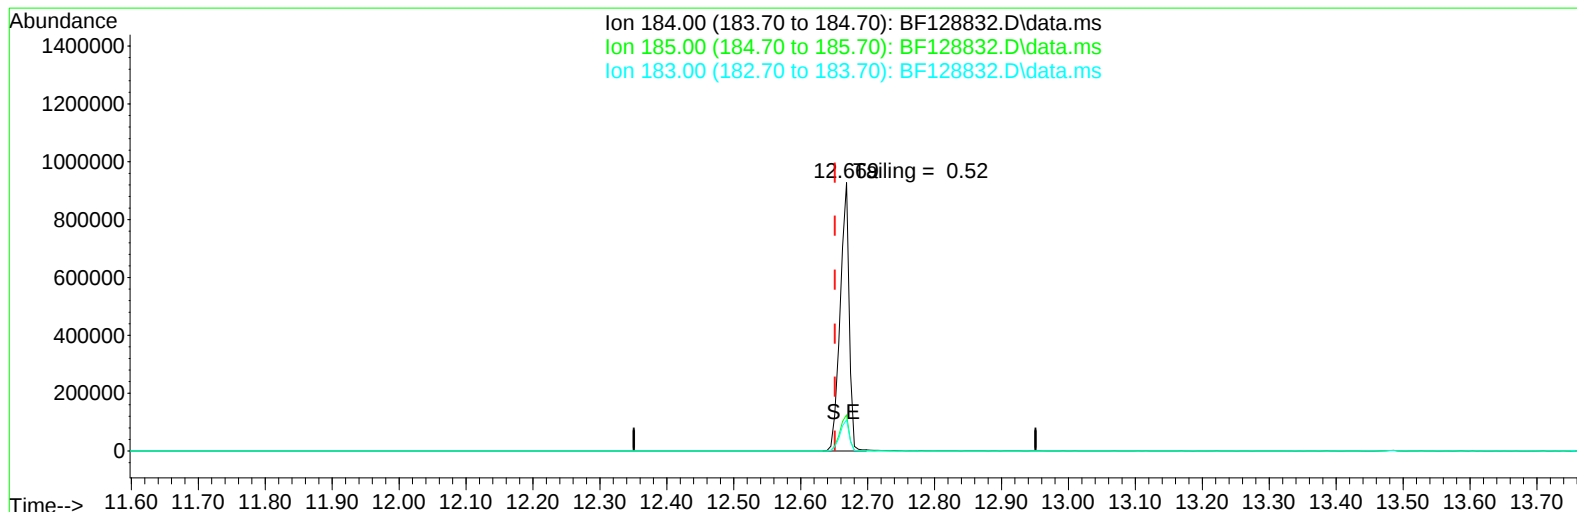

TIC: BF128832.D\data.ms

(77) Benzidine

12.669min (+ 0.018) 349560.40 ng

response **857101**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.90	13.49
--------	-------	-------

183.00	11.60	11.64
--------	-------	-------

0.00 0.00 0.00