

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\
 Data File : BF128834.D
 Acq On : 16 Jun 2022 12:25
 Operator : CG\JU
 Sample : PB145561BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145561BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128834.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	532	535	548	rBV	3607327	3449714	78.36%	15.500%
2	6.445	703	707	710	rBV	3014834	3131274	71.13%	14.070%
3	6.786	761	765	768	rBV	380781	318252	7.23%	1.430%
4	7.357	855	862	864	rBV	1788279	2040539	46.35%	9.169%
5	8.069	978	983	986	rBV	475644	424421	9.64%	1.907%
6	9.151	1160	1167	1170	rBV	3978842	4008977	91.07%	18.013%
7	9.827	1276	1282	1285	rBV	603877	513324	11.66%	2.306%
8	10.627	1411	1418	1421	rBV	2587267	2393492	54.37%	10.755%
9	11.316	1530	1535	1539	rBV	646504	551899	12.54%	2.480%
10	12.915	1801	1807	1810	rBV	4621230	4402168	100.00%	19.780%
11	13.968	1982	1986	1989	rBV	508551	489723	11.12%	2.200%
12	14.057	1998	2001	2006	rVB	118473	109461	2.49%	0.492%
13	15.427	2230	2234	2238	rVB	364211	422358	9.59%	1.898%




Sum of corrected areas: 22255602

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\
Data File : BF128834.D
Acq On : 16 Jun 2022 12:25
Operator : CG\JU
Sample : PB145561BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145561BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

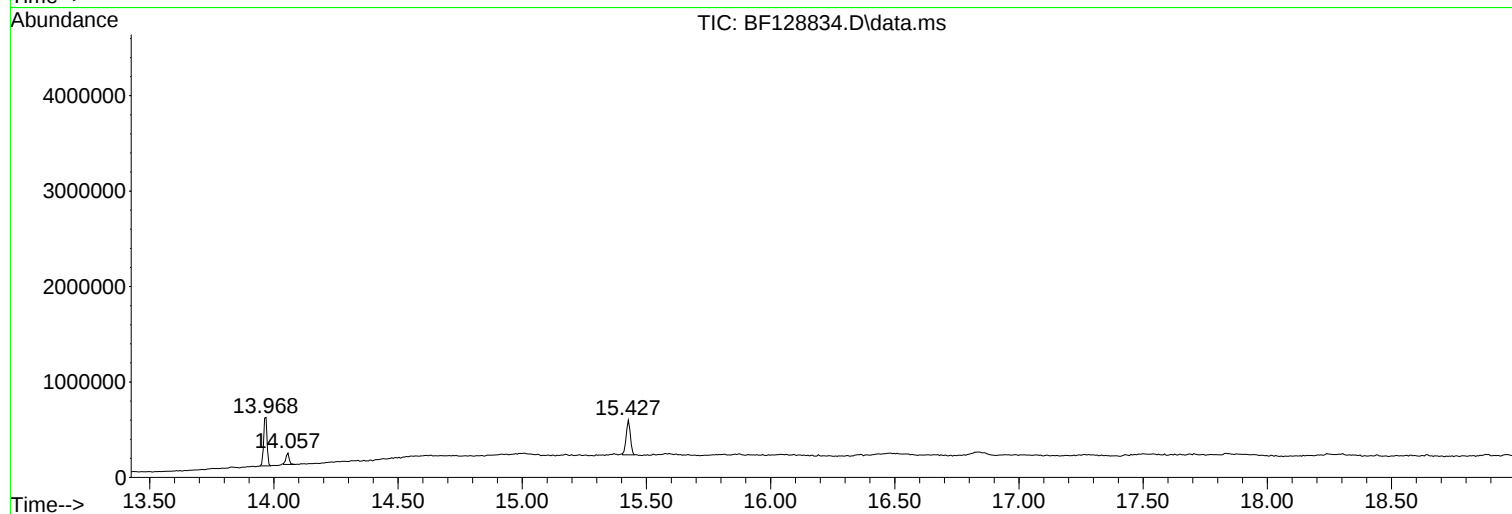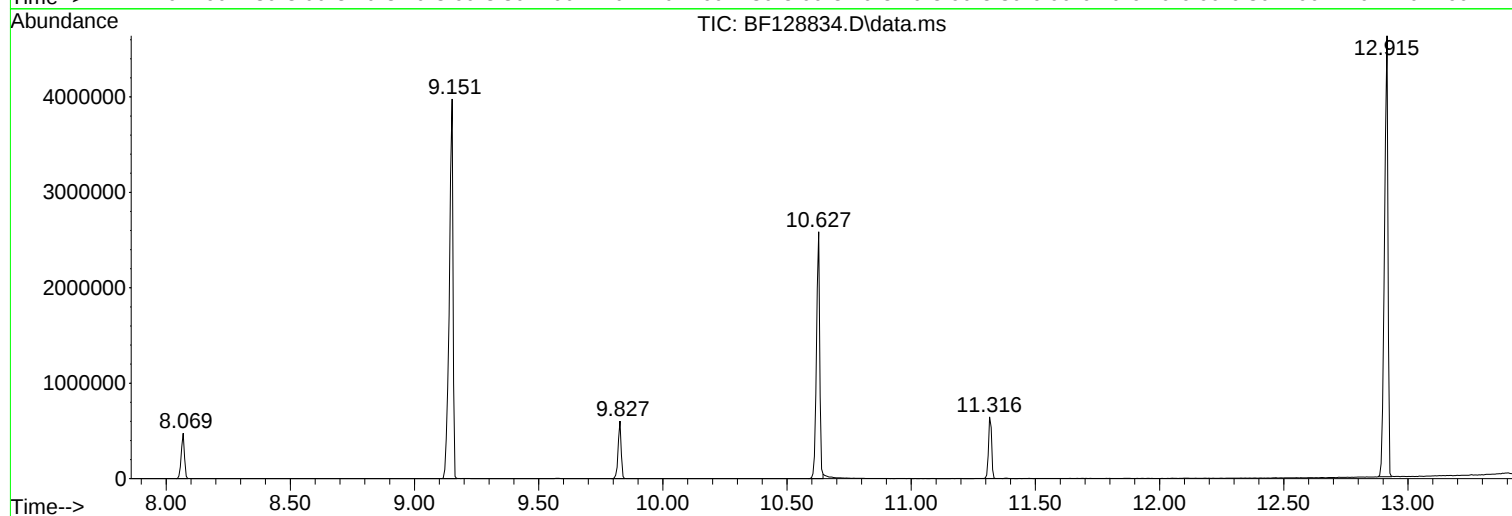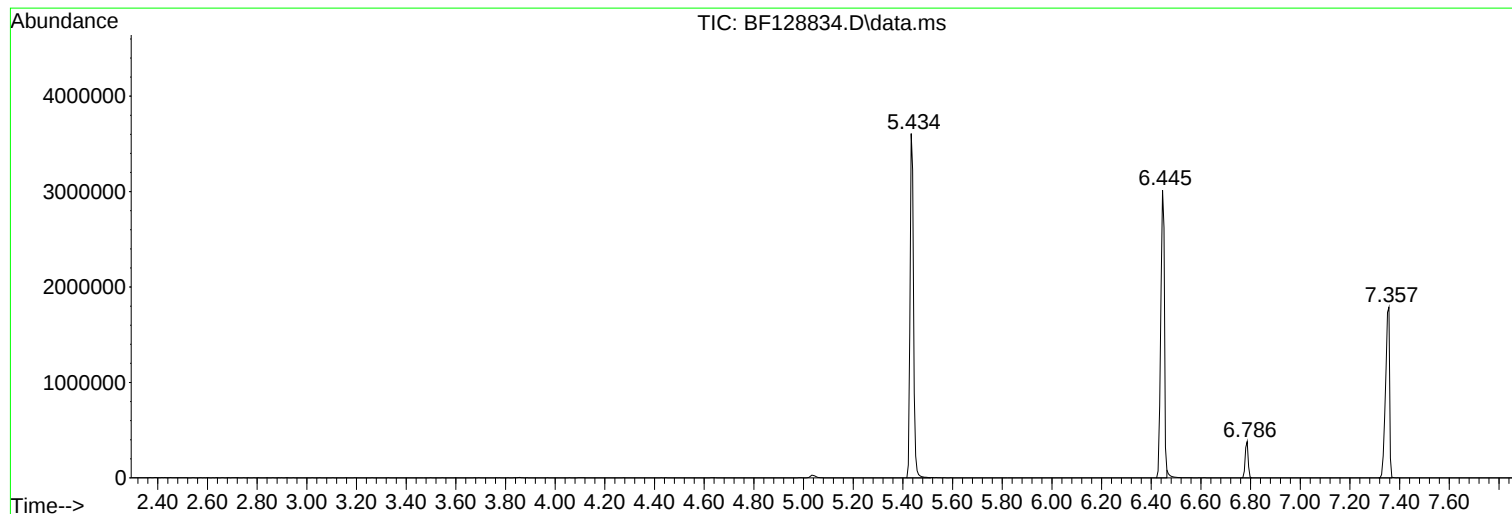

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\
Data File : BF128834.D
Acq On : 16 Jun 2022 12:25
Operator : CG\JU
Sample : PB145561BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145561BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.057	4.47 ng	109461	Chrysene-d12	13.968

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	98
2			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	64
3			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19N03S	1000483-83-4	49
4			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	32
5			4,5-Benzo-2-oxa-1,1,3,3-tetra(is...	320	C18H32OSi2	1000434-30-8	28

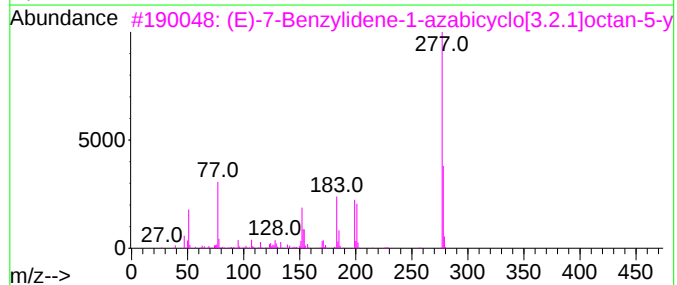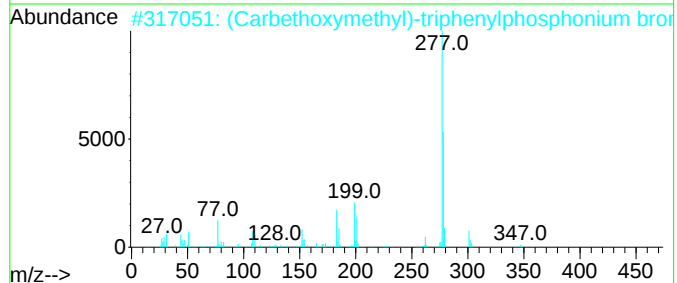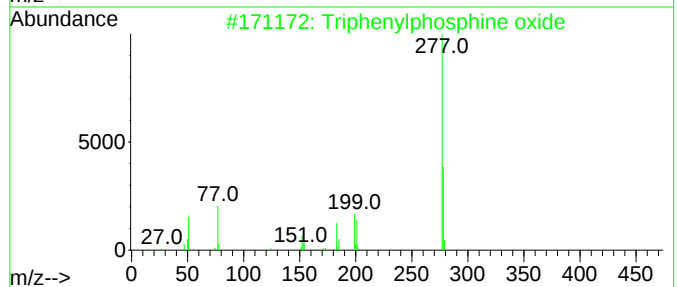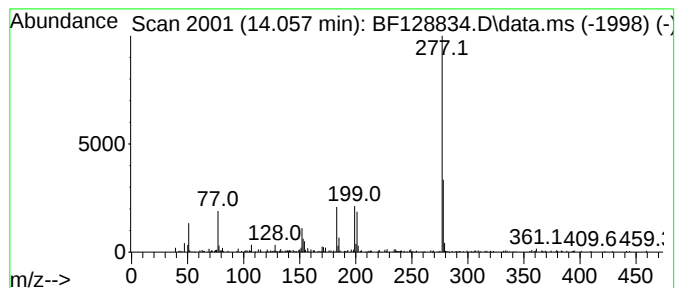

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\
Data File : BF128834.D
Acq On : 16 Jun 2022 12:25
Operator : CG\JU
Sample : PB145561BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145561BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.057	4.5	ng	109461	5	13.968	489723	20.0