

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\
 Data File : BF128836.D
 Acq On : 16 Jun 2022 13:23
 Operator : CG\JU
 Sample : PB145586BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145586BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128836.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	532	535	549	rBV	3332177	3201446	70.82%	14.081%
2	6.445	702	707	710	rBV	3241065	3148502	69.65%	13.848%
3	6.781	761	764	768	rVB	425523	345212	7.64%	1.518%
4	7.351	855	861	864	rBV	1919568	2256564	49.92%	9.925%
5	8.069	978	983	986	rBV	519445	466756	10.33%	2.053%
6	9.151	1159	1167	1170	rBV	4024409	4239328	93.78%	18.646%
7	9.822	1275	1281	1285	rBV	597924	536876	11.88%	2.361%
8	10.622	1410	1417	1420	rBV	2518468	2414998	53.42%	10.622%
9	11.316	1531	1535	1538	rVB	653414	558352	12.35%	2.456%
10	12.910	1798	1806	1809	rBV	4733512	4520413	100.00%	19.882%
11	13.963	1981	1985	1988	rBV	563457	492317	10.89%	2.165%
12	14.051	1994	2000	2006	rBV	125161	161062	3.56%	0.708%
13	15.421	2229	2233	2238	rVB	337778	394212	8.72%	1.734%




Sum of corrected areas: 22736038

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\
Data File : BF128836.D
Acq On : 16 Jun 2022 13:23
Operator : CG\JU
Sample : PB145586BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145586BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

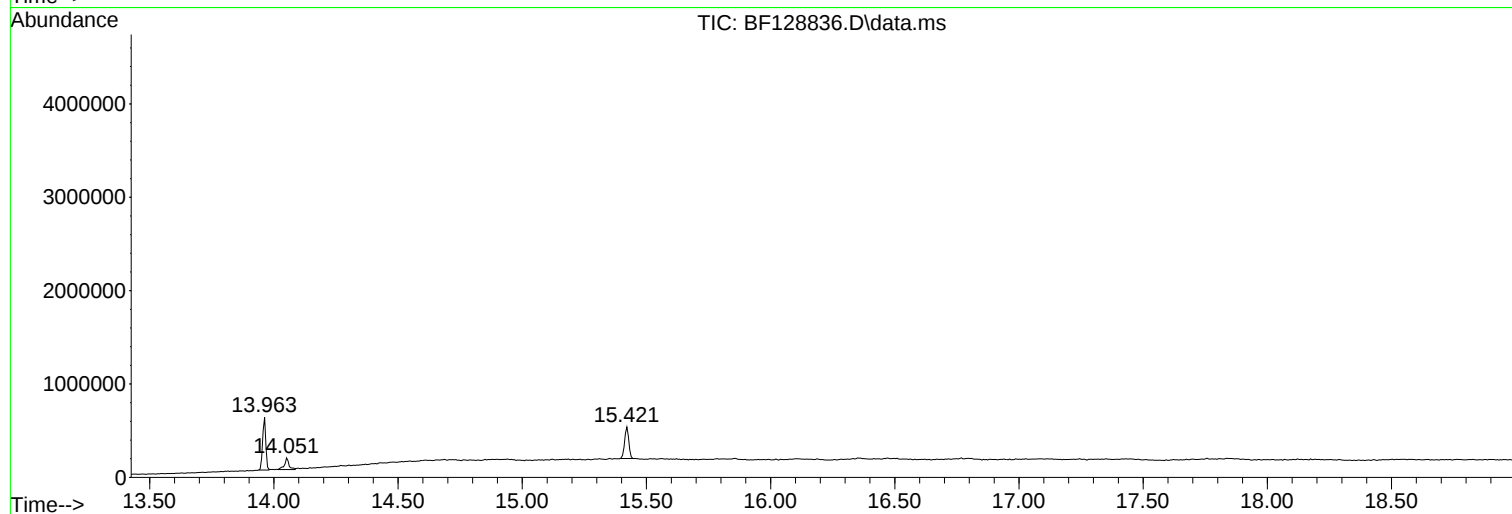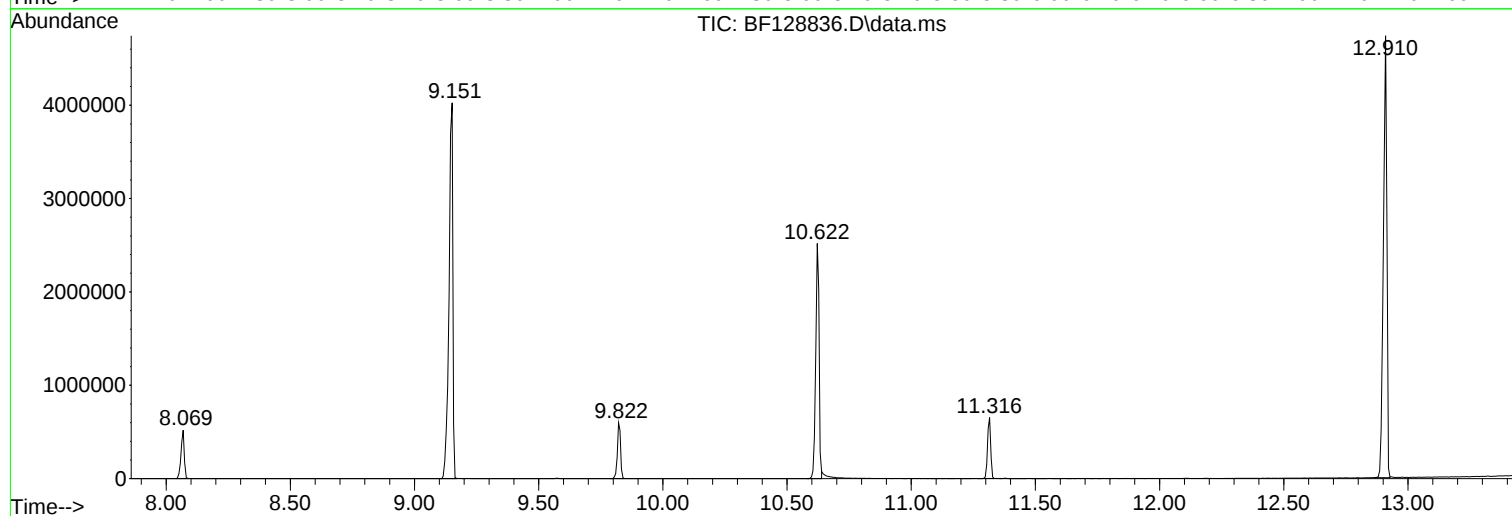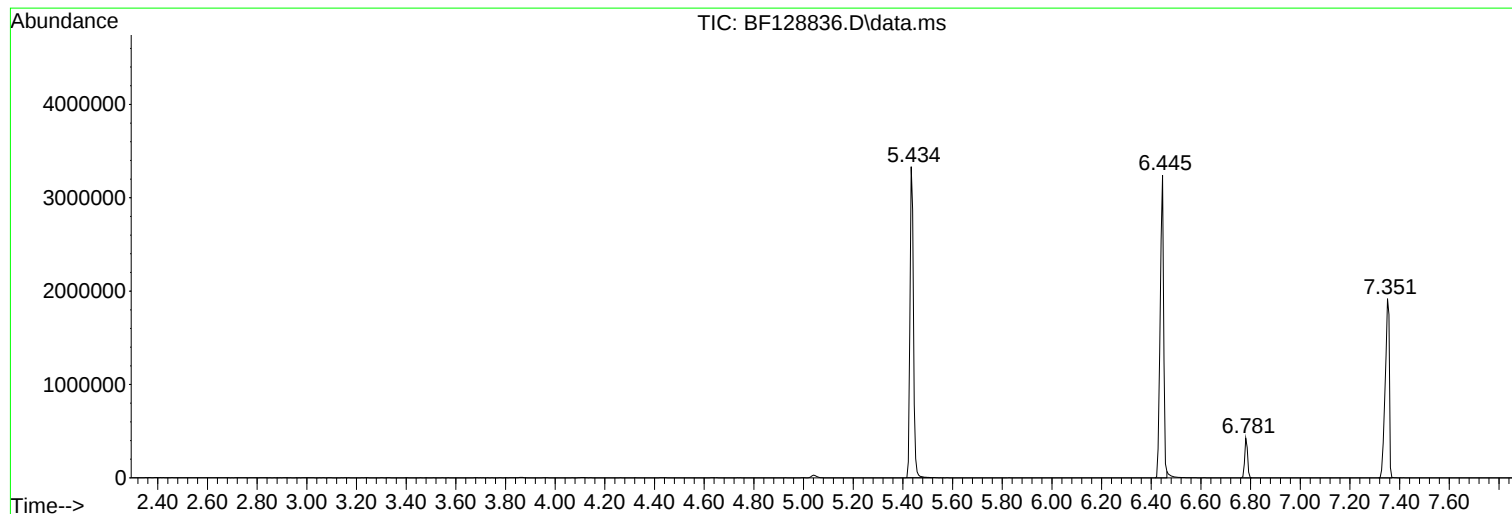

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\
Data File : BF128836.D
Acq On : 16 Jun 2022 13:23
Operator : CG\JU
Sample : PB145586BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145586BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.051	6.54 ng	161062	Chrysene-d12	13.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	94
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	70
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	64
4			Dimethoxymethyl-hydroxy-tripheny...	354	C21H23O3P	1000132-00-1	43
5			Benzoic acid, 2-(diphenylphosphi...	306	C19H15O2P	017261-28-8	40

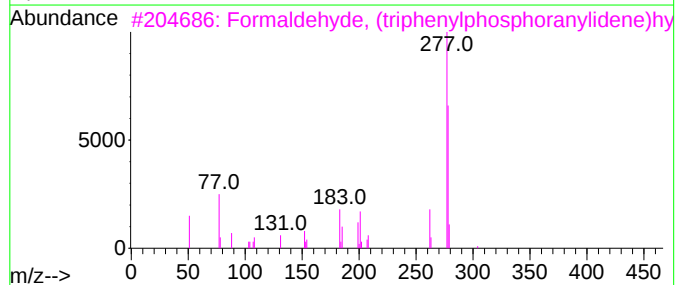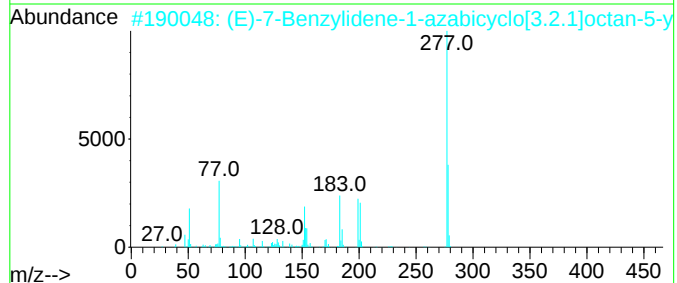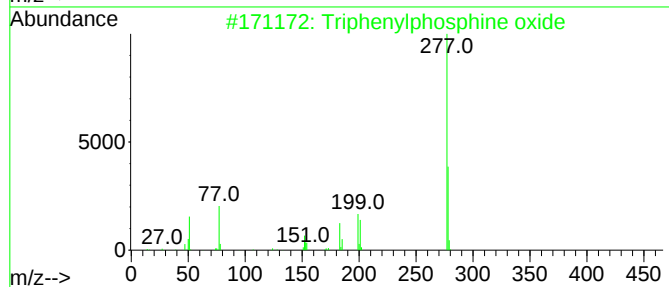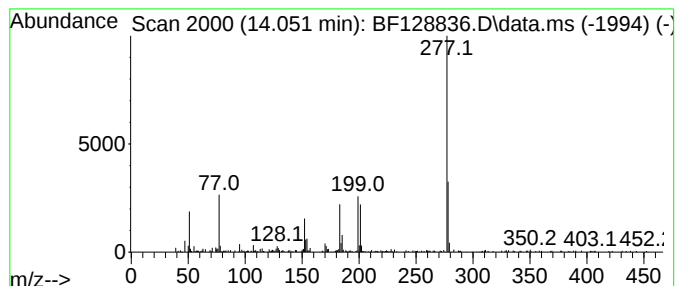

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\
Data File : BF128836.D
Acq On : 16 Jun 2022 13:23
Operator : CG\JU
Sample : PB145586BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145586BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.051	6.5	ng	161062	5	13.963	492317	20.0