


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\
 Data File : BF128832.D
 Acq On : 16 Jun 2022 11:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 14 14:53:53 2022

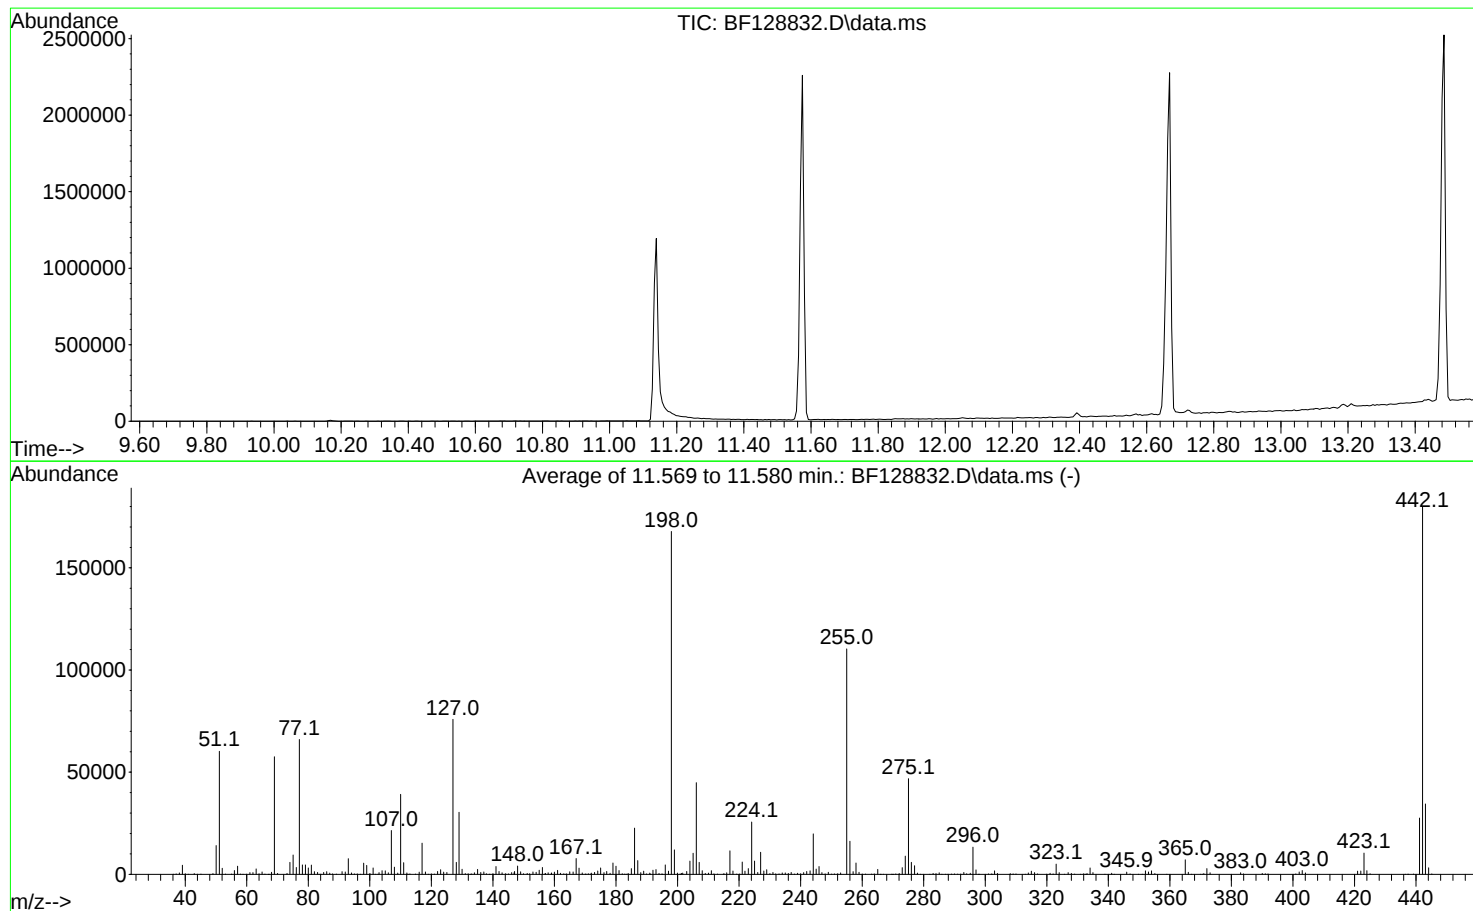




AutoFind: Scans 1578, 1579, 1580; Background Corrected with Scan 1569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	60217	PASS
68	69	0.00	2	1.8	1016	PASS
69	198	0.00	100	34.3	57588	PASS
70	69	0.00	2	0.8	460	PASS
127	198	10	80	45.2	75856	PASS
197	198	0.00	2	0.9	1593	PASS
198	198	100	100	100.0	167803	PASS
199	198	5	9	7.1	11949	PASS
275	198	10	60	27.9	46816	PASS
365	198	1	100	4.3	7149	PASS
441	198	0.01	100	16.4	27576	PASS
442	442	50	100	100.0	180029	PASS
443	442	15	24	19.1	34464	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\
 Data File : BF128832.D
 Acq On : 16 Jun 2022 11:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 17 02:28:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 14 14:53:53 2022
 Response via : Initial Calibration

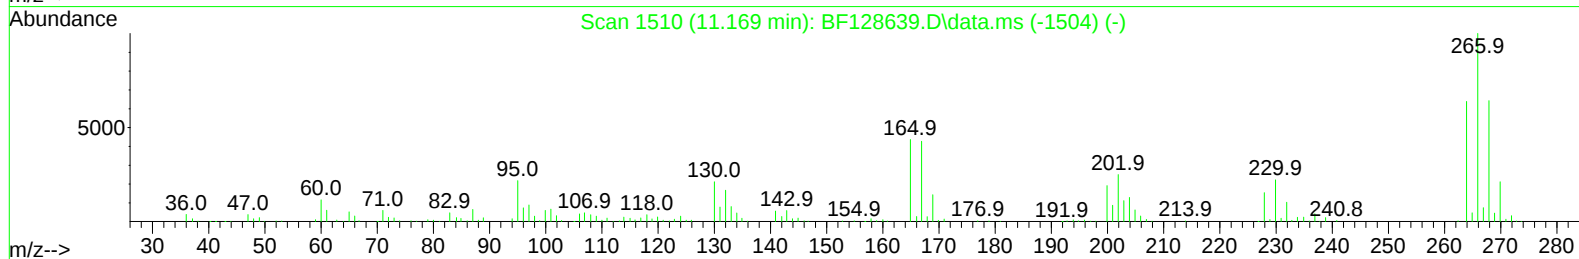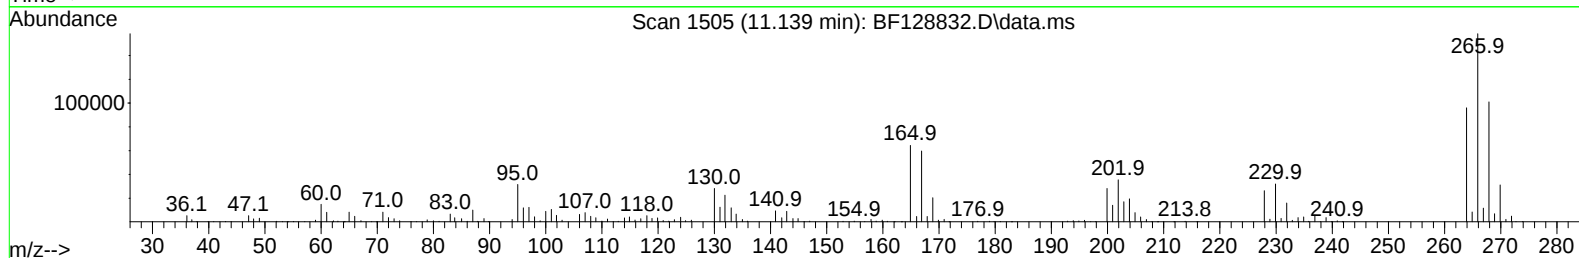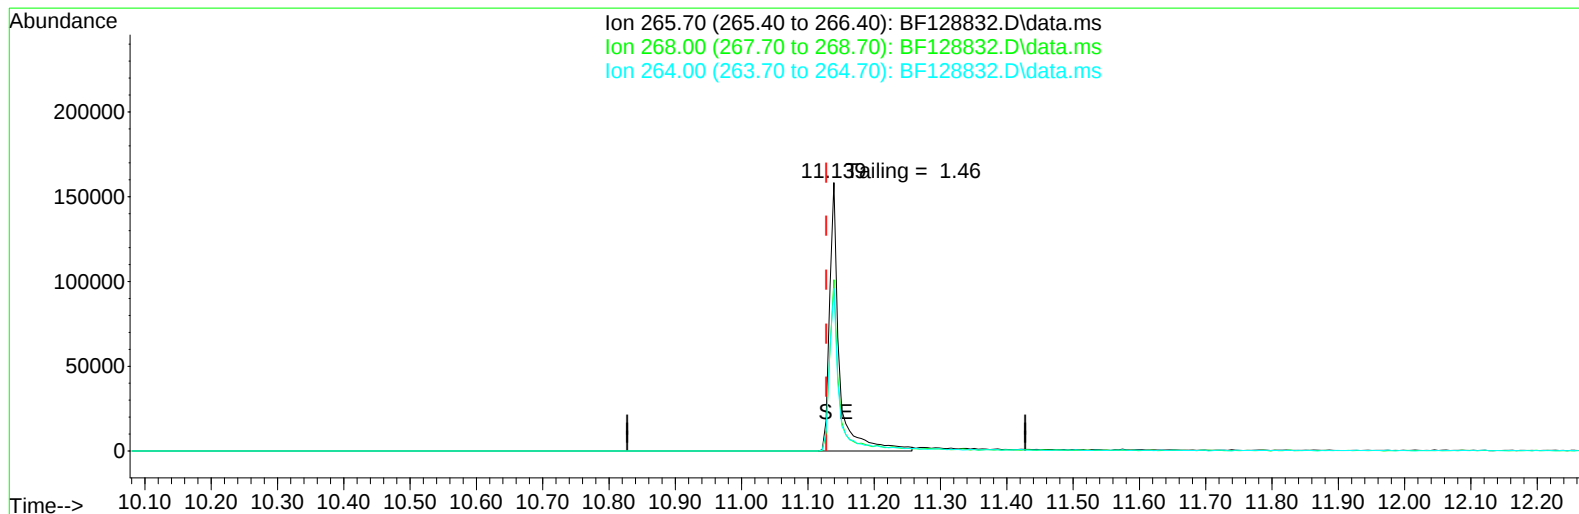

TIC: BF128832.D\data.ms

(70) Pentachlorophenol (C)

11.139min (+ 0.012) 26300.22 ng




response 164220

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.77
264.00	61.80	60.60
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061622\  
Data File : BF128832.D  
Acq On    : 16 Jun 2022  11:22  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 17 02:28:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 14 14:53:53 2022
Response via : Initial Calibration

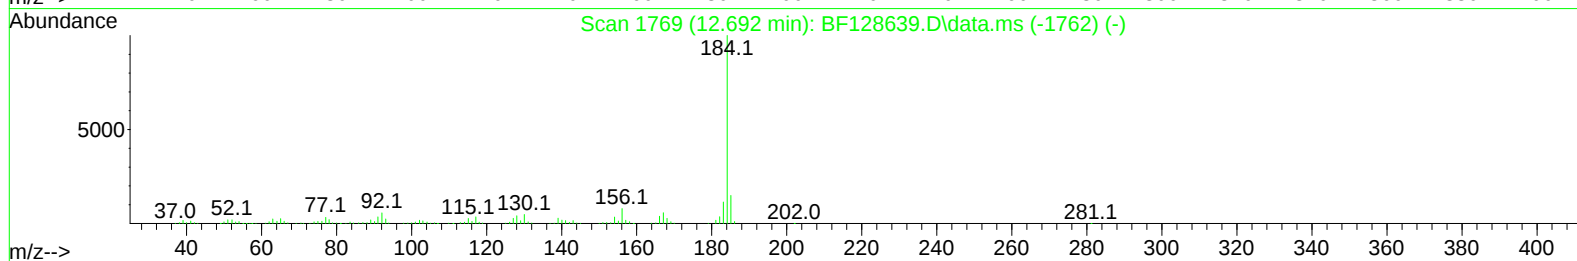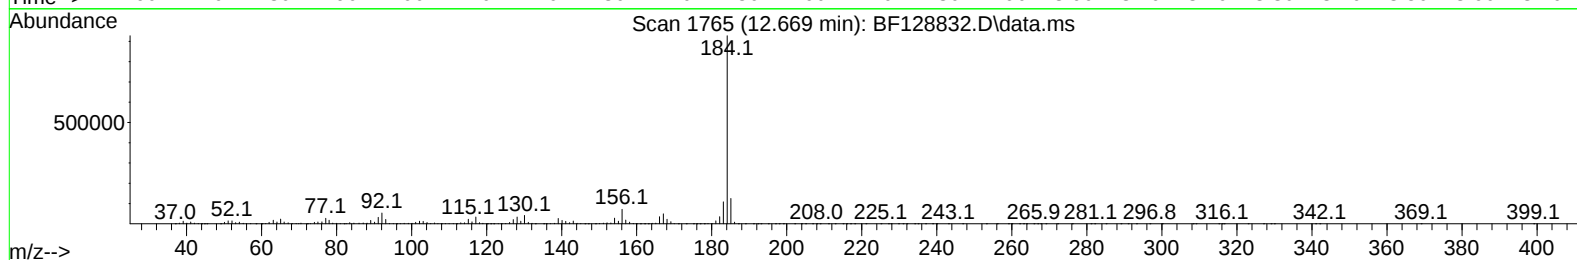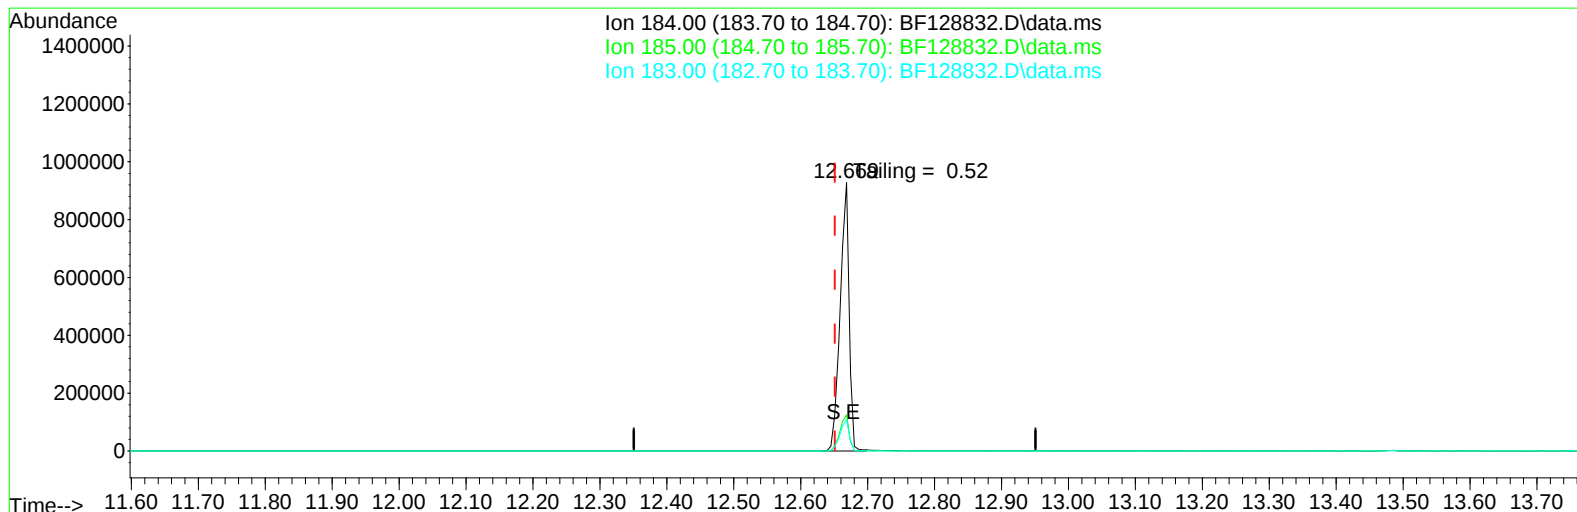

TIC: BF128832.D\data.ms

(77) Benzidine

12.669min (+ 0.018) 349560.40 ng

response **857101**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.90	13.49
--------	-------	-------

183.00	11.60	11.64
--------	-------	-------

0.00 0.00 0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/16/2022	BNA_F	<u>BF128832.D</u>
Compound Name	Response	Retention Time
DDT	413815	13.486
DDD	7486	13.186
DDE	1137	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8623	422438	2.04

Instrument :
BNA_F
ClientSampleId :
DFTPP