
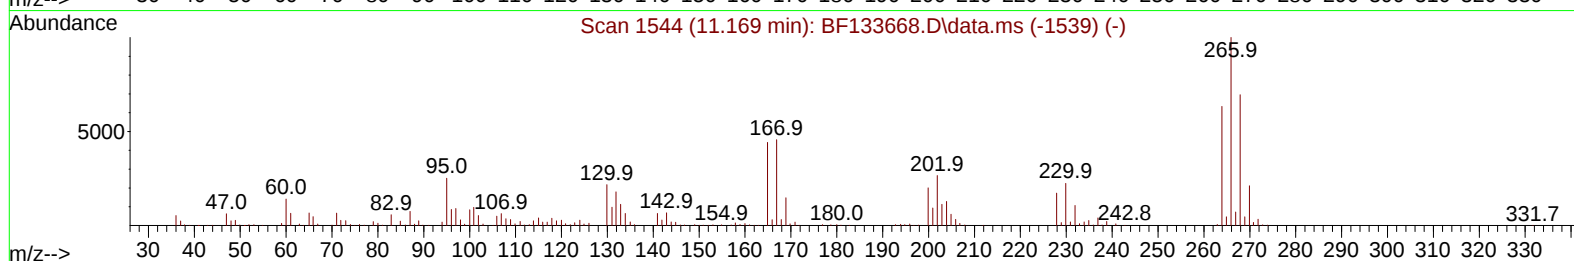
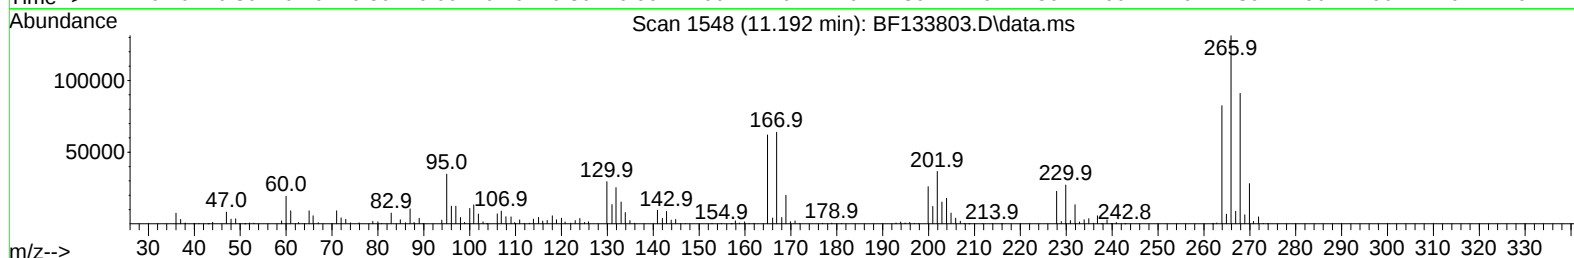


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061623\
Data File : BF133803.D
Acq On : 16 Jun 2023 13:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 15:40:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 14:54:03 2023
Response via : Initial Calibration

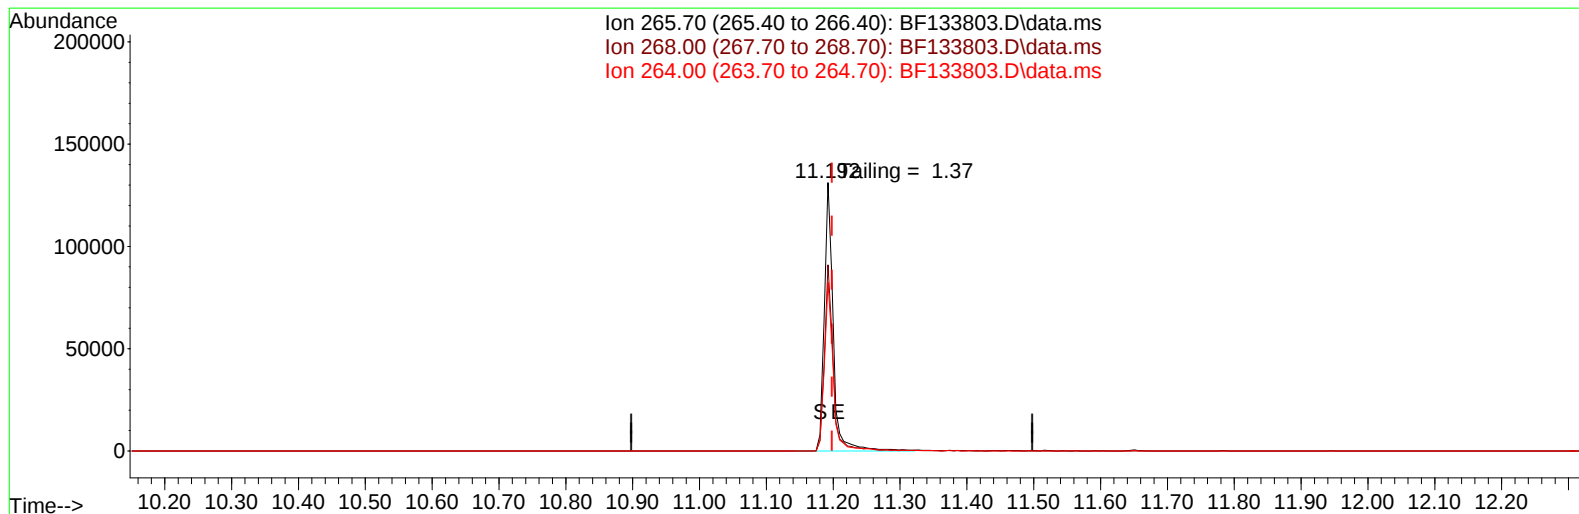

TIC: BF133803.D\data.ms

(70) Pentachlorophenol (C)




11.192min (-0.006) 23570.37 ng

response 121261

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	69.37
264.00	63.40	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061623\
Data File : BF133803.D
Acq On : 16 Jun 2023 13:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 15:40:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 14:54:03 2023
Response via : Initial Calibration

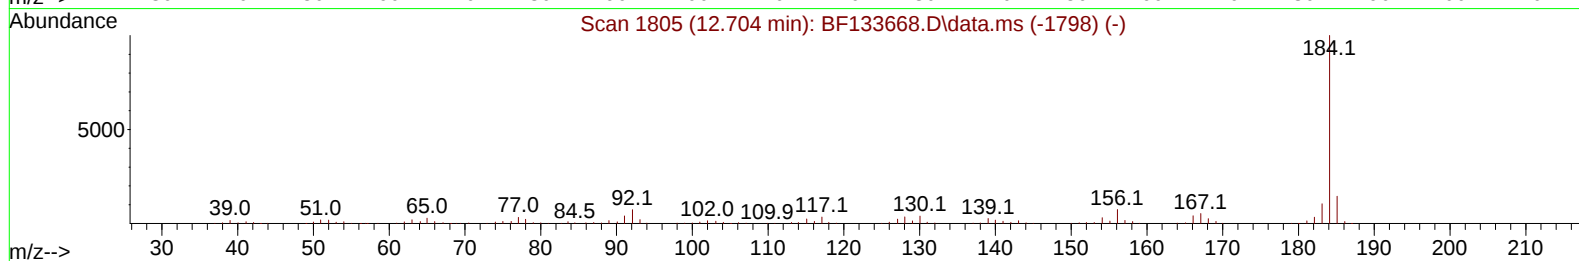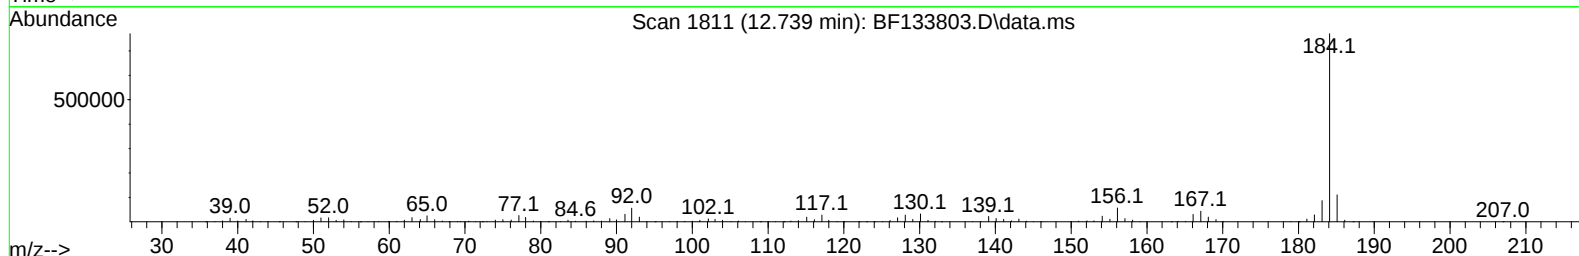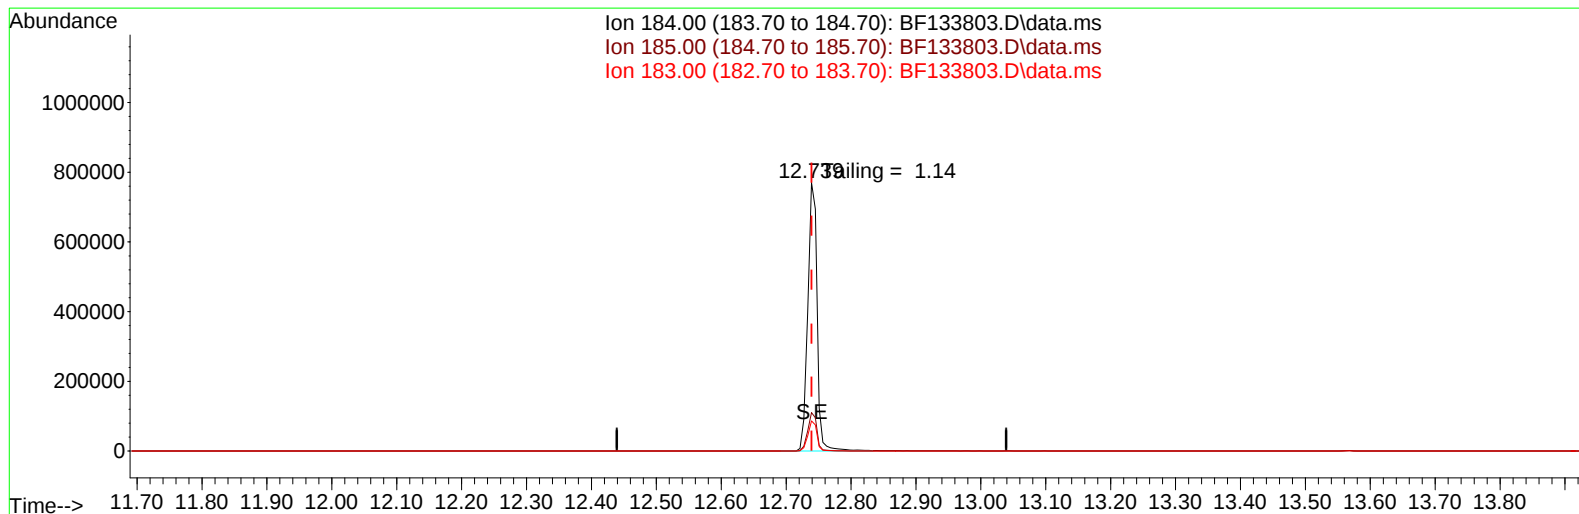

TIC: BF133803.D\data.ms

(77) Benzidine

12.739min (-0.000) 0.00 ng

response 770955

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.30
183.00	10.50	11.25
0.00	0.00	0.00