


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061623\
 Data File : BF133803.D
 Acq On : 16 Jun 2023 13:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 16 14:54:03 2023

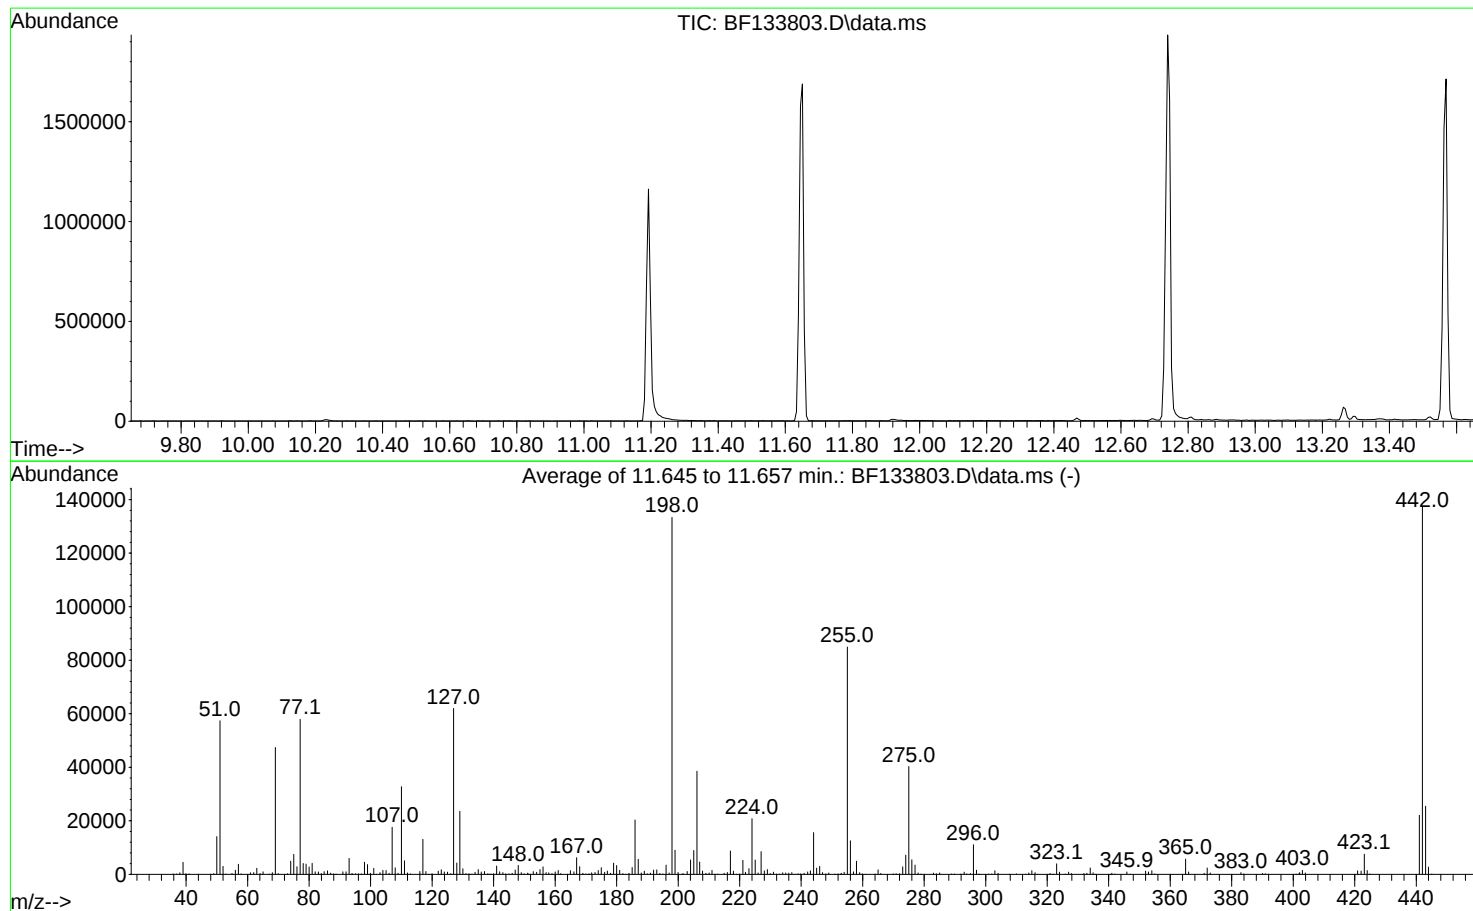

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	57408	PASS
68	69	0.00	2	1.4	666	PASS
69	198	0.00	100	35.5	47403	PASS
70	69	0.00	2	0.6	280	PASS
127	198	10	80	46.5	61960	PASS
197	198	0.00	2	0.4	551	PASS
198	198	100	100	100.0	133357	PASS
199	198	5	9	6.8	9016	PASS
275	198	10	60	30.2	40304	PASS
365	198	1	100	4.3	5702	PASS
441	198	0.01	100	16.5	22069	PASS
442	442	50	100	100.0	137411	PASS
443	442	15	24	18.5	25472	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/16/2023	BNA_F	<u>BF133803.D</u>
Compound Name	Response	Retention Time
DDT	287408	13.568
DDD	14957	13.268
DDE	480	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15437	302845	5.10

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061623\
 Data File : BF133803.D
 Acq On : 16 Jun 2023 13:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 16 15:40:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 16 14:54:03 2023
 Response via : Initial Calibration

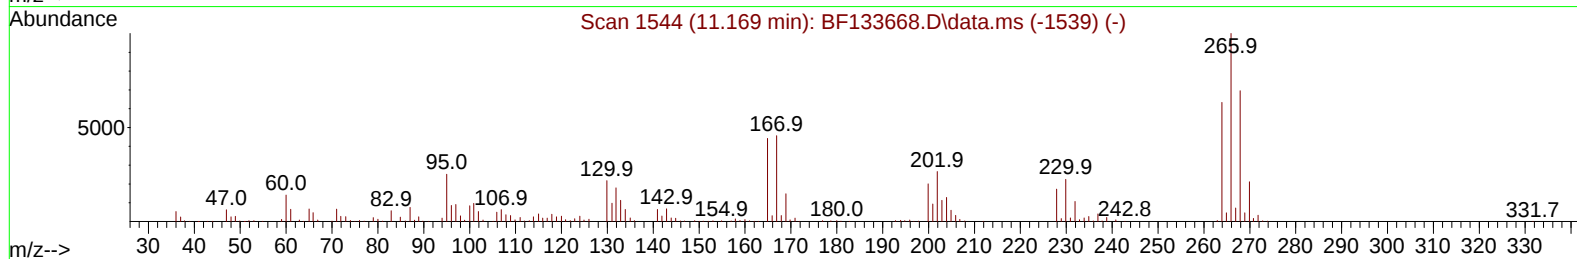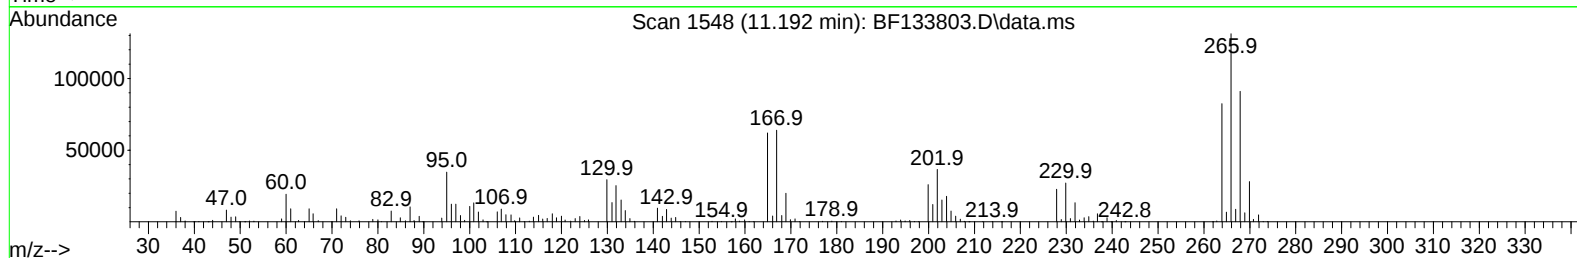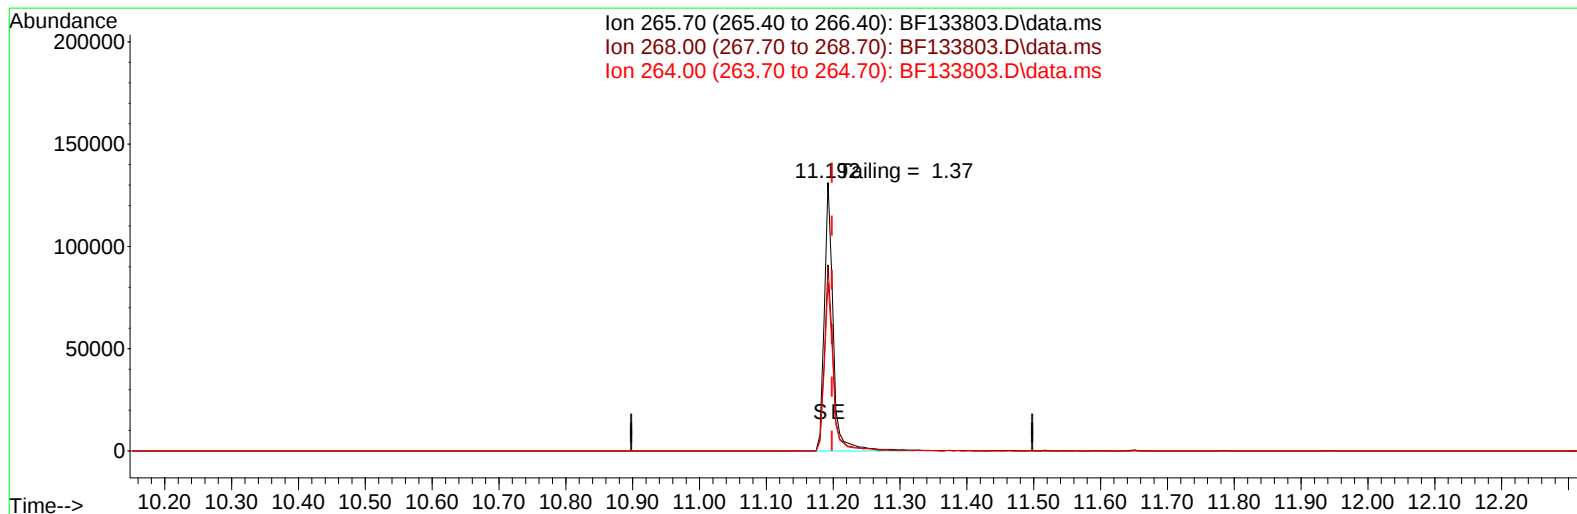

TIC: BF133803.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 23570.37 ng




response 121261

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	69.37
264.00	63.40	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061623\
Data File : BF133803.D
Acq On : 16 Jun 2023 13:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 16 15:40:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 14:54:03 2023
Response via : Initial Calibration

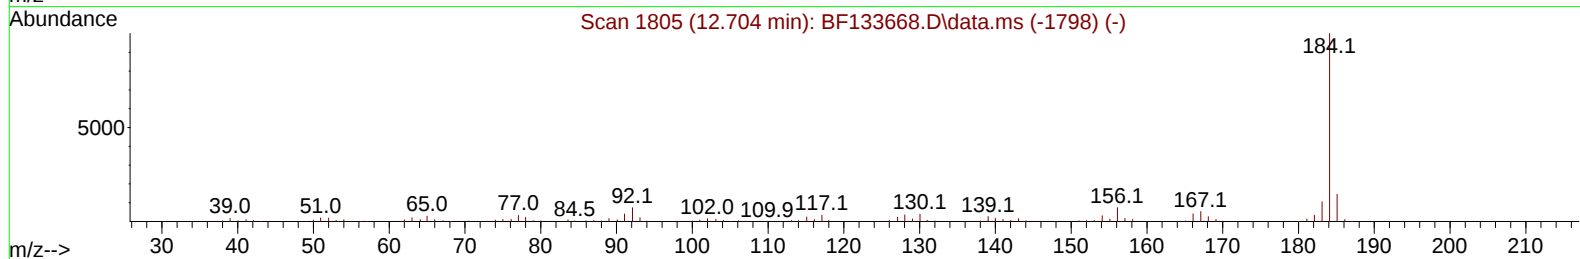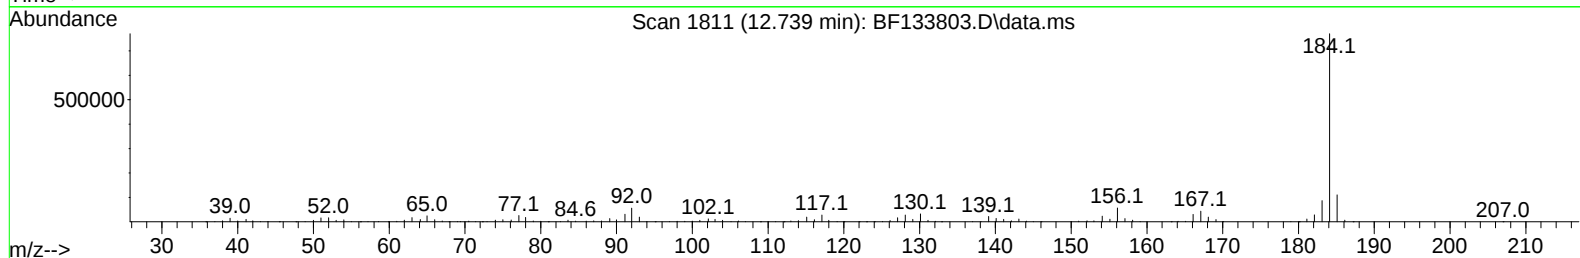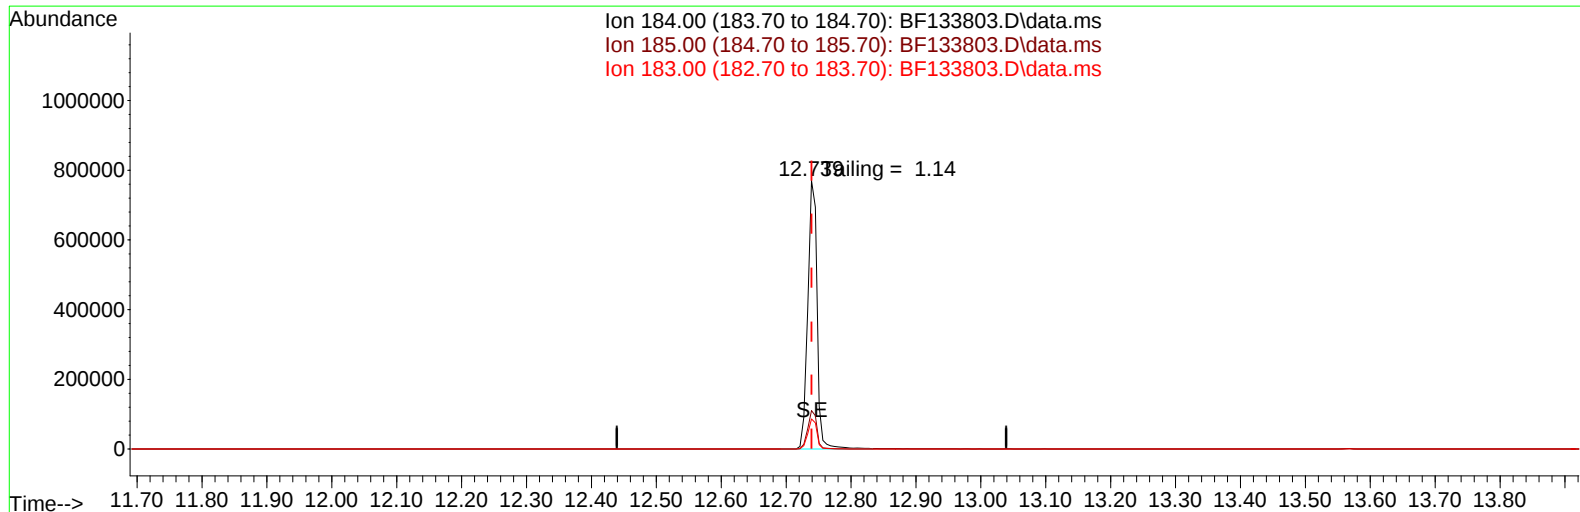

TIC: BF133803.D\data.ms

(77) Benzidine

12.739min (-0.000) 0.00 ng

response 770955

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.30
183.00	10.50	11.25
0.00	0.00	0.00