
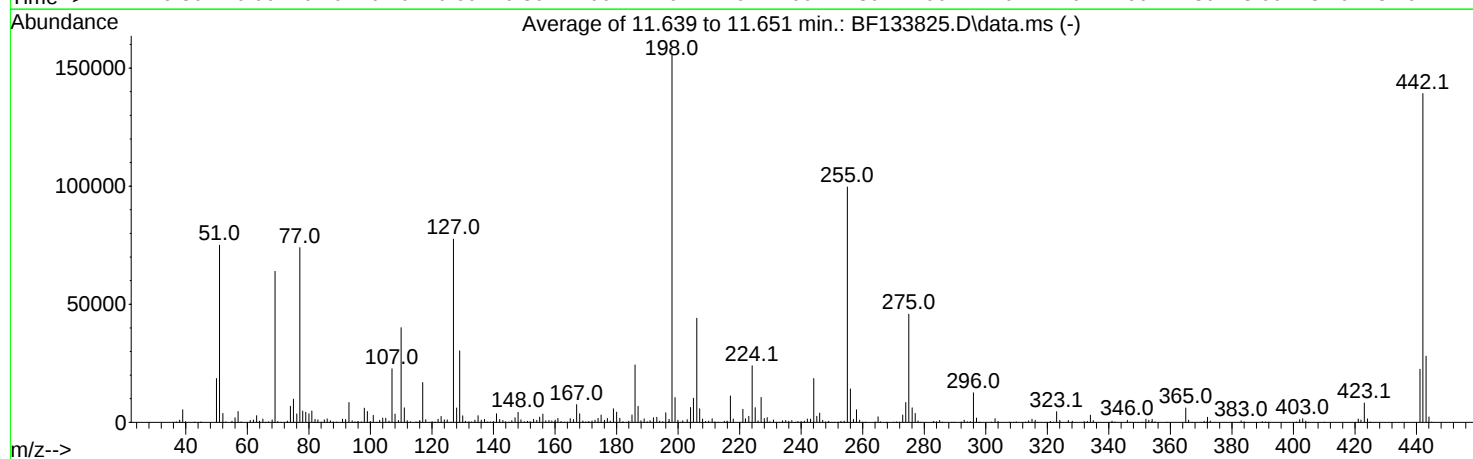


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061923\
 Data File : BF133825.D
 Acq On : 19 Jun 2023 10:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 19 16:00:59 2023

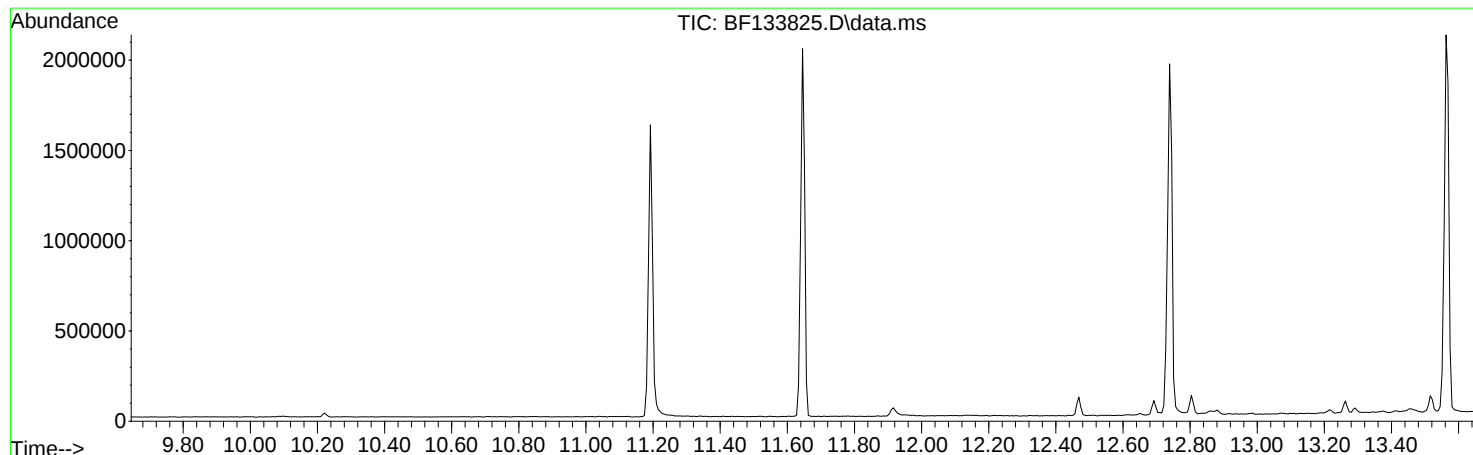




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	75004	PASS
68	69	0.00	2	1.7	1065	PASS
69	198	0.00	100	41.1	63973	PASS
70	69	0.00	2	0.5	348	PASS
127	198	10	80	49.8	77547	PASS
197	198	0.00	2	0.8	1266	PASS
198	198	100	100	100.0	155741	PASS
199	198	5	9	6.8	10517	PASS
275	198	10	60	29.4	45787	PASS
365	198	1	100	3.9	6095	PASS
441	198	0.01	100	14.4	22482	PASS
442	442	50	100	100.0	139232	PASS
443	442	15	24	20.2	28079	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061923\
Data File : BF133825.D
Acq On : 19 Jun 2023 10:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 19 11:52:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 14:54:03 2023
Response via : Initial Calibration

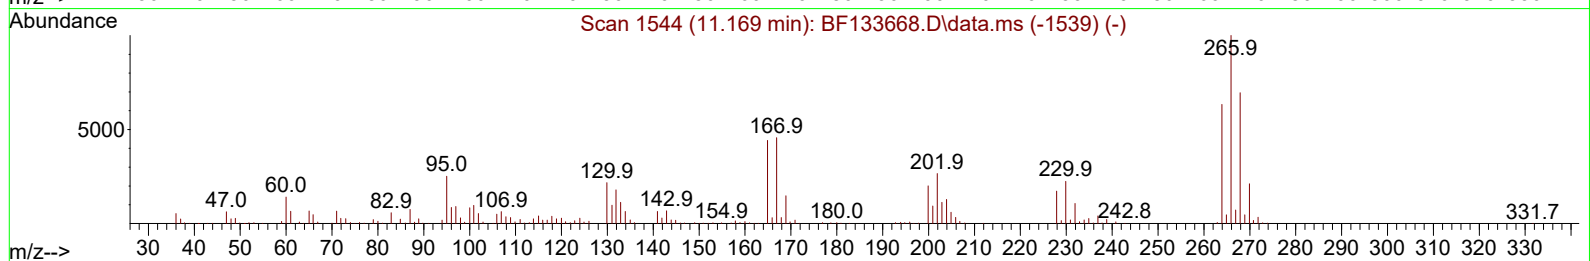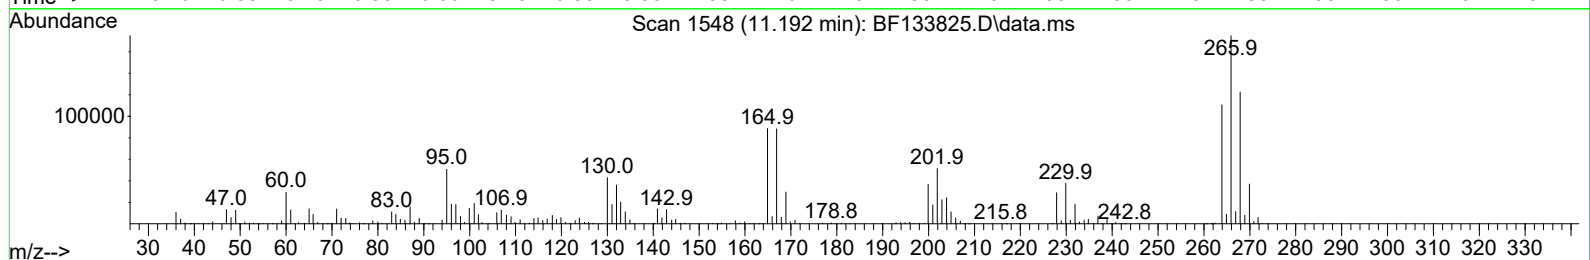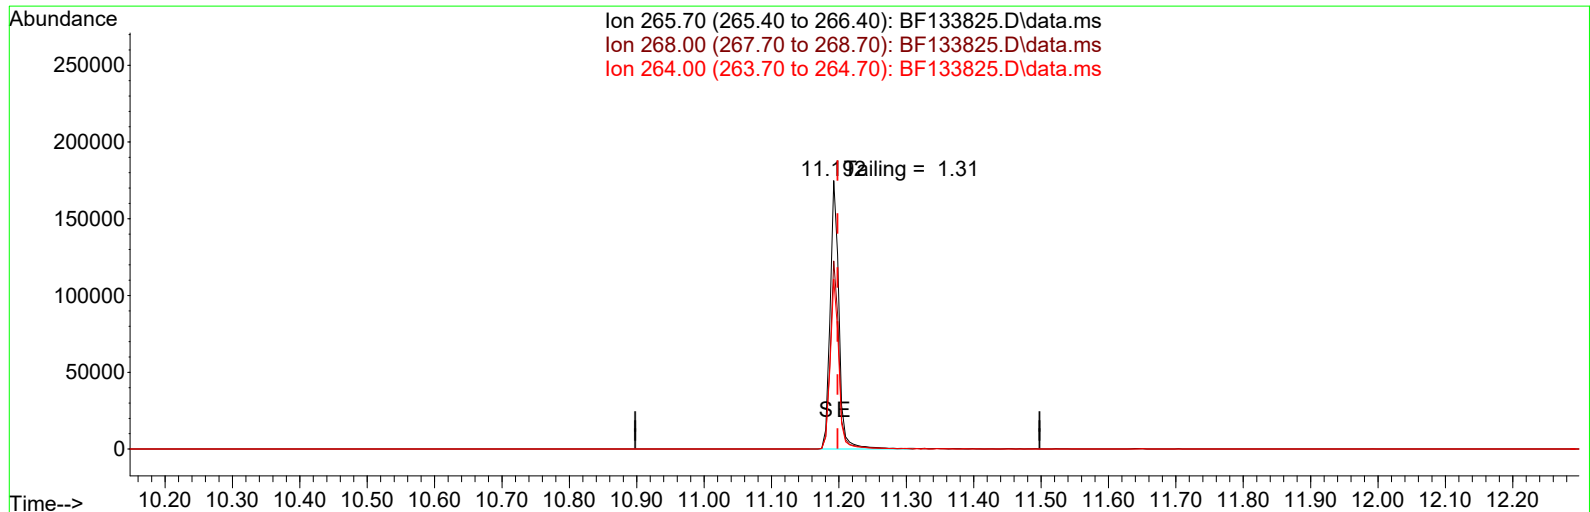

TIC: BF133825.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 91353.24 ng




response 159870

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	70.09
264.00	63.40	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF061923\
 Data File : BF133825.D
 Acq On : 19 Jun 2023 10:22
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 19 11:52:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 16 14:54:03 2023
 Response via : Initial Calibration

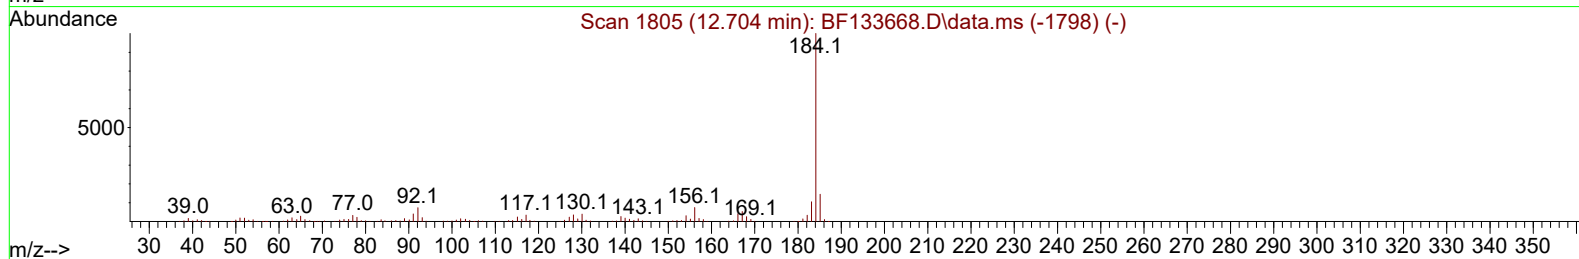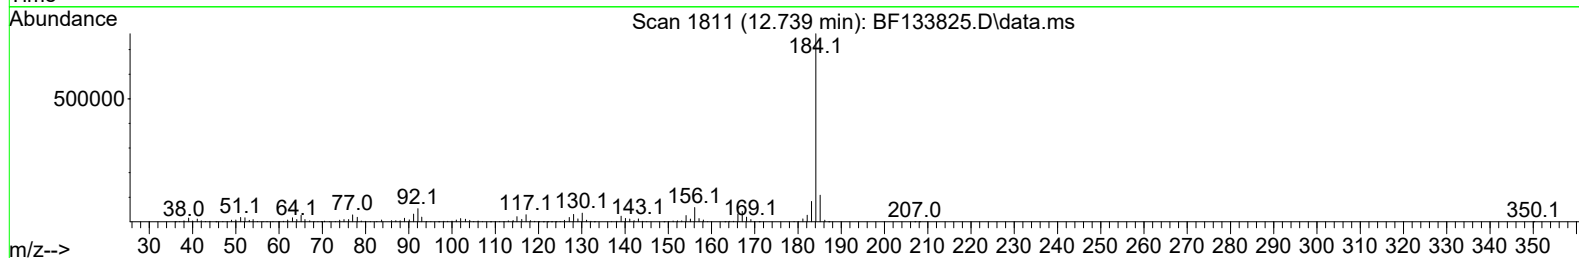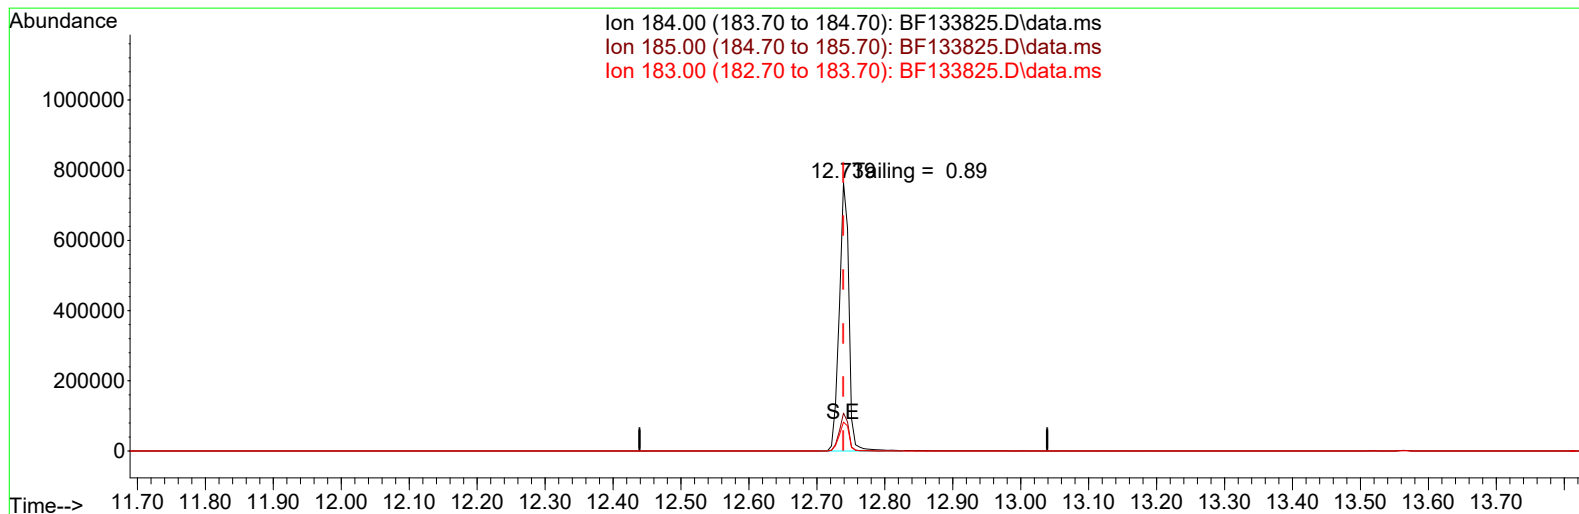

TIC: BF133825.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 53213.20 ng

response 748175

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.16
183.00	10.50	10.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/19/2023	BNA_F	<u>BF133825.D</u>
Compound Name	Response	Retention Time
DDT	364687	13.563
DDD	14310	13.263
DDE	354	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14664	379351	3.87

Instrument :
BNA_F
ClientSampleId :
DFTPP