
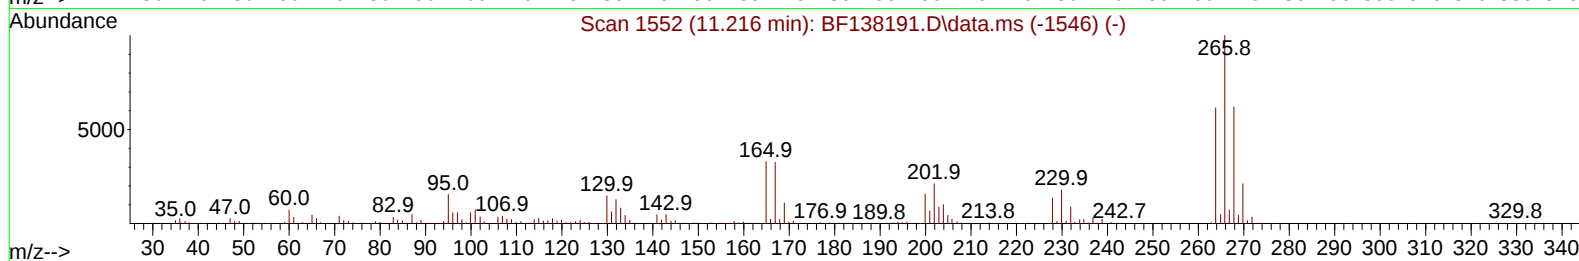
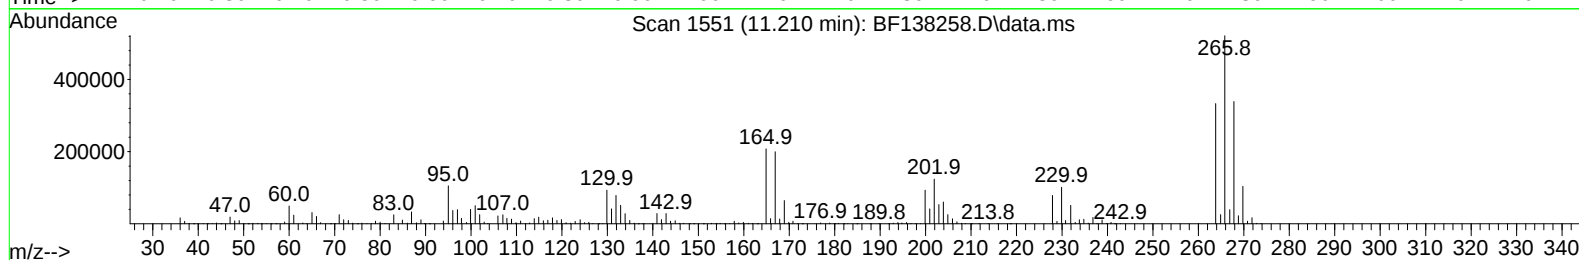


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF062024\  
Data File : BF138258.D  
Acq On : 20 Jun 2024 11:14  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 11:57:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF061224.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 13 01:52:47 2024  
Response via : Initial Calibration

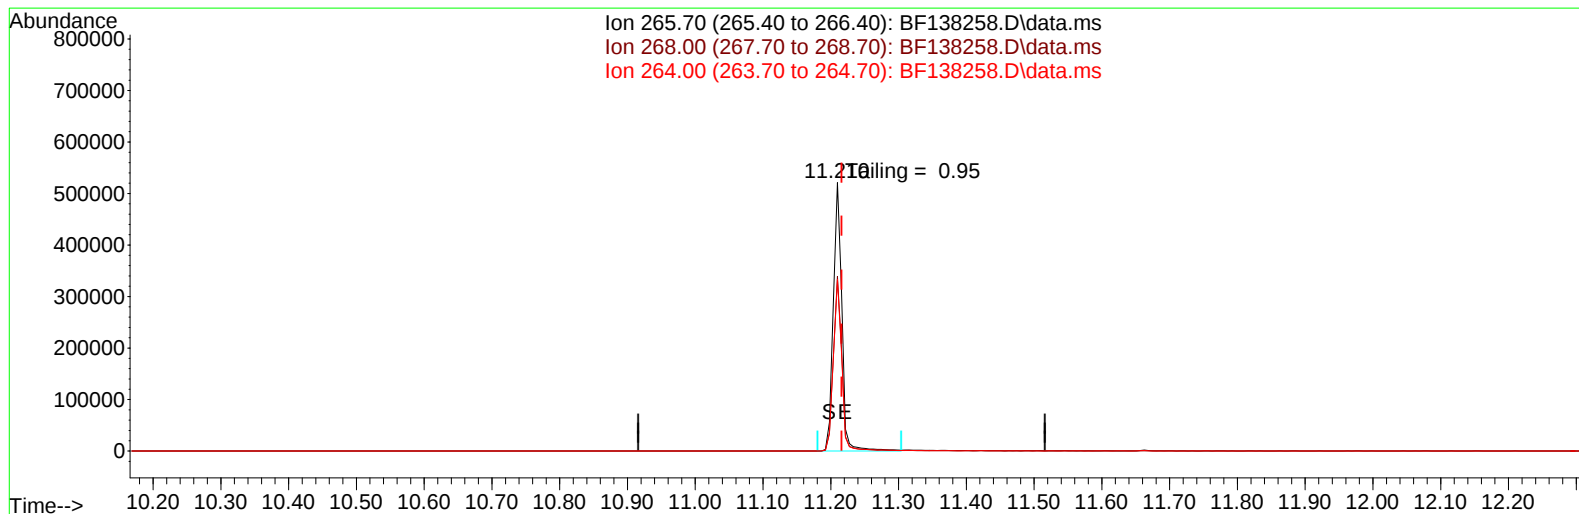

TIC: BF138258.D\data.ms

**(70) Pentachlorophenol (C)**




**11.210min (-0.006) 313866.19 ng**

**response 457351**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.90  | 65.06  |
| 264.00 | 61.50  | 63.93  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF062024\  
Data File : BF138258.D  
Acq On : 20 Jun 2024 11:14  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 11:57:43 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF061224.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jun 13 01:52:47 2024  
Response via : Initial Calibration

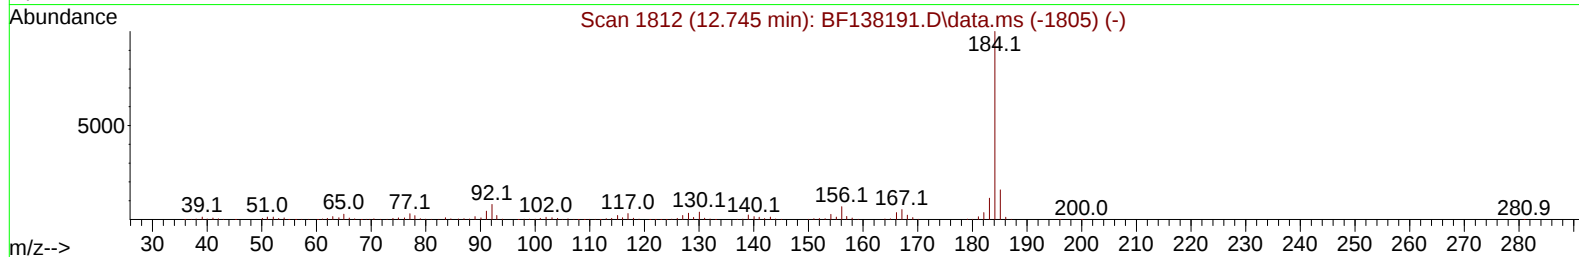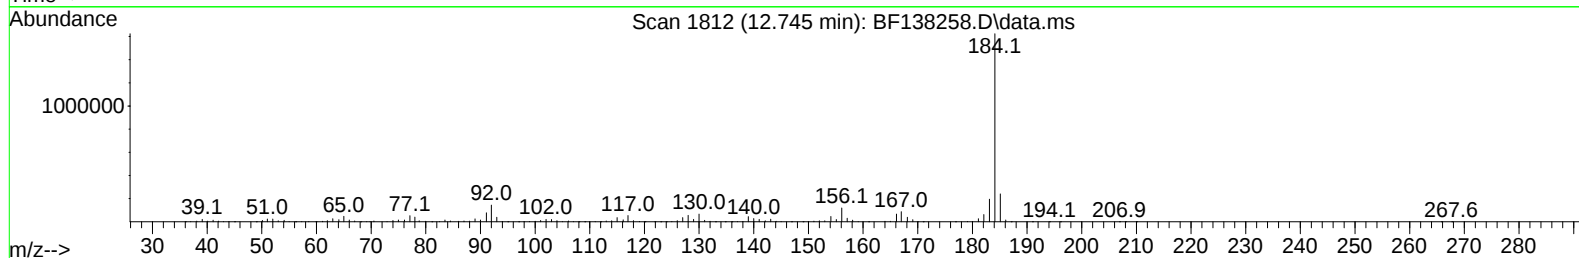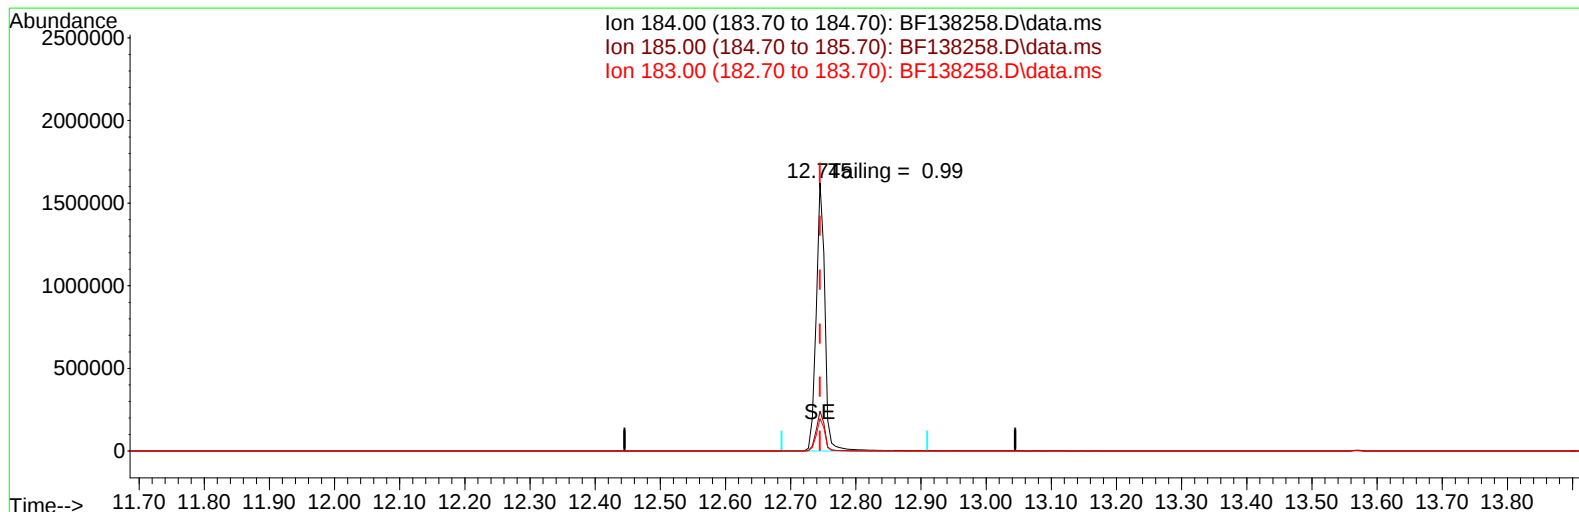

TIC: BF138258.D\data.ms

**(77) Benzidine**

12.745min (-0.000) 2324132.74 ng

response 1505424

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.80  | 14.79  |
| 183.00 | 11.30  | 12.05  |
| 0.00   | 0.00   | 0.00   |