


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062024\
Data File : BF138258.D
Acq On : 20 Jun 2024 11:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 13 01:52:47 2024

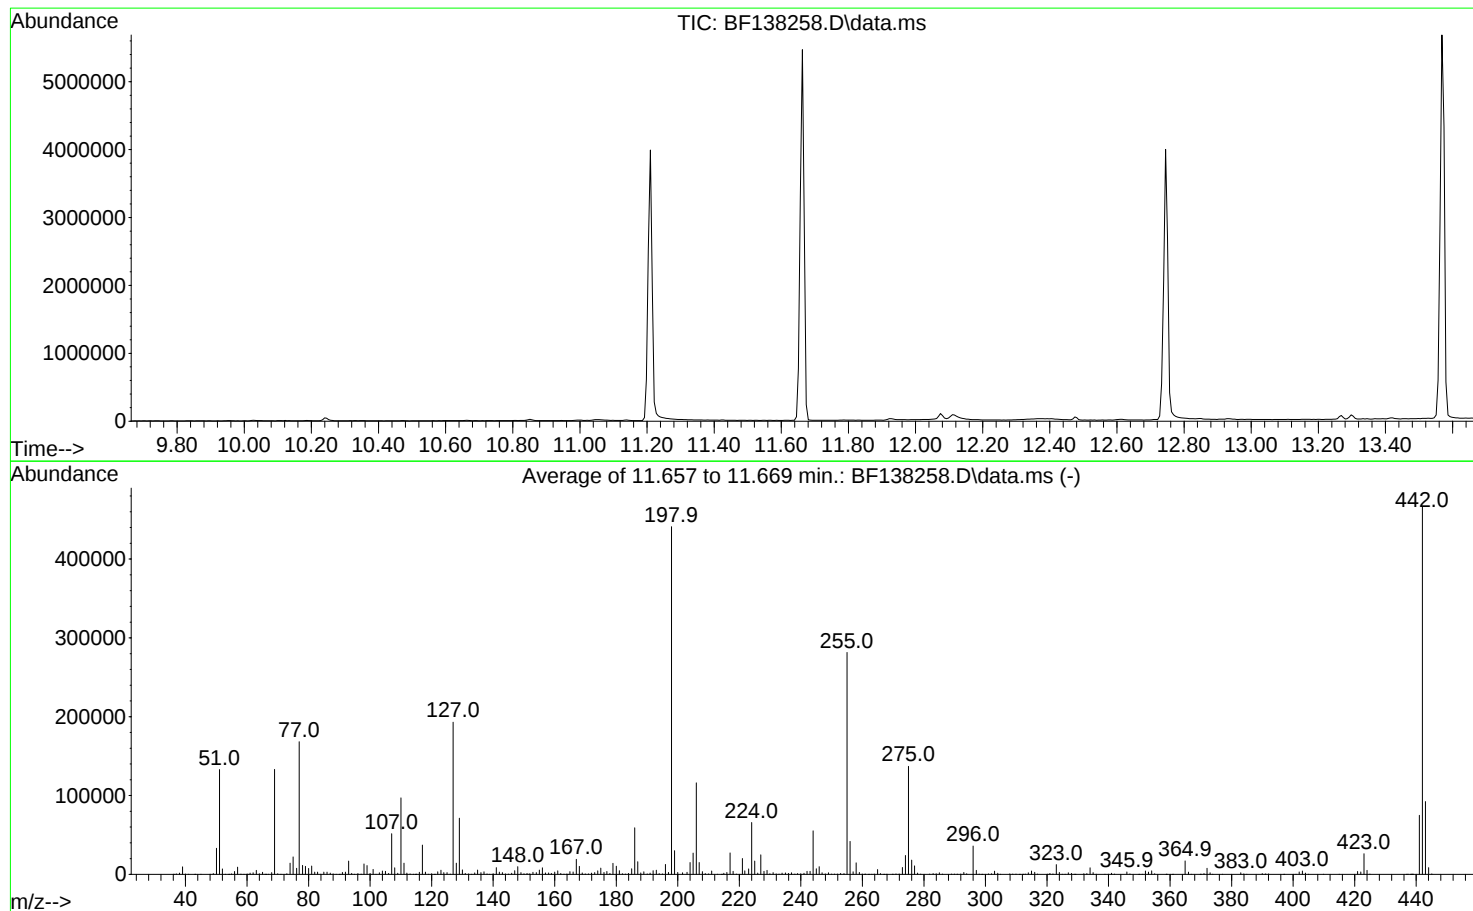

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	133064	PASS
68	69	0.00	2	1.7	2240	PASS
69	198	0.00	100	30.2	133174	PASS
70	69	0.00	2	0.5	721	PASS
127	198	10	80	43.8	193032	PASS
197	198	0.00	2	0.6	2524	PASS
198	198	100	100	100.0	441131	PASS
199	198	5	9	6.8	30131	PASS
275	198	10	60	31.1	137048	PASS
365	198	1	100	3.9	17135	PASS
441	198	0.01	100	17.0	74843	PASS
442	442	50	100	100.0	466688	PASS
443	442	15	24	19.8	92435	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/20/2024	BNA_F	<u>BF138258.D</u>
Compound Name	Response	Retention Time
DDT	1019473	13.568
DDD	18772	13.268
DDE	2673	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21445	1040918	2.06

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062024\
 Data File : BF138258.D
 Acq On : 20 Jun 2024 11:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 20 11:57:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 13 01:52:47 2024
 Response via : Initial Calibration

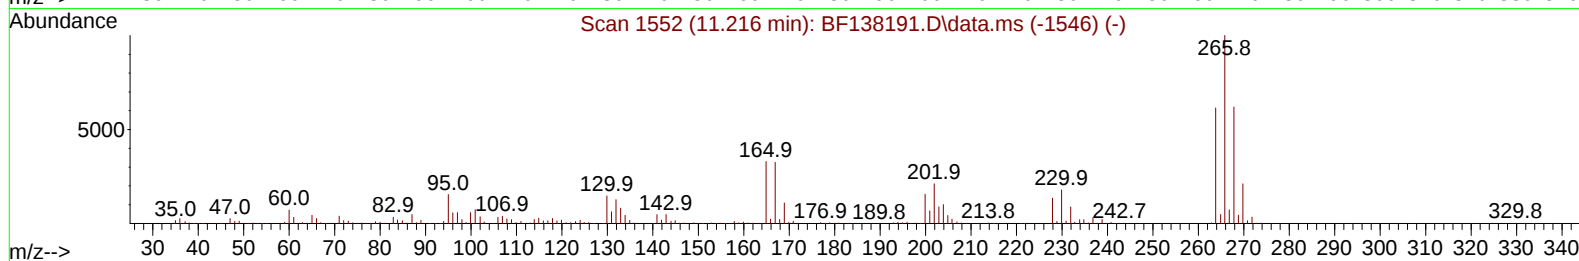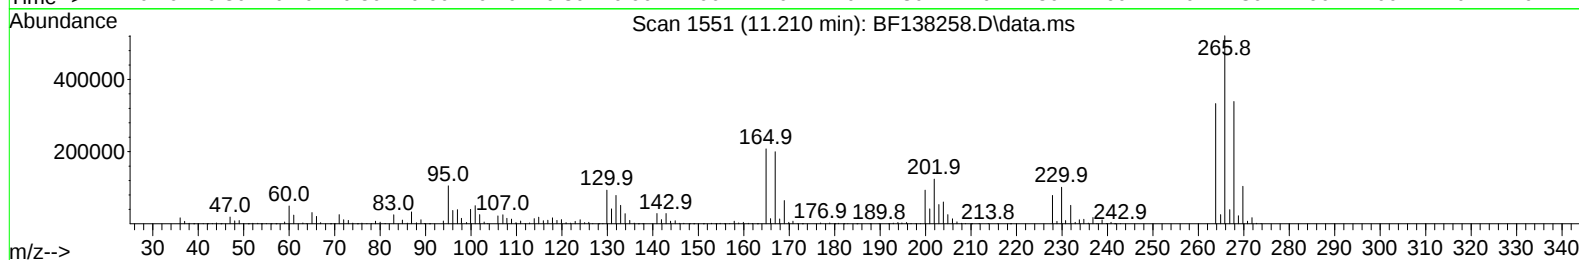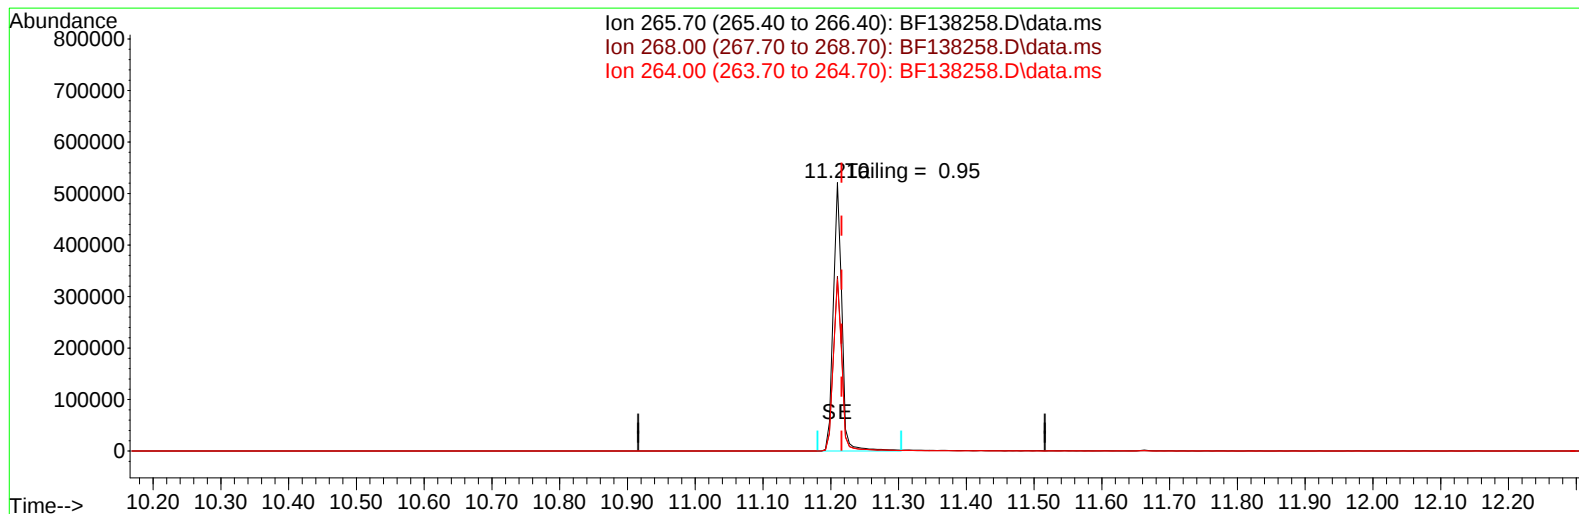

TIC: BF138258.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 313866.19 ng




response 457351

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	65.06
264.00	61.50	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062024\
Data File : BF138258.D
Acq On : 20 Jun 2024 11:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 20 11:57:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF061224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 13 01:52:47 2024
Response via : Initial Calibration

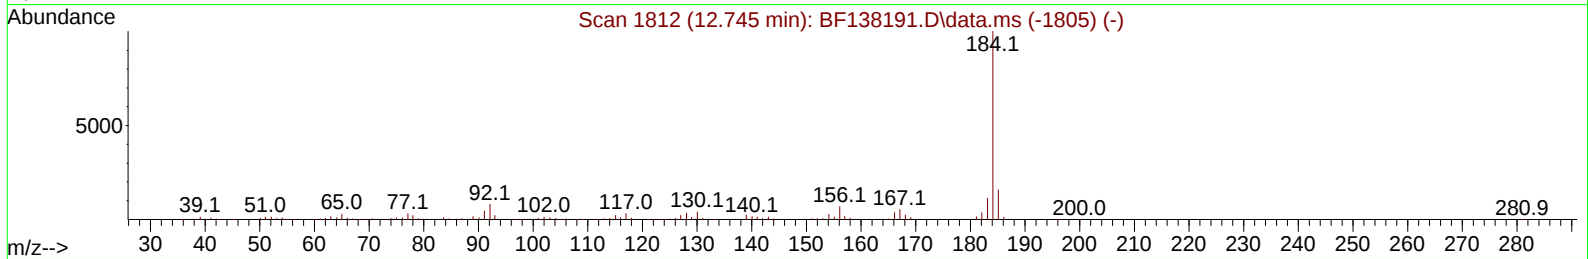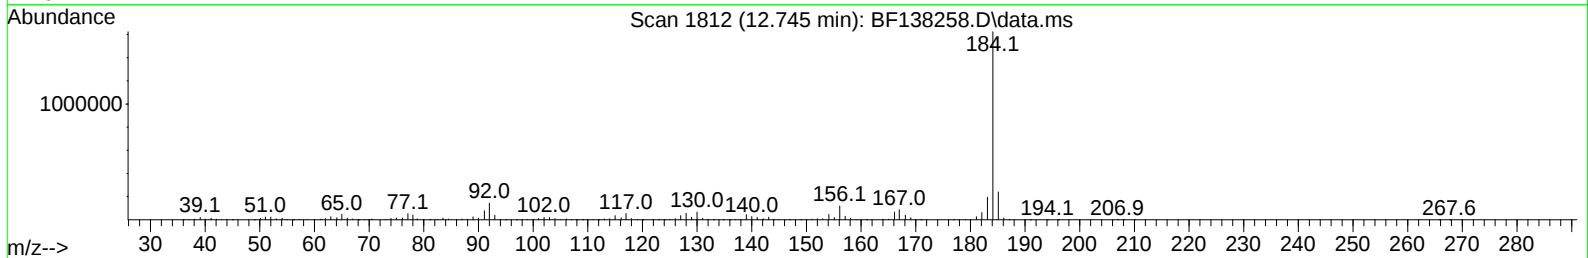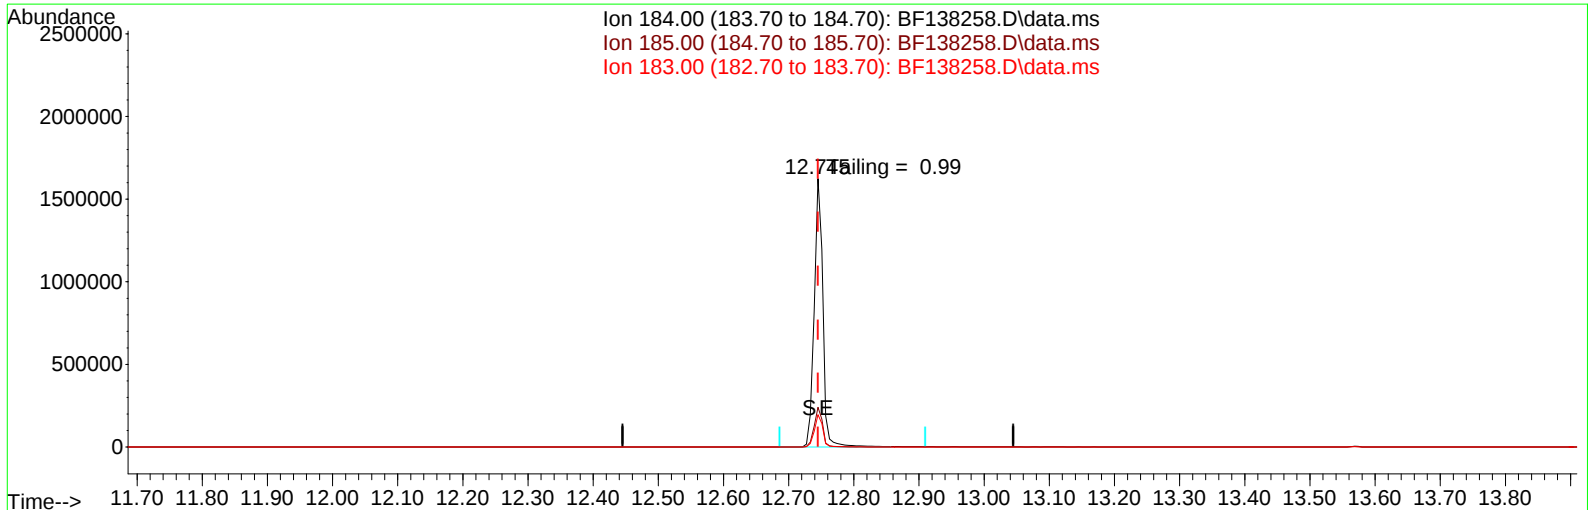

TIC: BF138258.D\data.ms

(77) Benzidine

12.745min (-0.000) 2324132.74 ng

response 1505424

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.80	14.79
183.00	11.30	12.05
0.00	0.00	0.00