

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062118\
 Data File : BF106658.D
 Acq On : 21 Jun 2018 13:39
 Operator : JU/SJ
 Sample : J3584-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-12-D

Quant Time: Jun 21 14:33:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 19 14:32:09 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.96	152	93049	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	362747	20.00	ng	0.00
38) Acenaphthene-d10	10.00	164	181351	20.00	ng	0.00
63) Phenanthrene-d10	11.49	188	329358	20.00	ng	0.00
75) Chrysene-d12	14.15	240	269134	20.00	ng	0.00
86) Perylene-d12	15.69	264	210090	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	561662	102.21	ng	0.00
7) Phenol-d6	6.61	99	724922	105.64	ng	0.00
23) Nitrobenzene-d5	7.52	82	481832	73.82	ng	0.00
41) 2,4,6-Tribromophenol	10.79	330	233368	111.03	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	831650	76.07	ng	0.00
78) Terphenyl-d14	13.08	244	888678	79.98	ng	0.00
Target Compounds						
10) Phenol	6.62	94	18054	2.305	ng	99
19) n-Nitroso-di-n-propylamine	7.52	70	62844	13.893	ng	# 75
25) Isophorone	7.52	82	481826	41.890	ng	# 64
49) Dimethylphthalate	9.71	163	126654	9.312	ng	98
56) 2,4-Dinitrotoluene	10.00	165	23468	6.242	ng	# 23
66) 4-Bromophenyl-phenylether	10.79	248	14458	3.678	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062118\
Data File : BF106658.D
Acq On : 21 Jun 2018 13:39
Operator : JU/SJ
Sample : J3584-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-12-D

Quant Time: Jun 21 14:33:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 19 14:32:09 2018
Response via : Initial Calibration

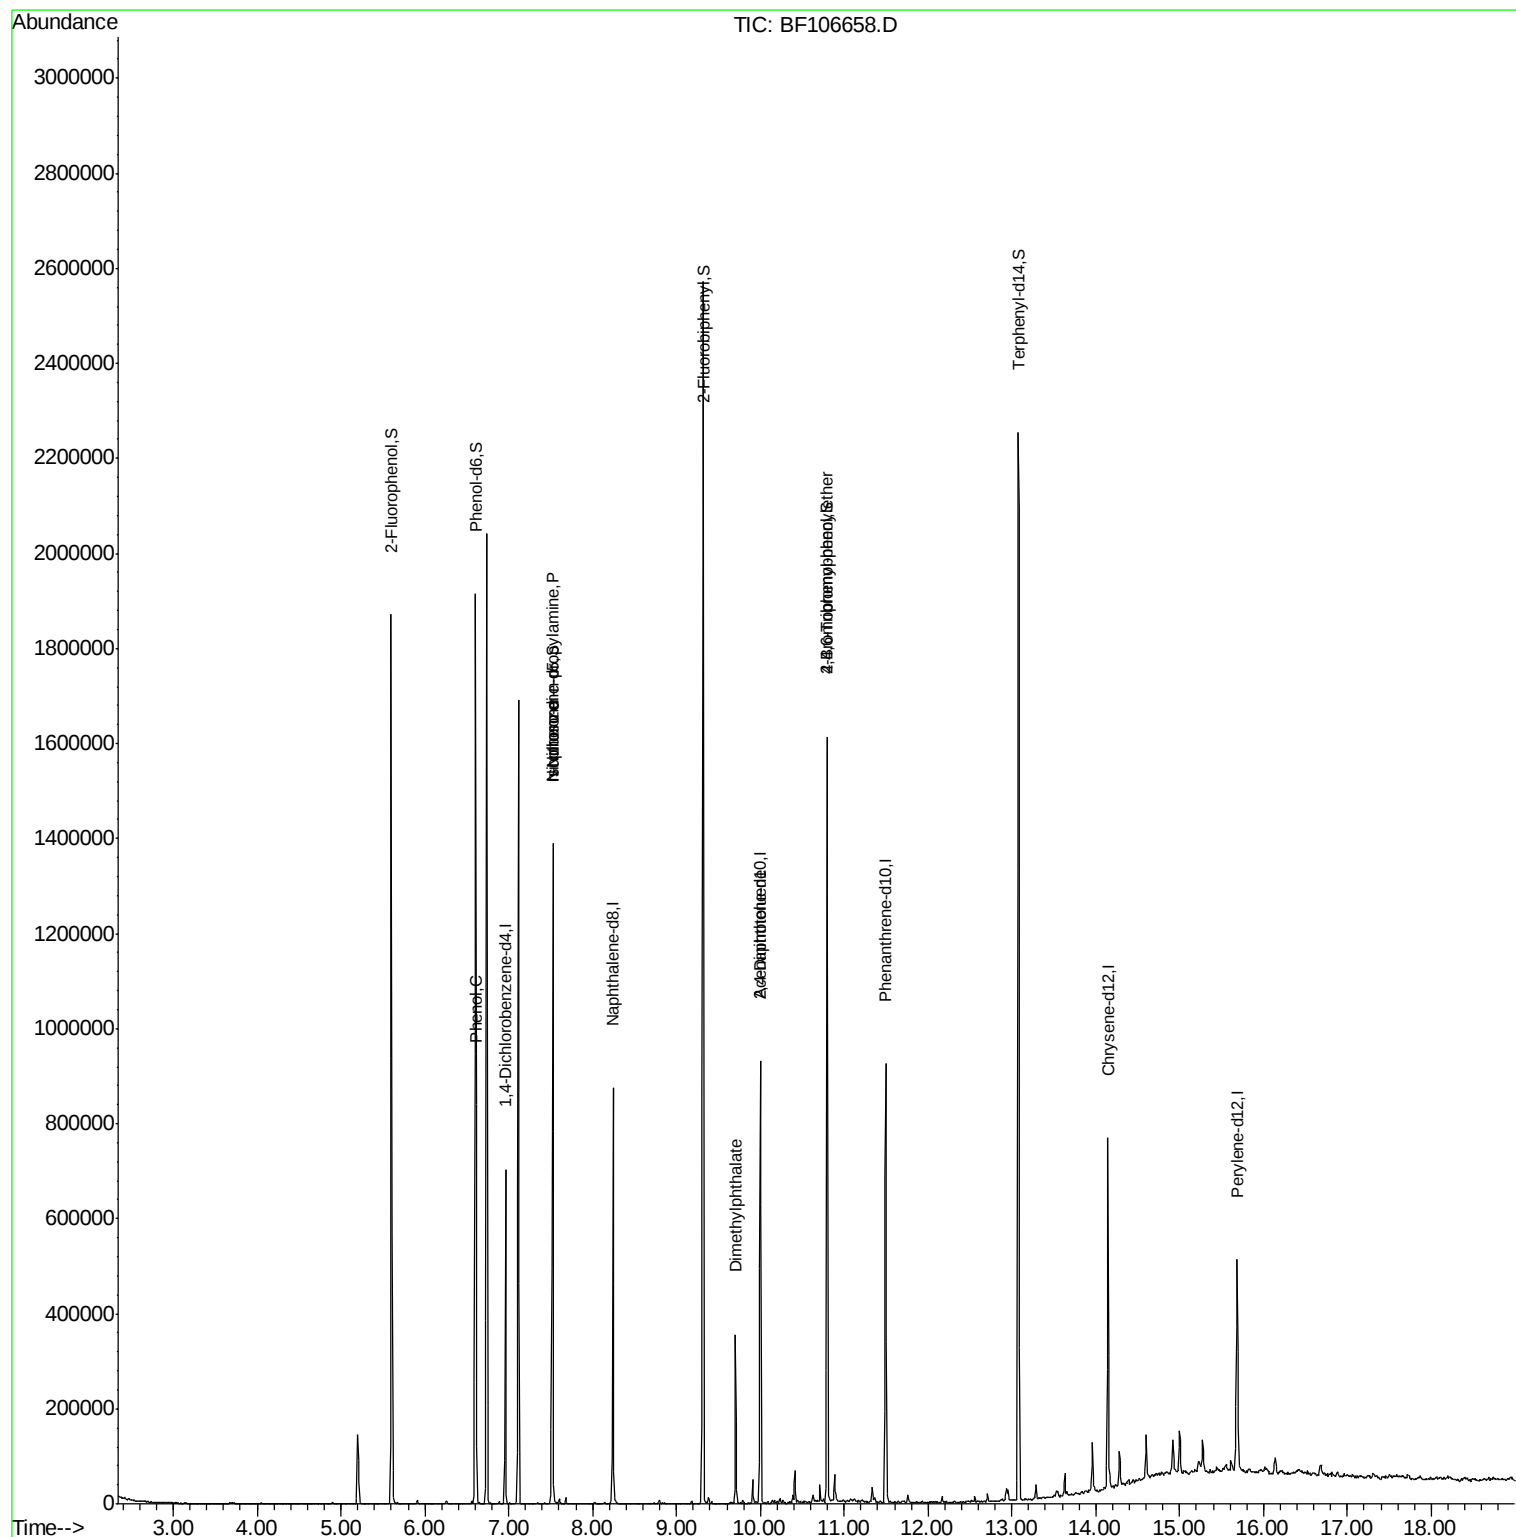

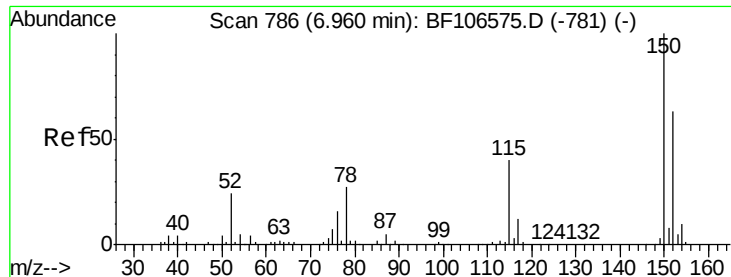


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.96 min Scan# 786
Delta R.T. 0.00 min
Lab File: BF106658.D
Acq: 21 Jun 2018 13:39

Instrument :
BNA_F
ClientSampleId :
TP-12-D

Tgt Ion:152 Resp: 93049
Ion Ratio Lower Upper
152 100
150 153.8 124.6 186.8
115 58.5 50.1 75.1

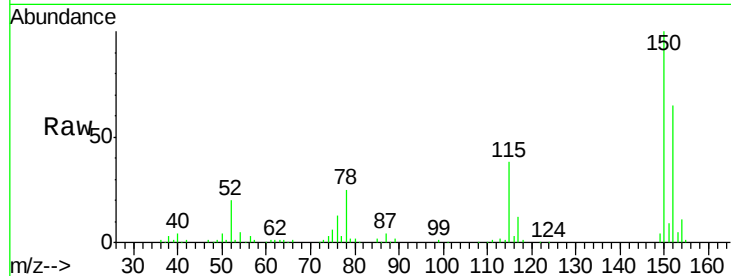


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

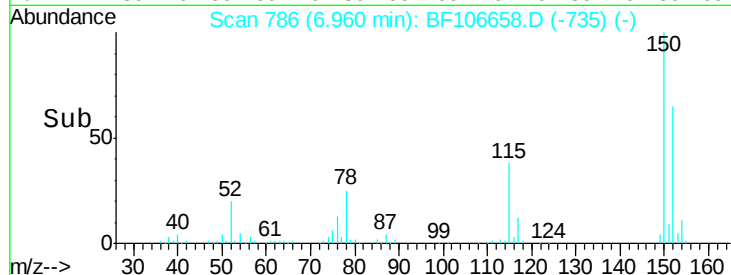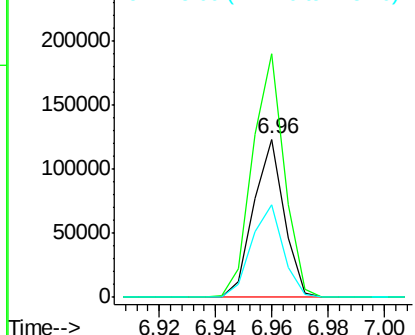



#5

2-Fluorophenol
Concen: 102.212 ng
RT: 5.61 min Scan# 556
Delta R.T. 0.01 min
Lab File: BF106658.D
Acq: 21 Jun 2018 13:39

Tgt Ion:112 Resp: 561662
Ion Ratio Lower Upper
112 100
64 56.8 47.9 71.9
63 28.8 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

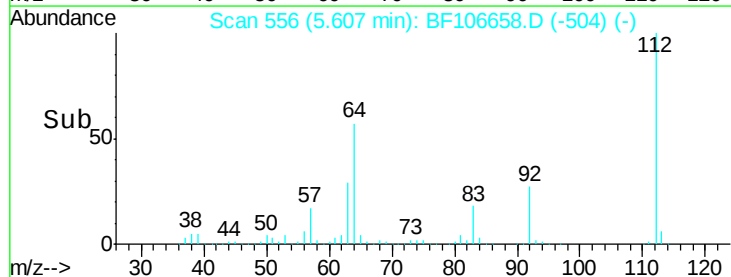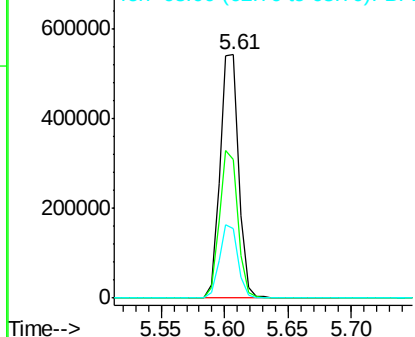



#7

Phenol-d6

Concen: 105.639 ng

RT: 6.61 min Scan# 726

Delta R.T. 0.00 min

Lab File: BF106658.D

Acq: 21 Jun 2018 13:39

Instrument :

BNA_F

ClientSampleId :

TP-12-D


Tgt Ion: 99 Resp: 724922

Ion Ratio Lower Upper

99 100

42 16.7 14.5 21.7




71 34.2 25.4 38.0

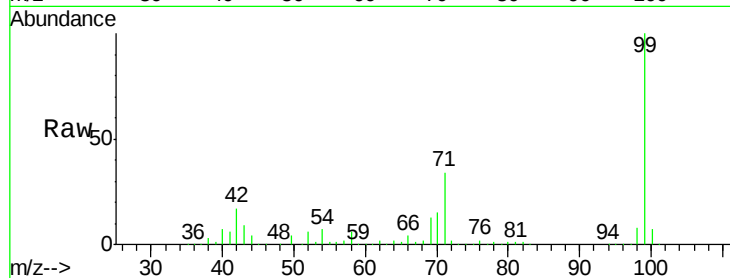

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

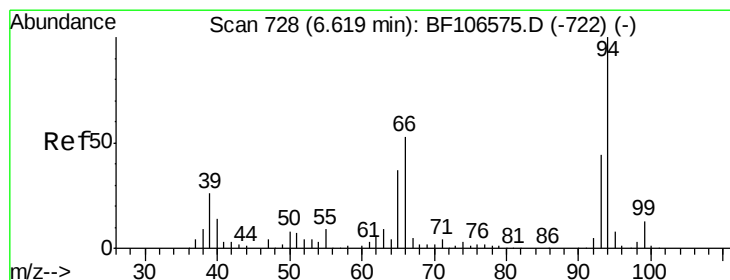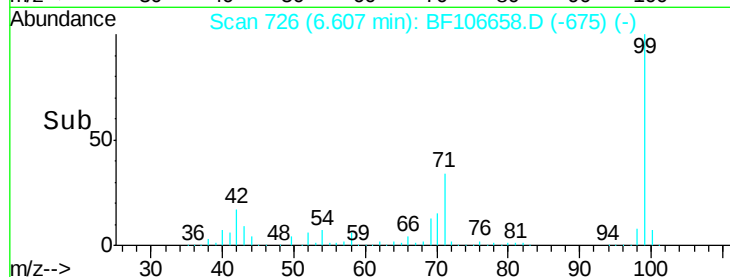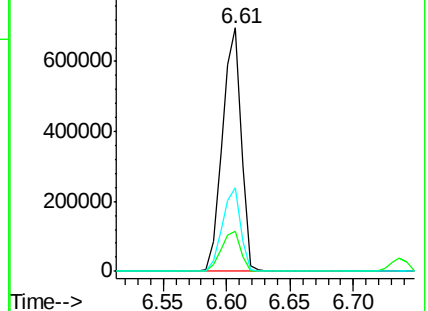

#10

Phenol

Concen: 2.305 ng

RT: 6.62 min Scan# 728

Delta R.T. -0.00 min

Lab File: BF106658.D

Acq: 21 Jun 2018 13:39


Tgt Ion: 94 Resp: 18054

Ion Ratio Lower Upper

94 100

65 28.2 7.9 47.9



66 36.7 16.2 56.2

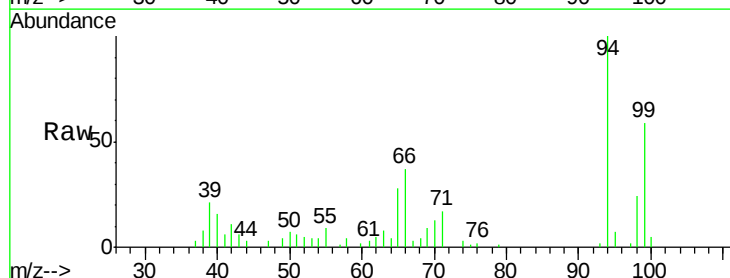

Abundance Ion 94.00 (93.70 to 94.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

Ion 66.00 (65.70 to 66.70): BF1



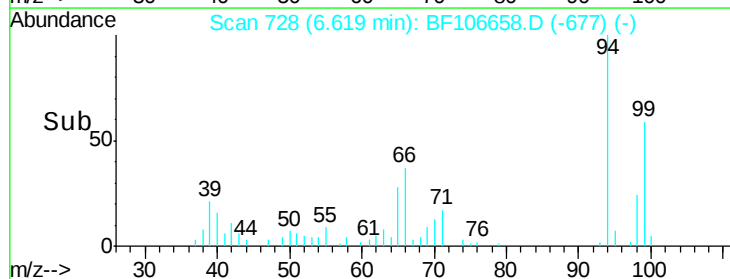
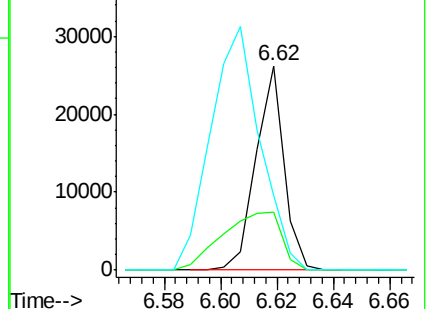




#19
n-Nitroso-di-n-propylamine
Concen: 13.893 ng
RT: 7.52 min Scan# 882
Delta R.T. 0.15 min
Lab File: BF106658.D
Acq: 21 Jun 2018 13:39




Instrument :
BNA_F
ClientSampled :
TP-12-D


Tgt Ion: 70 Resp: 62844
Ion Ratio Lower Upper
70 100
42 44.4 47.5 71.3#
101 0.0 7.4 11.2#
130 1.9 16.6 25.0#

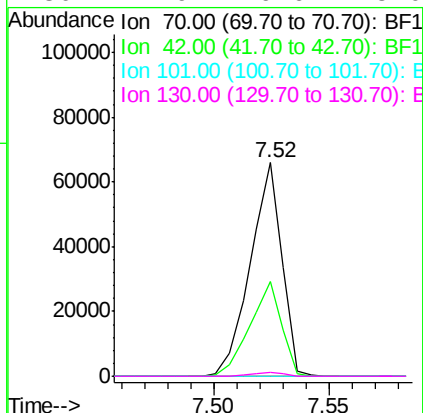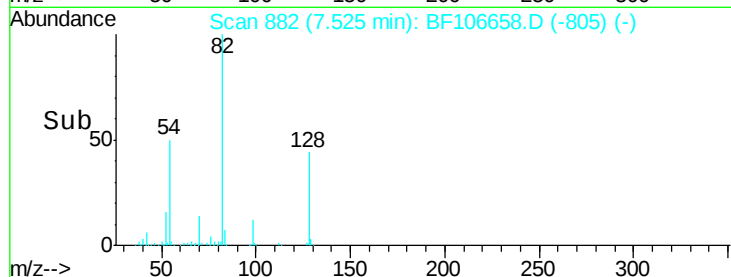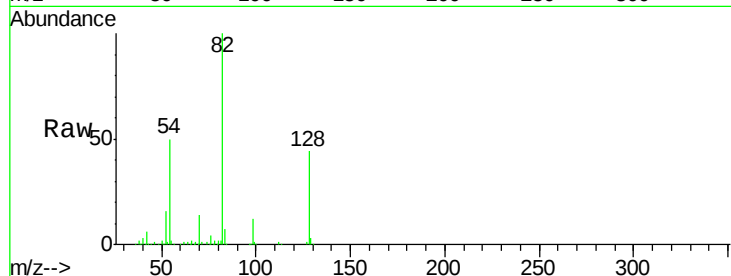

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.24 min Scan# 1004
Delta R.T. -0.01 min
Lab File: BF106658.D
Acq: 21 Jun 2018 13:39

Tgt Ion: 136 Resp: 362747
Ion Ratio Lower Upper
136 100
137 10.8 8.9 13.3
54 8.6 6.6 9.8
68 6.7 5.0 7.4

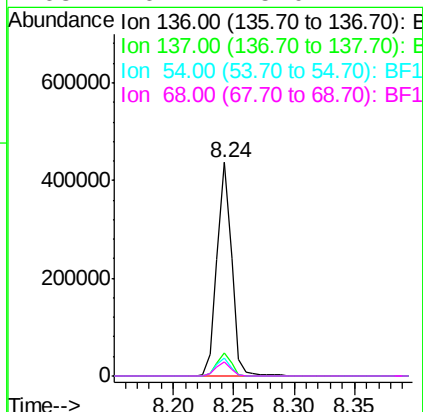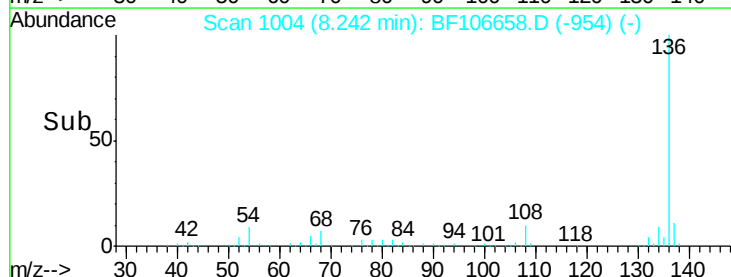

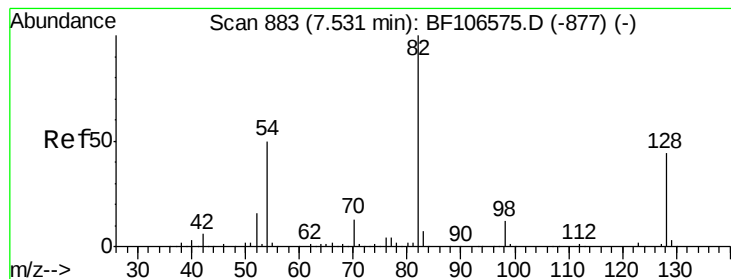

#23

Nitrobenzene-d5

Concen: 73.818 ng

RT: 7.52 min Scan# 882

Delta R.T. -0.01 min

Lab File: BF106658.D

Acq: 21 Jun 2018 13:39

Instrument :

BNA_F

ClientSampleId :

TP-12-D


Tgt Ion: 82 Resp: 481832

Ion Ratio Lower Upper

82 100

128 44.4 36.1 54.1




54 49.6 41.4 62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

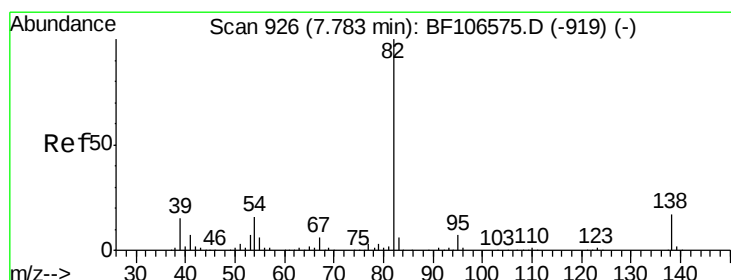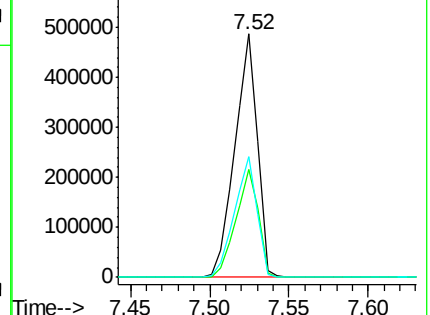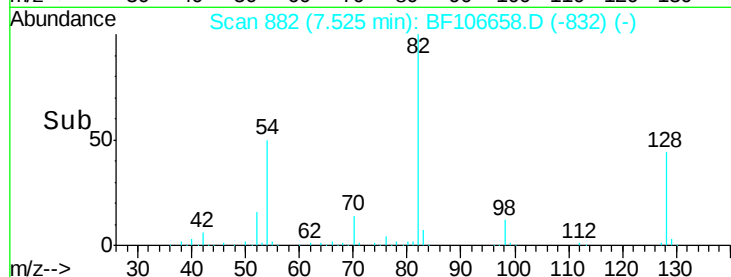

#25

Isophorone

Concen: 41.890 ng

RT: 7.52 min Scan# 882

Delta R.T. -0.26 min

Lab File: BF106658.D

Acq: 21 Jun 2018 13:39


Tgt Ion: 82 Resp: 481826

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#



138 0.0 14.9 22.3#




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

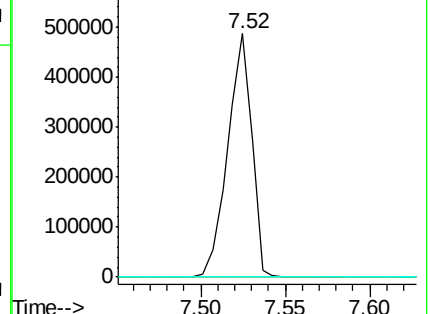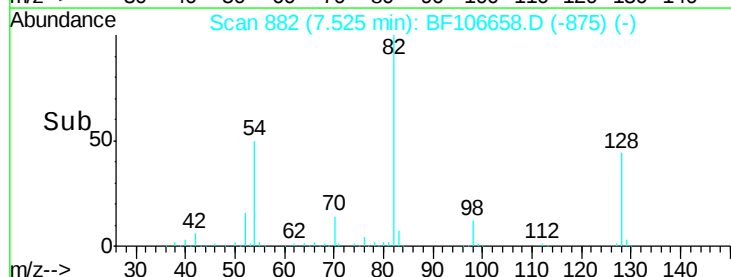

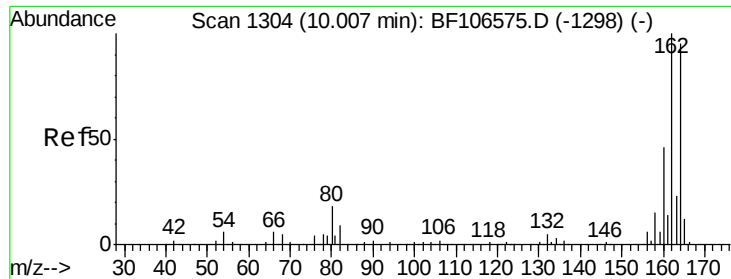

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.00 min Scan# 1303

Delta R.T. -0.01 min

Lab File: BF106658.D

Acq: 21 Jun 2018 13:39

Instrument :

BNA_F

ClientSampleId :

TP-12-D


Tgt Ion:164 Resp: 181351

Ion Ratio Lower Upper

164 100

162 97.7 86.1 129.1




160 44.7 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

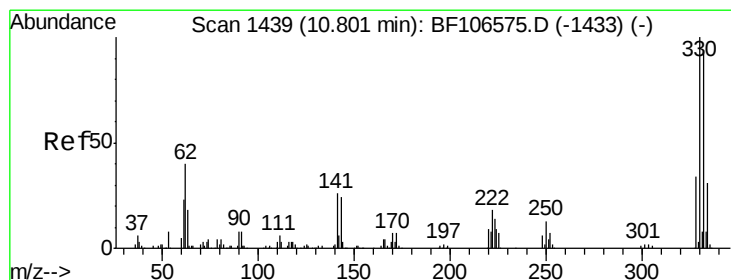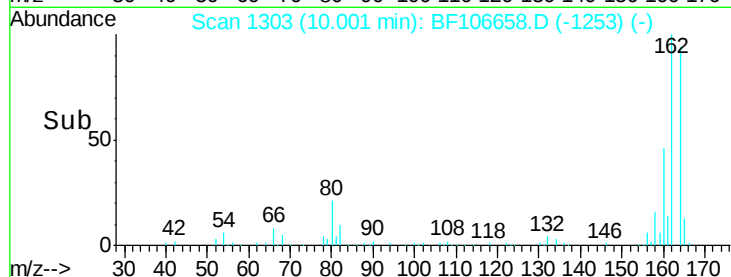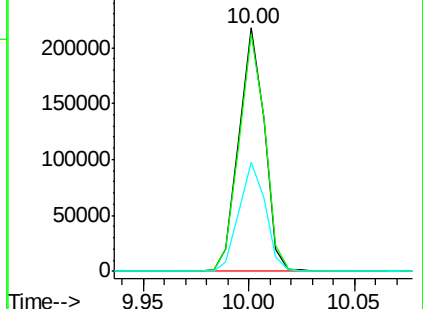

#41

2,4,6-Tribromophenol

Concen: 111.027 ng

RT: 10.79 min Scan# 1438

Delta R.T. -0.01 min

Lab File: BF106658.D

Acq: 21 Jun 2018 13:39


Tgt Ion:330 Resp: 233368

Ion Ratio Lower Upper

330 100

332 95.9 77.0 115.6



141 23.8 29.9 44.9#



Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

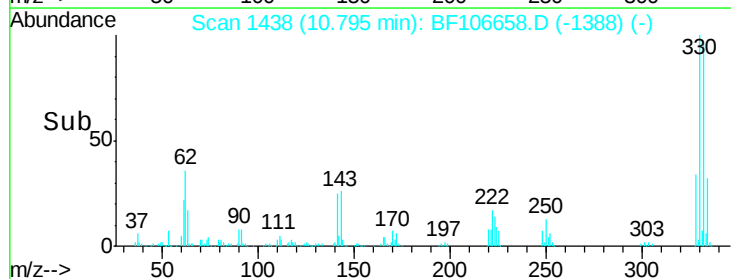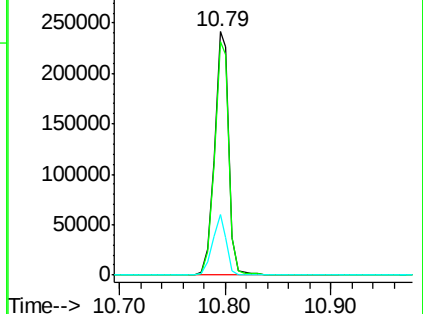







#44
2-Fluorobiphenyl
Concen: 76.072 ng
RT: 9.32 min Scan# 1187
Delta R.T. -0.01 min
Lab File: BF106658.D
Acq: 21 Jun 2018 13:39

Instrument :
BNA_F
ClientSampleId :
TP-12-D

Tgt Ion:172 Resp: 831650
Ion Ratio Lower Upper
172 100
171 36.5 29.7 44.5
170 25.1 19.6 29.4

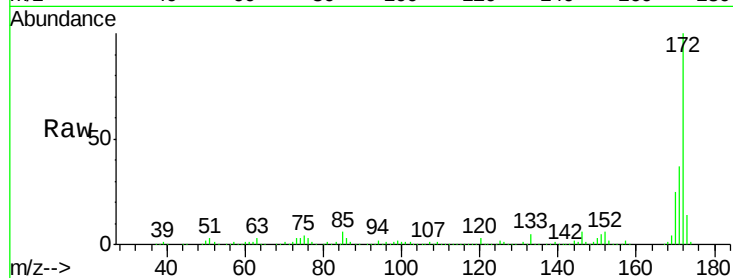


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

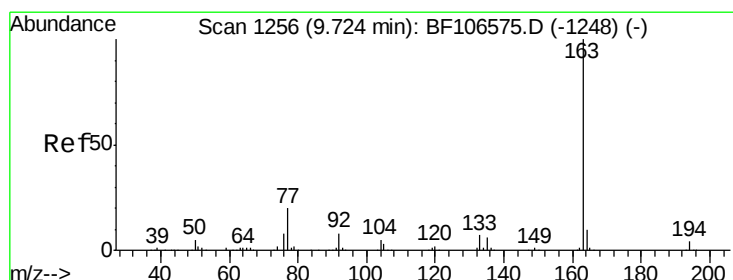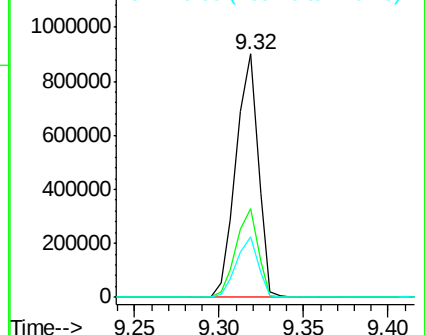
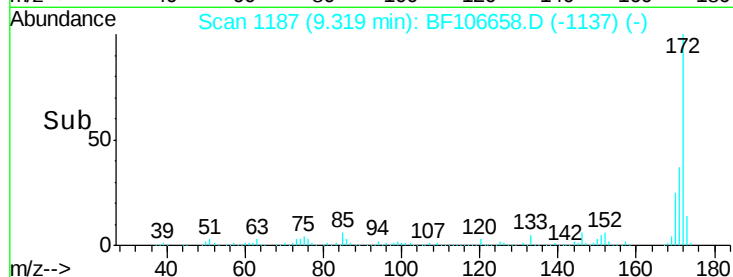


#49
Dimethylphthalate
Concen: 9.312 ng
RT: 9.71 min Scan# 1253
Delta R.T. -0.02 min
Lab File: BF106658.D
Acq: 21 Jun 2018 13:39

Tgt Ion:163 Resp: 126654
Ion Ratio Lower Upper
163 100
194 4.0 2.7 4.1
164 10.8 8.2 12.2

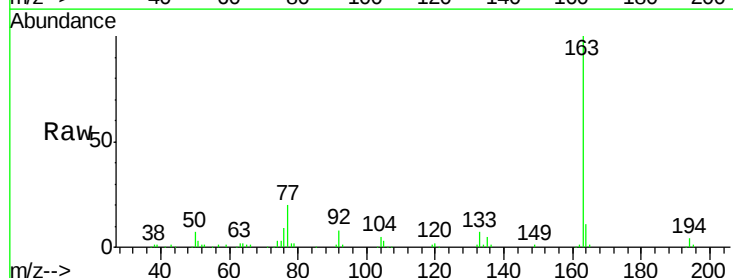

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E



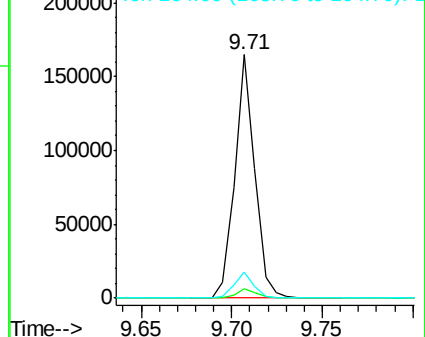
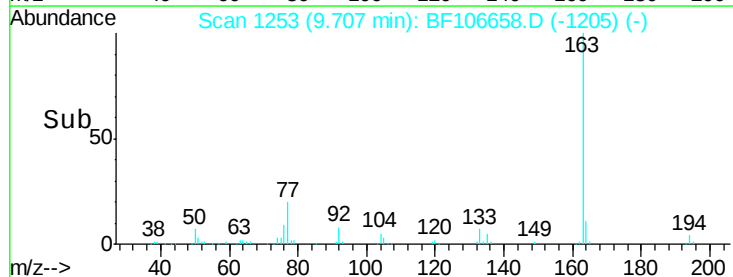




#56
2,4-Dinitrotoluene
Concen: 6.242 ng
RT: 10.00 min Scan# 1303
Delta R.T. -0.19 min
Lab File: BF106658.D
Acq: 21 Jun 2018 13:39




Instrument :
BNA_F
ClientSampleId :
TP-12-D


Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	36.4	54.6#
89	1.8	57.8	86.6#
182	0.0	1.6	2.4#

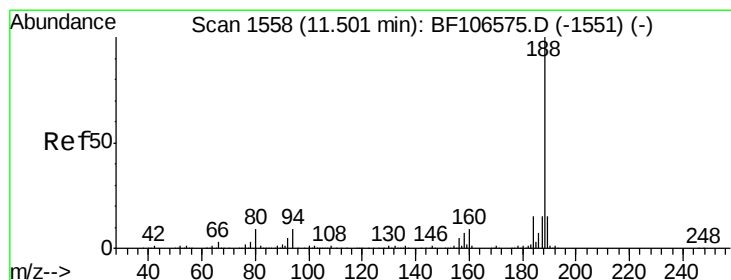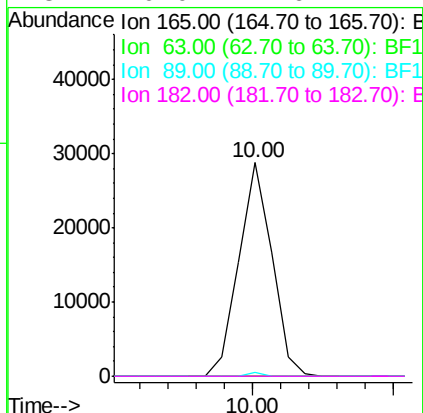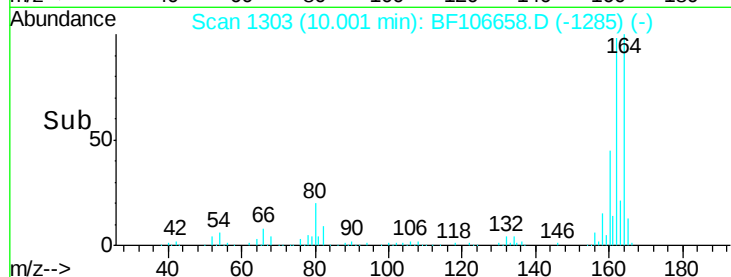

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.49 min Scan# 1557
Delta R.T. -0.01 min
Lab File: BF106658.D
Acq: 21 Jun 2018 13:39

Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.8	8.5	12.7
80	9.6	9.2	13.8

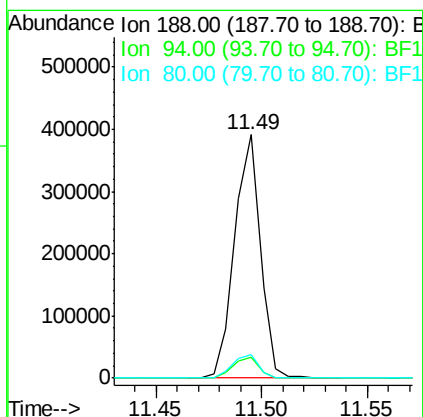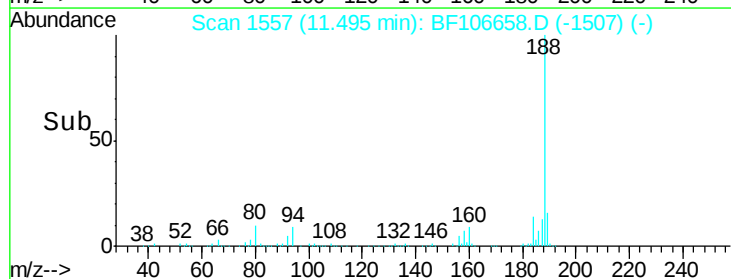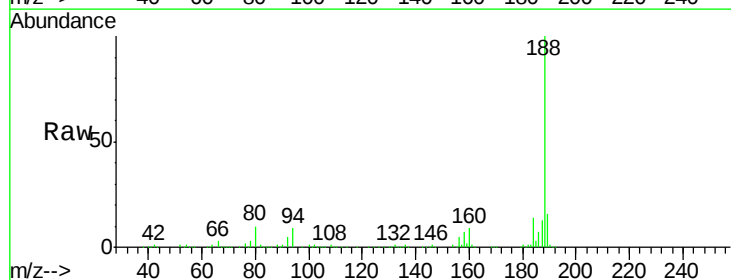


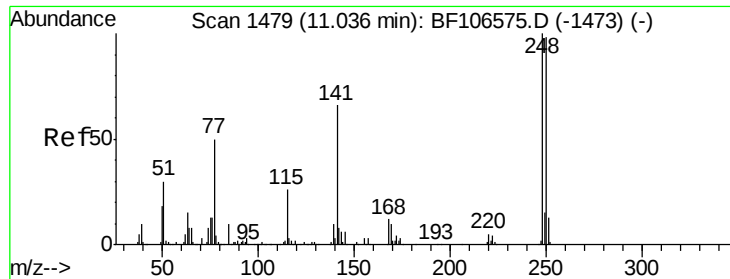




#66
4-Bromophenyl-phenylether
Concen: 3.678 ng
RT: 10.79 min Scan# 1438
Delta R.T. -0.24 min
Lab File: BF106658.D
Acq: 21 Jun 2018 13:39

Instrument :
BNA_F
ClientSampleId :
TP-12-D

Tgt Ion: 248 Resp: 14458
Ion Ratio Lower Upper
248 100
250 197.7 76.9 115.3#
141 371.8 74.4 111.6#

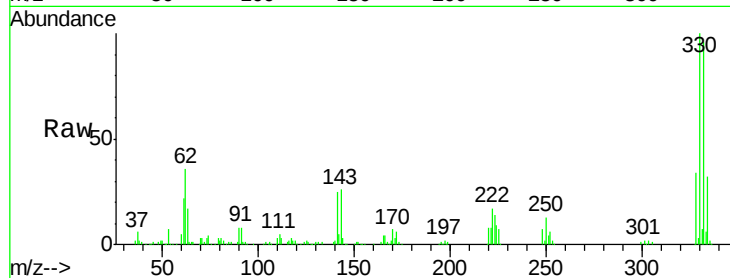


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

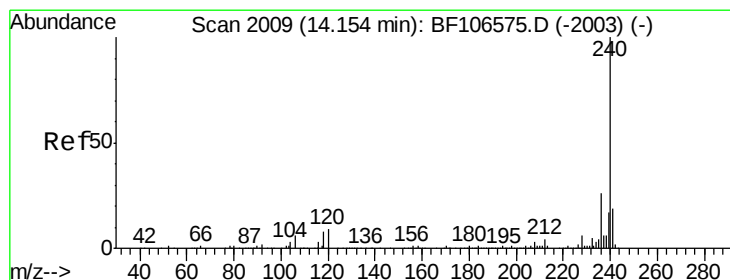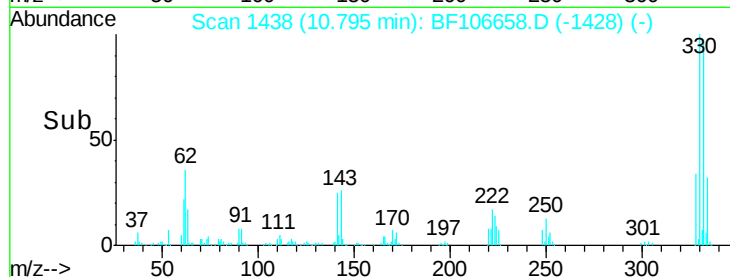
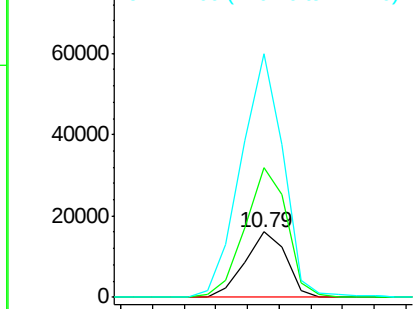


#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.15 min Scan# 2008
Delta R.T. -0.01 min
Lab File: BF106658.D
Acq: 21 Jun 2018 13:39

Tgt Ion: 240 Resp: 269134
Ion Ratio Lower Upper
240 100
120 8.7 9.5 14.3#
236 25.8 20.7 31.1

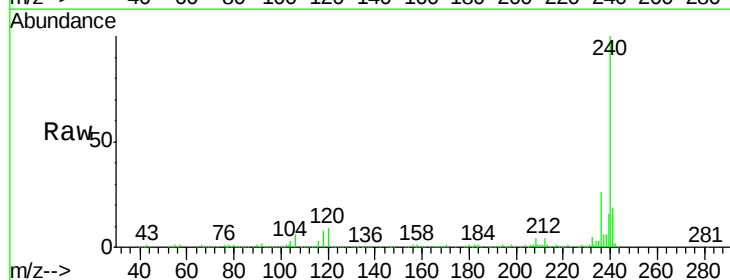

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

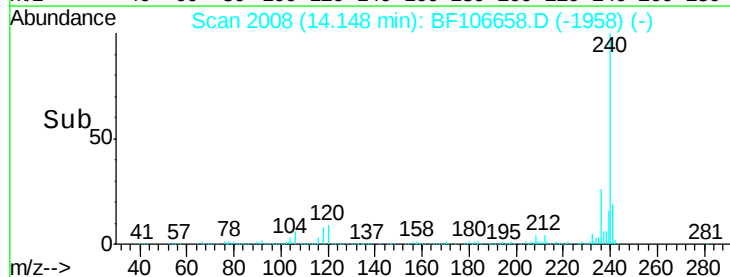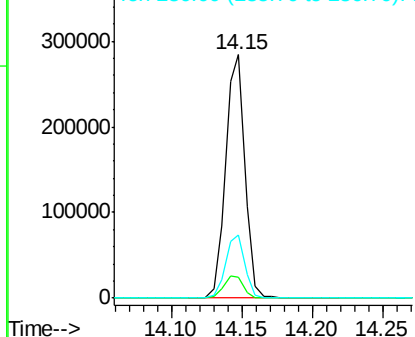







#78
 Terphenyl-d14
 Concen: 79.984 ng
 RT: 13.08 min Scan# 1826
 Delta R.T. -0.01 min
 Lab File: BF106658.D
 Acq: 21 Jun 2018 13:39

Instrument :
 BNA_F
 ClientSampleId :
 TP-12-D

Tgt Ion:244 Resp: 888678
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.4 8.0
 122 9.4 11.0 16.4#




Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

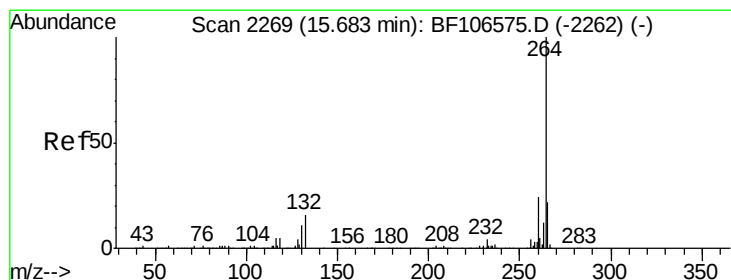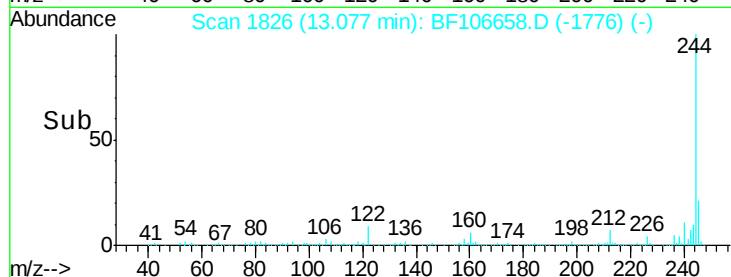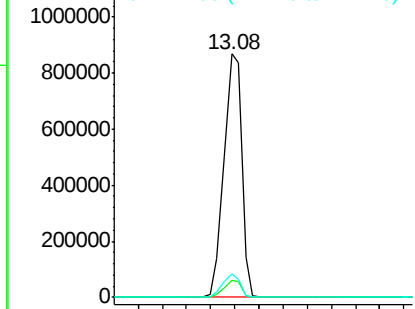

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.69 min Scan# 2270
 Delta R.T. 0.01 min
 Lab File: BF106658.D
 Acq: 21 Jun 2018 13:39

Tgt Ion:264 Resp: 210090
 Ion Ratio Lower Upper
 264 100
 260 24.2 19.2 28.8
 265 21.0 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

