


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF062118\  
 Data File : BF106650.D  
 Acq On : 21 Jun 2018 10:00  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061918.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jun 19 14:32:09 2018

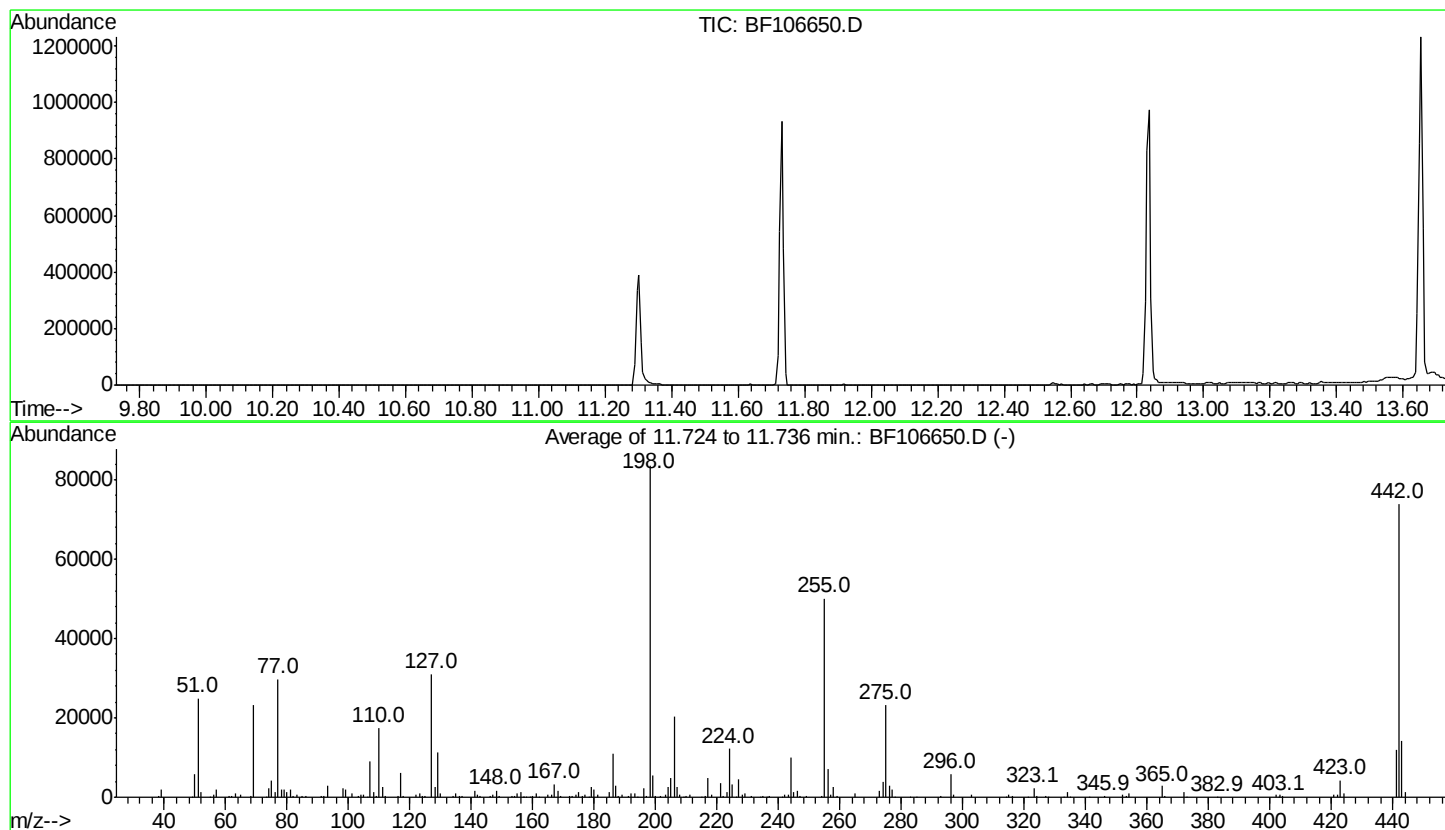

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 29.8         | 24908      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.4          | 320        | PASS                |
| 69             | 198             | 0.00            | 100             | 27.9         | 23352      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 37.2         | 31080      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 367        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 83565      | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 5648       | PASS                |
| 275            | 198             | 10              | 60              | 27.9         | 23274      | PASS                |
| 365            | 198             | 1               | 100             | 3.3          | 2789       | PASS                |
| 441            | 443             | 0.01            | 100             | 84.0         | 11840      | PASS                |
| 442            | 198             | 50              | 100             | 88.5         | 73954      | PASS                |
| 443            | 442             | 15              | 24              | 19.0         | 14087      | PASS                |