
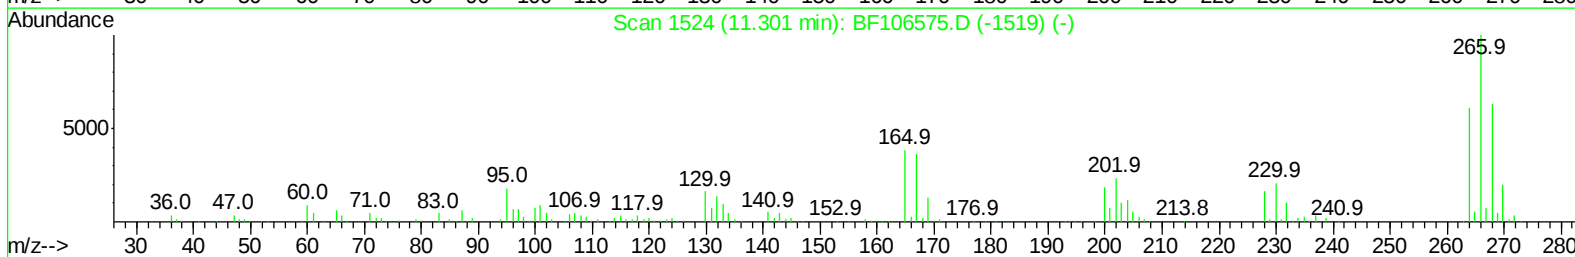
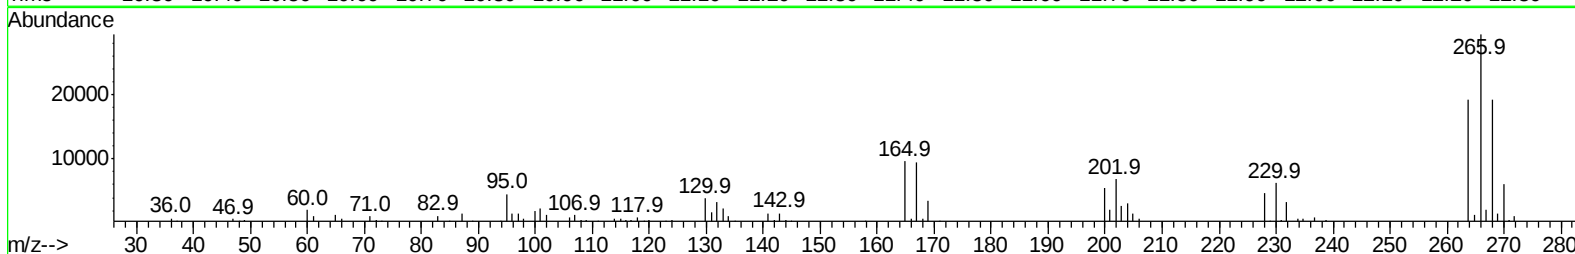


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062118\
Data File : BF106692.D
Acq On : 22 Jun 2018 5:20
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 09:22:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 19 14:32:09 2018
Response via : Initial Calibration

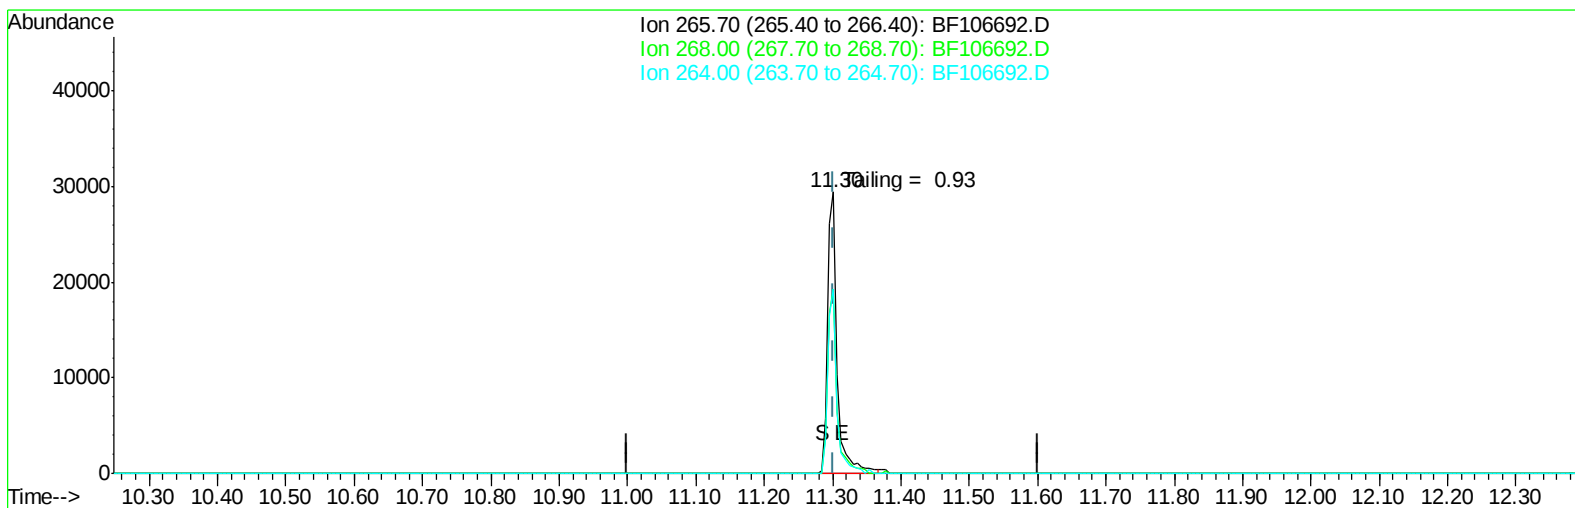

TIC: BF106692.D

(69) Pentachlorophenol (C)




11.301min (+0.000) 40173.92ng

response 29796

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.65
264.00	61.90	65.33
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062118\
Data File : BF106692.D
Acq On : 22 Jun 2018 5:20
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 09:22:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 19 14:32:09 2018
Response via : Initial Calibration

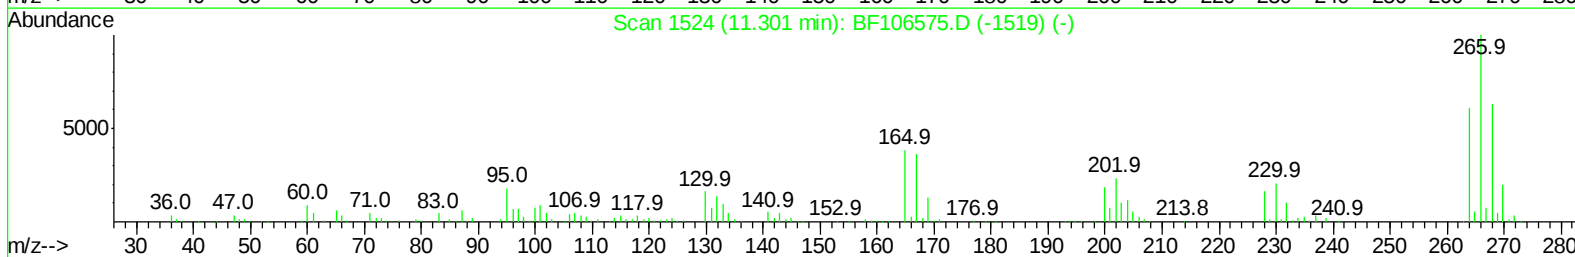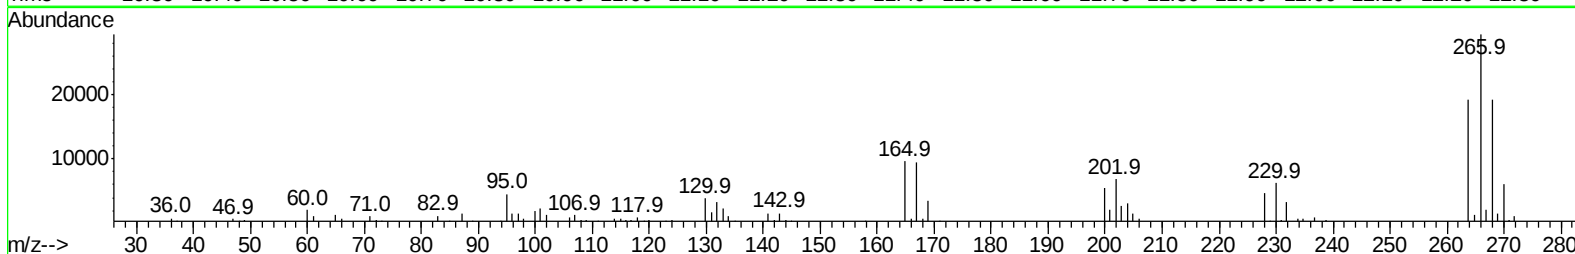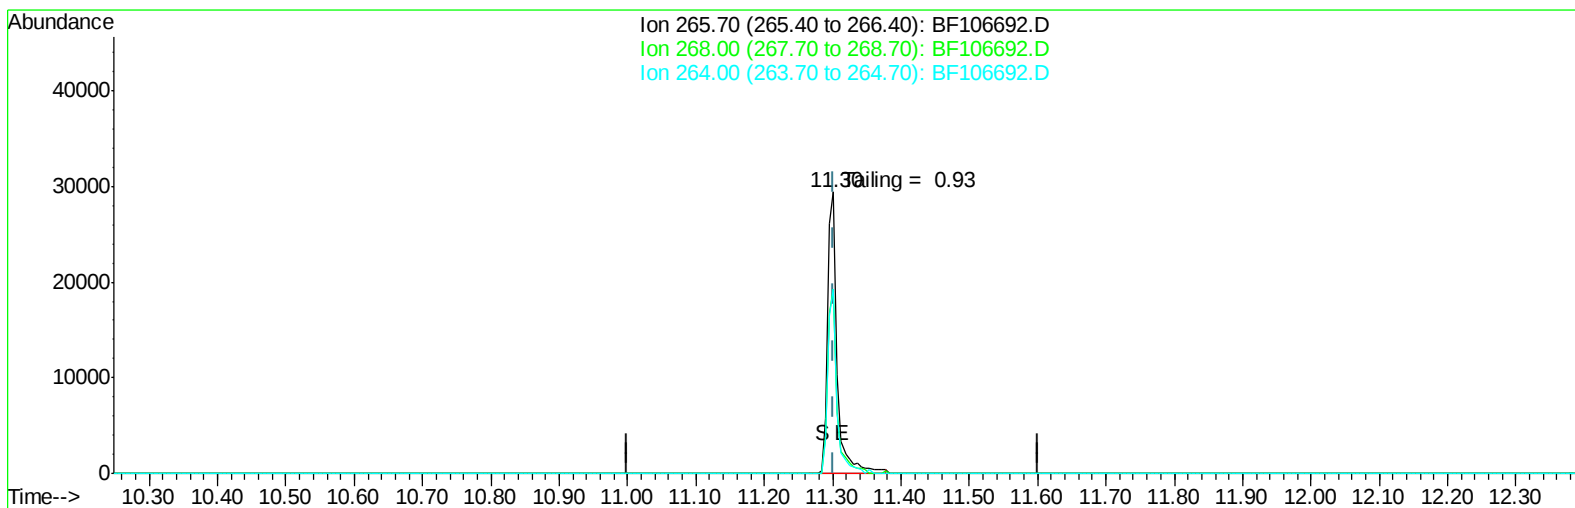

TIC: BF106692.D

(69) Pentachlorophenol (C)




11.301min (+0.000) 40173.92ng m

response 29796

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.65
264.00	61.90	65.33
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062118\
 Data File : BF106692.D
 Acq On : 22 Jun 2018 5:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 09:22:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 19 14:32:09 2018
 Response via : Initial Calibration

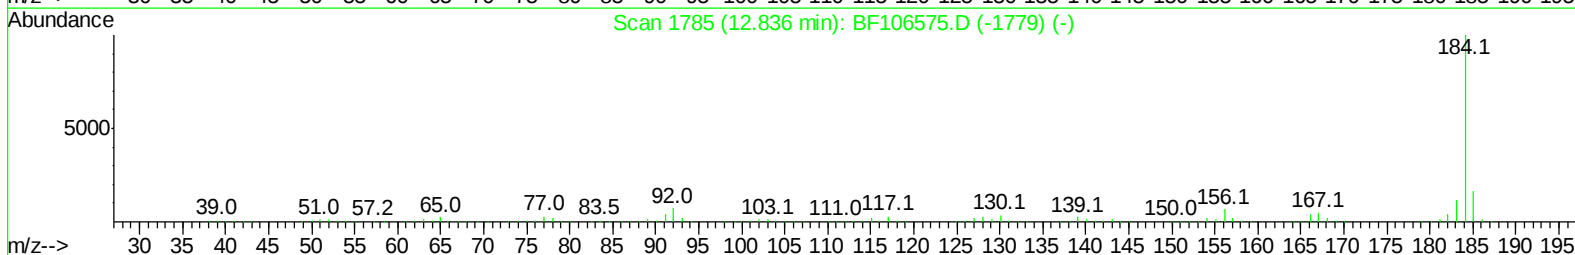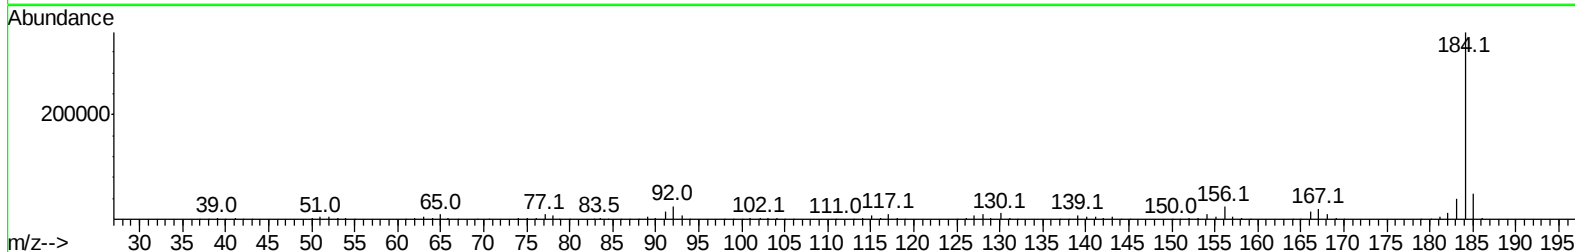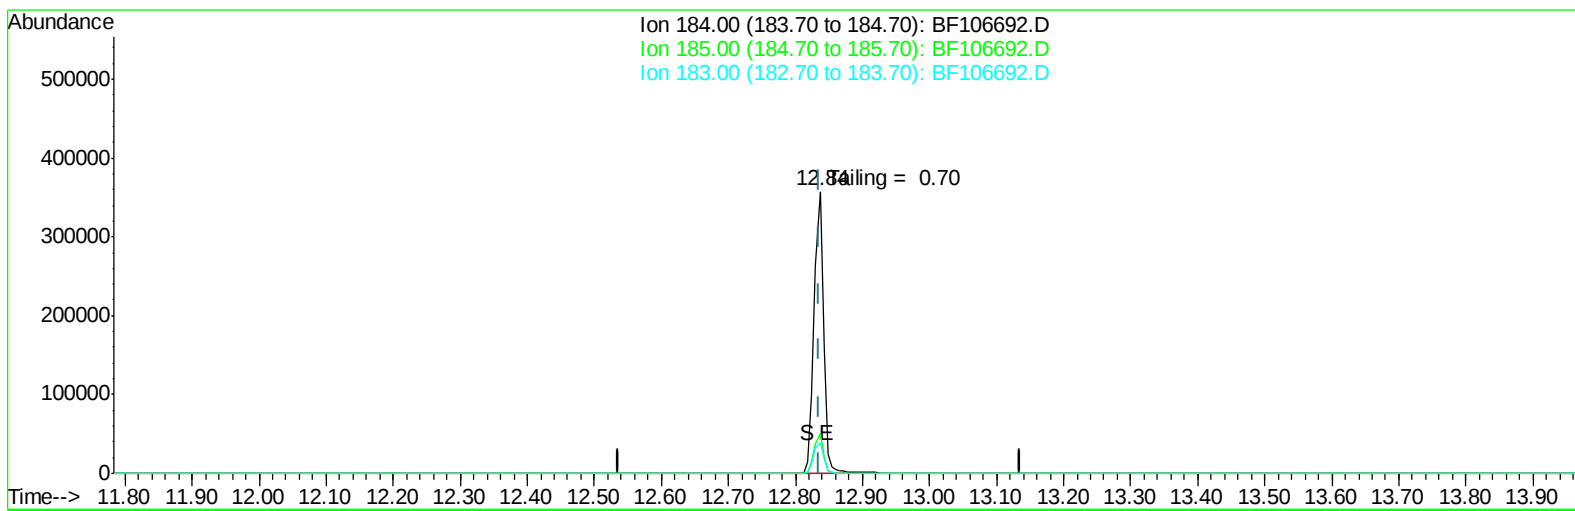

TIC: BF106692.D

(76) Benzidine

12.836min (+0.000) 0.00ng

response 336886

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.08
183.00	11.60	11.02
0.00	0.00	0.00