


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062118\
 Data File : BF106650.D
 Acq On : 21 Jun 2018 10:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 19 14:32:09 2018

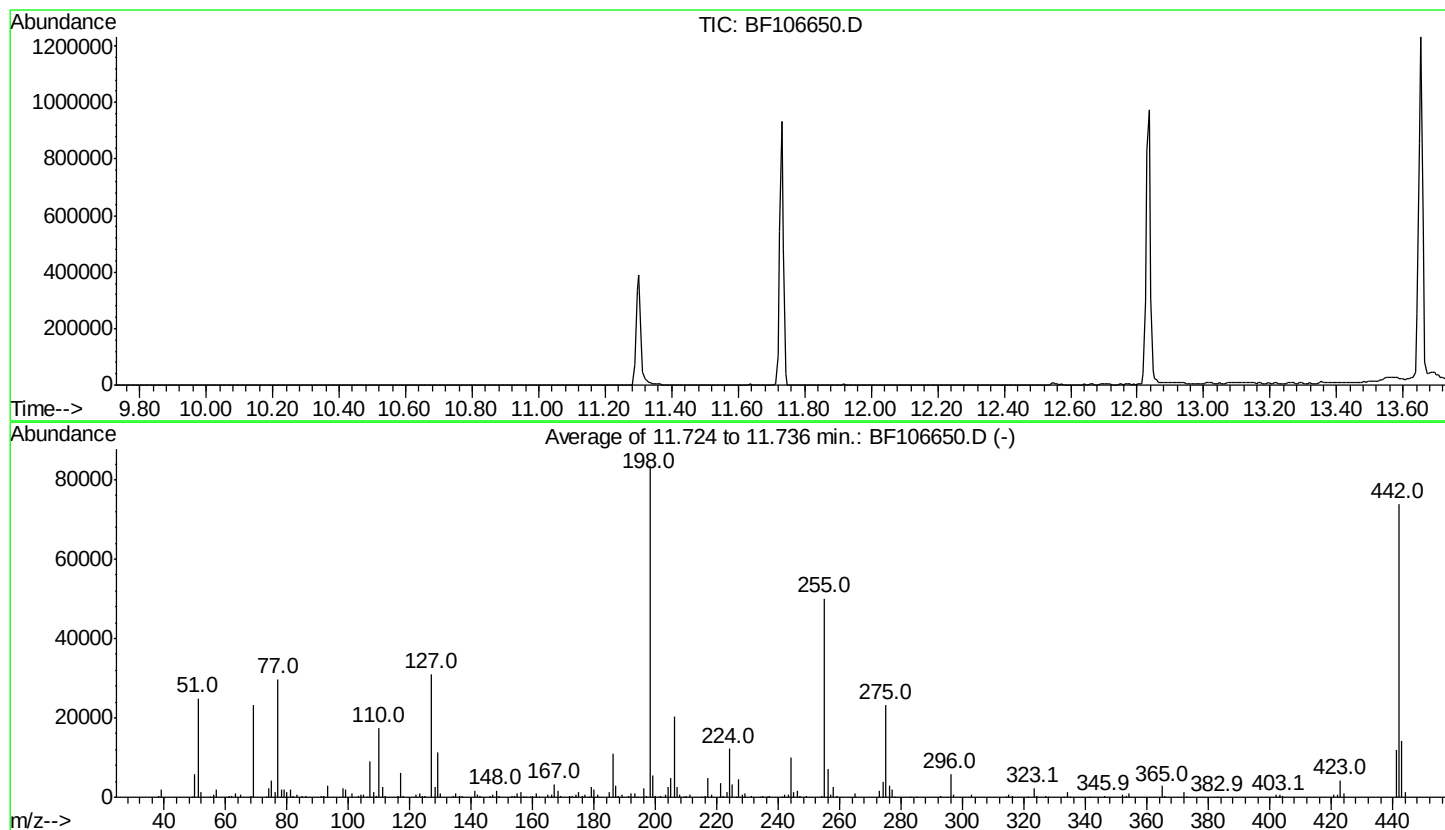

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	24908	PASS
68	69	0.00	2	1.4	320	PASS
69	198	0.00	100	27.9	23352	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.2	31080	PASS
197	198	0.00	2	0.4	367	PASS
198	198	100	100	100.0	83565	PASS
199	198	5	9	6.8	5648	PASS
275	198	10	60	27.9	23274	PASS
365	198	1	100	3.3	2789	PASS
441	443	0.01	100	84.0	11840	PASS
442	198	50	100	88.5	73954	PASS
443	442	15	24	19.0	14087	PASS