
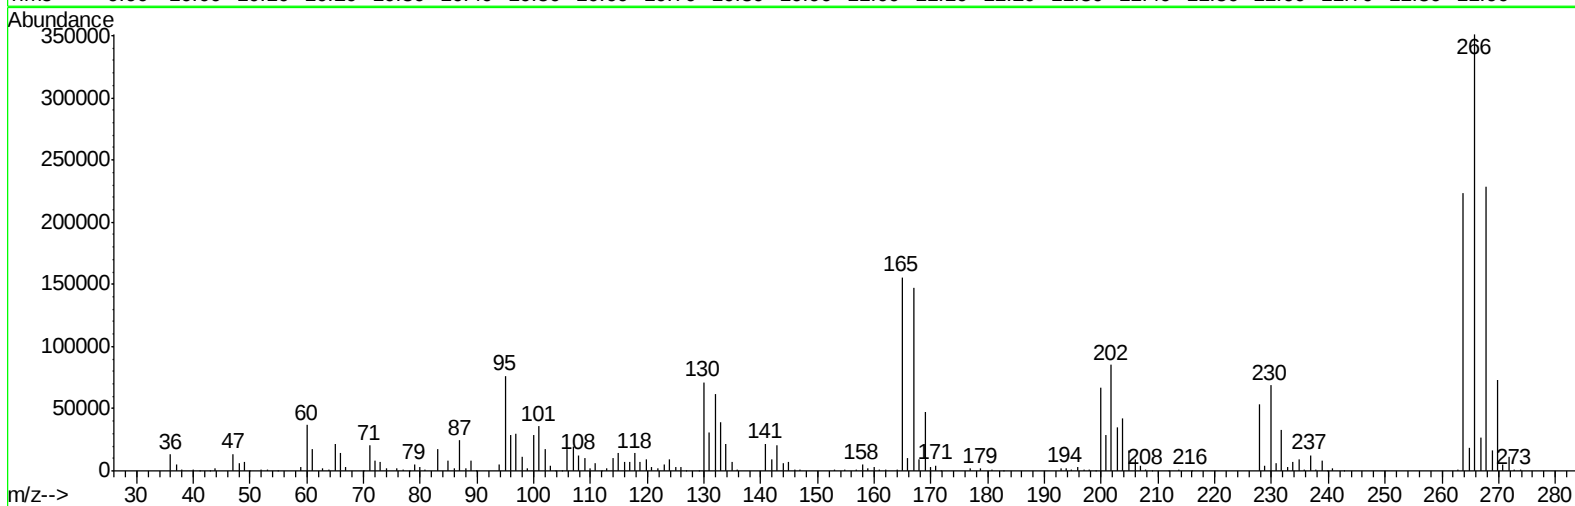


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062119\
Data File : BF115084.D
Acq On : 21 Jun 2019 18:11
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 09:53:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

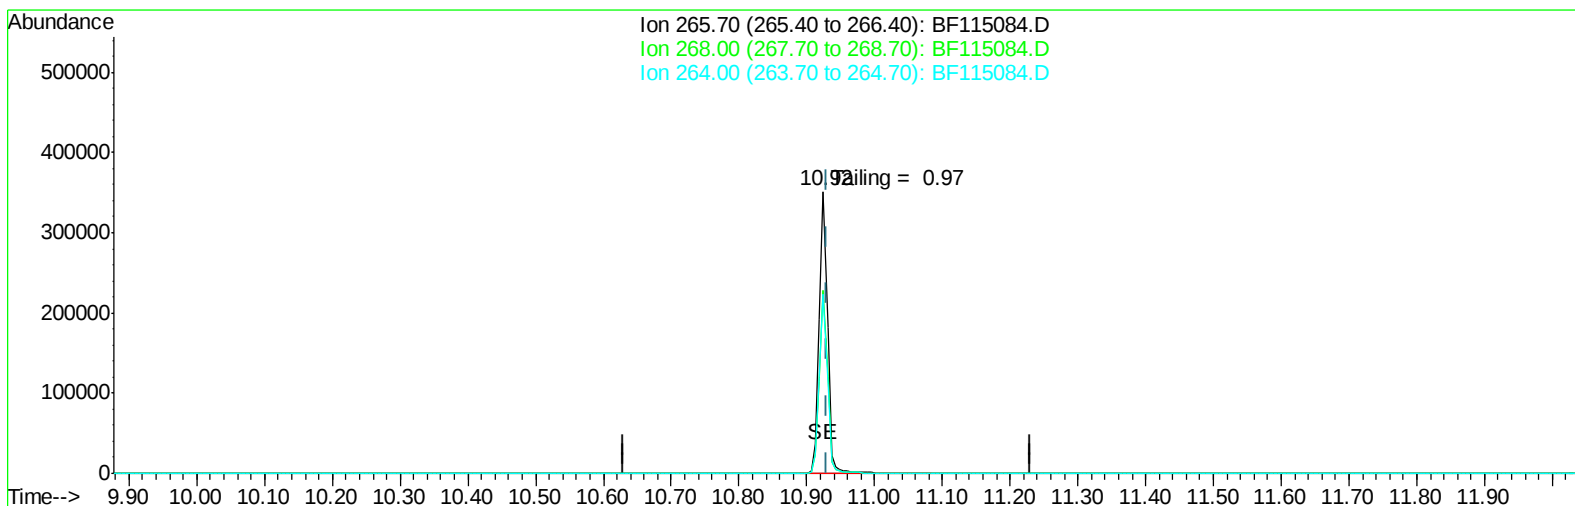

TIC: BF115084.D

(70) Pentachlorophenol (C)



11.019min (+0.088) 135.48ng m

response 581

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	53.23
264.00	61.60	56.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062119\
Data File : BF115084.D
Acq On : 21 Jun 2019 18:11
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 09:53:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

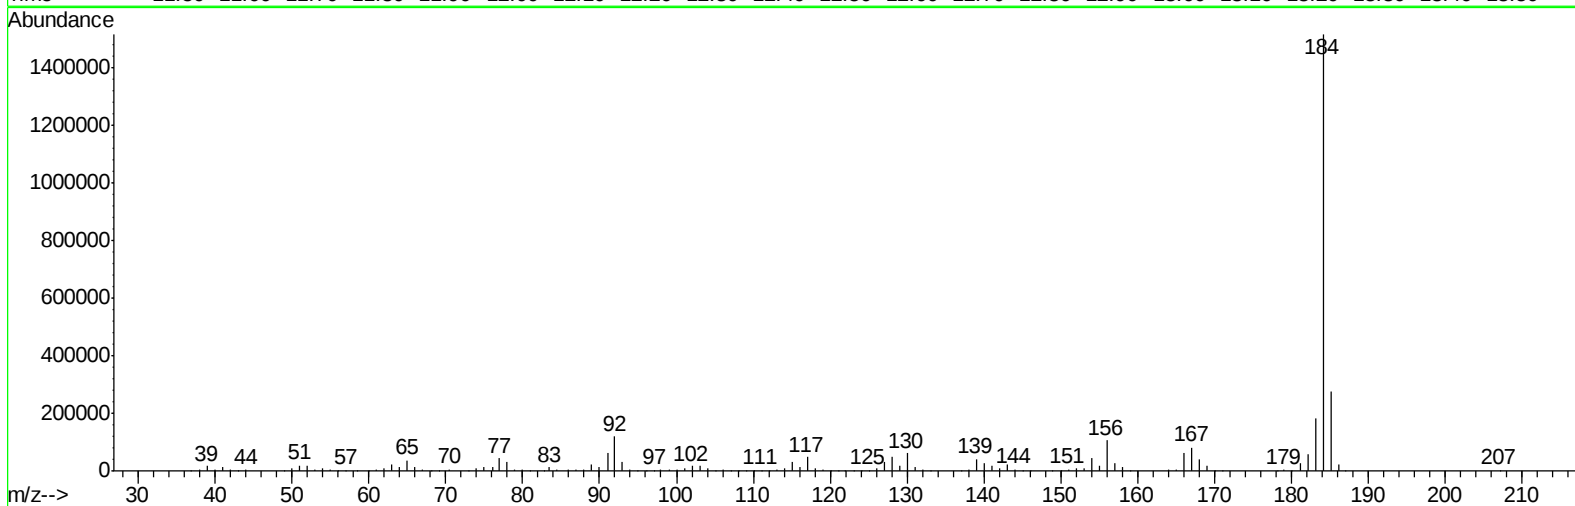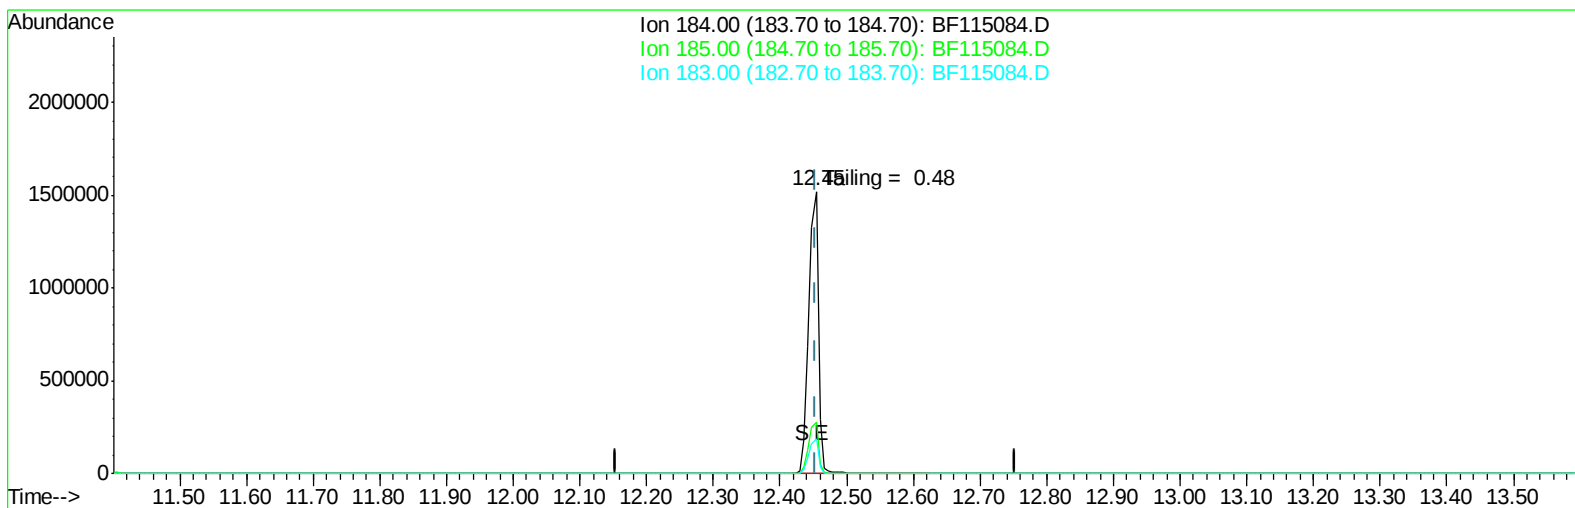

TIC: BF115084.D

(77) Benzidine

12.454min (+0.000) 73251.24ng

response 1450681

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	18.20
183.00	12.00	12.07
0.00	0.00	0.00