
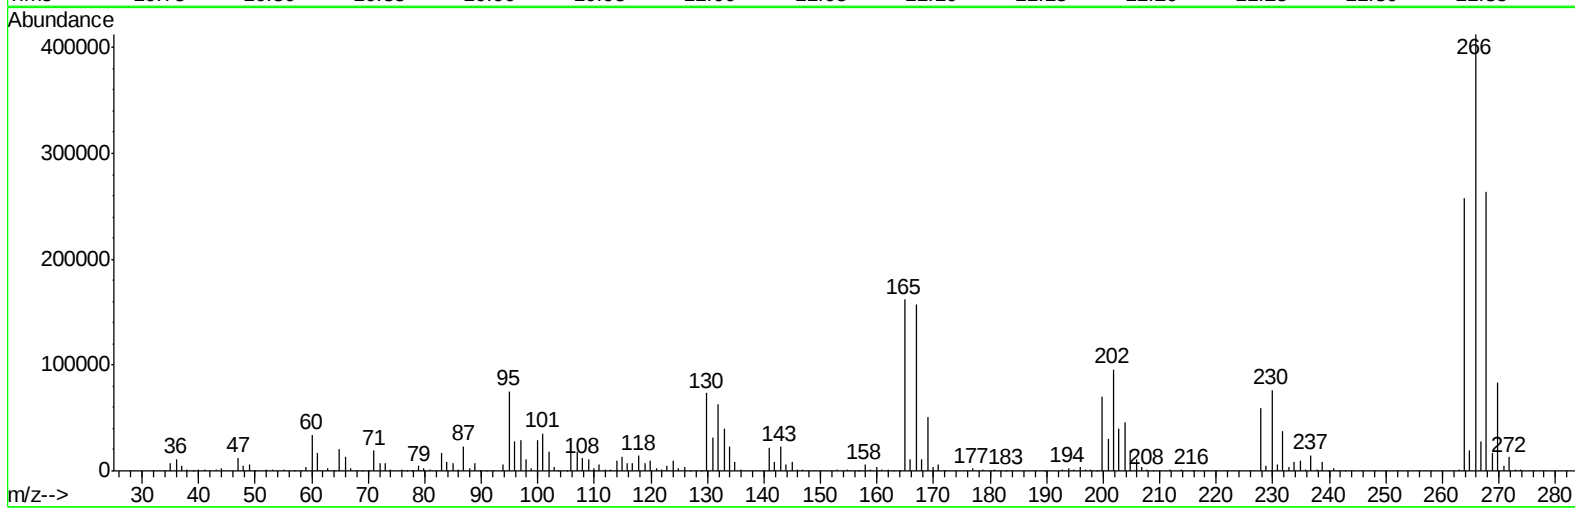


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062119\
Data File : BF115075.D
Acq On : 21 Jun 2019 13:19
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 06:51:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 21 17:55:32 2019
Response via : Initial Calibration

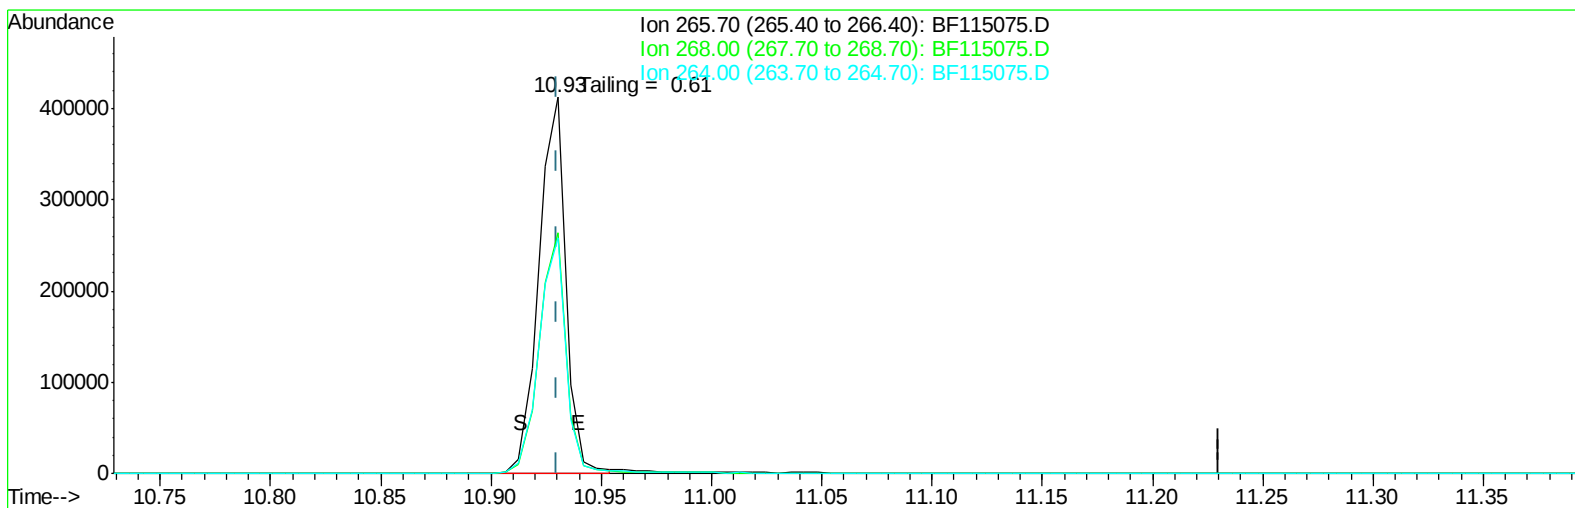

TIC: BF115075.D

(70) Pentachlorophenol (C)



10.930min (-0.000) 93231.76ng

response 362075

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	64.06
264.00	61.60	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062119\
Data File : BF115075.D
Acq On : 21 Jun 2019 13:19
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 22 06:51:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 21 17:55:32 2019
Response via : Initial Calibration

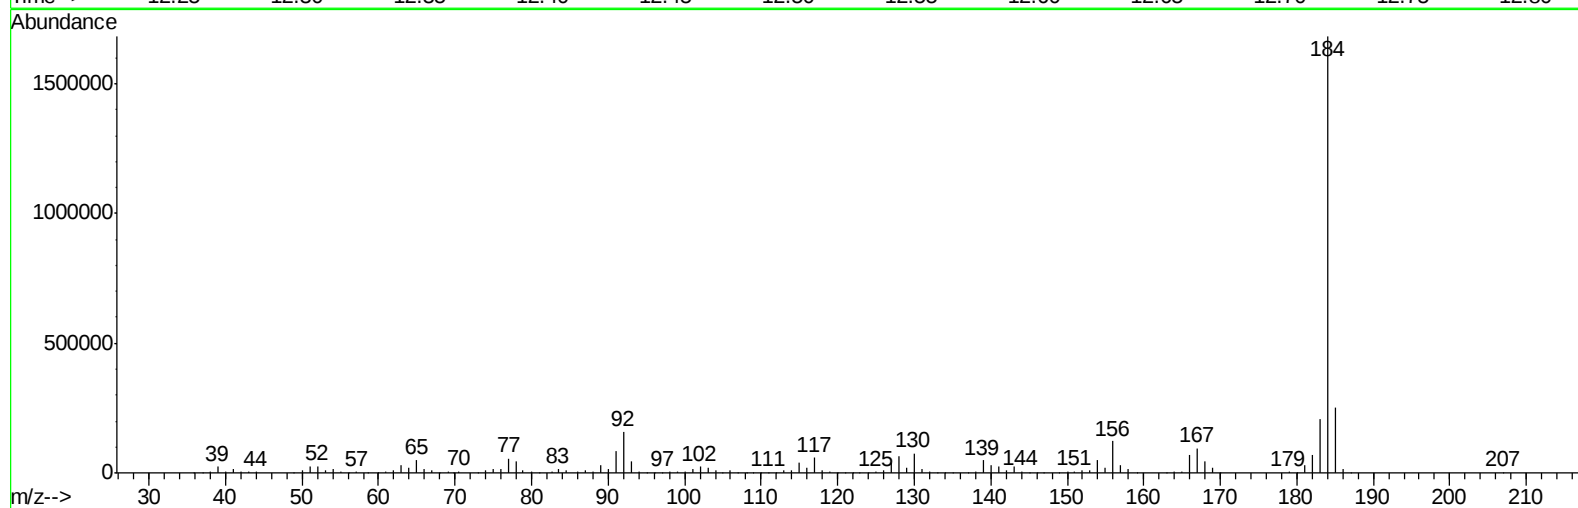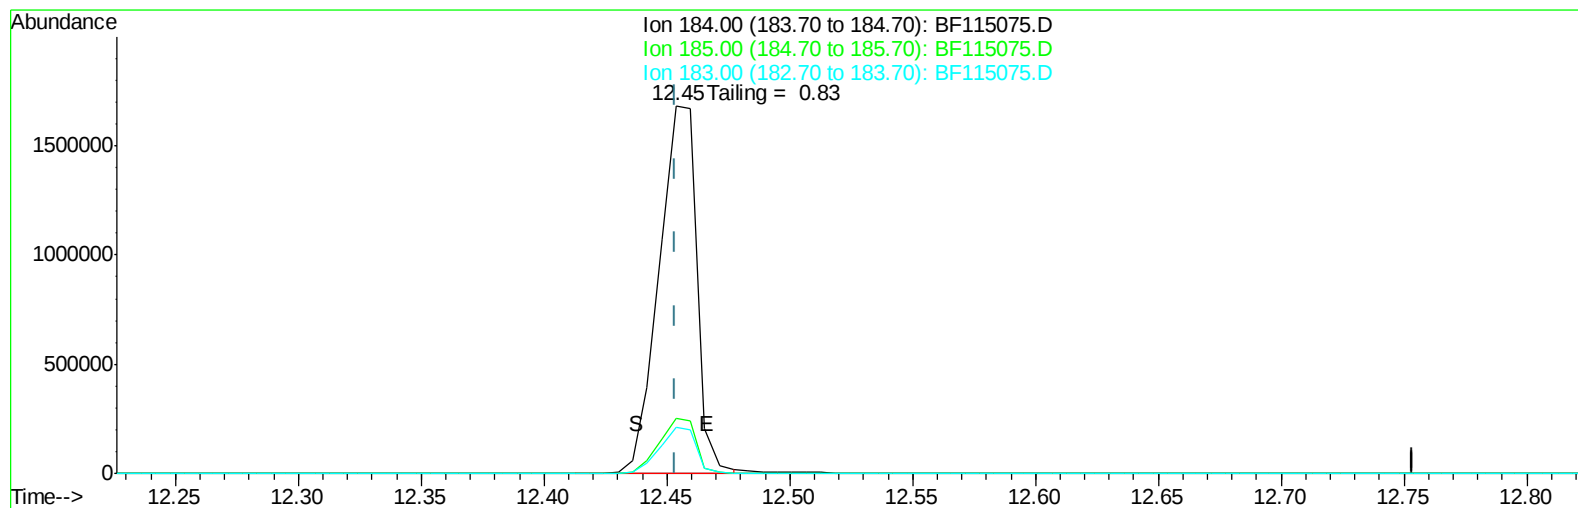

TIC: BF115075.D

(77) Benzidine

12.454min (-0.000) 109502.13ng

response 1828237

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.06
183.00	12.00	12.40
0.00	0.00	0.00