

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
 Data File : BF115100.D
 Acq On : 22 Jun 2019 1:24
 Operator : HP/JU
 Sample : PB120777BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120777BL

Quant Time: Jun 22 05:28:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 21 17:55:32 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.61	152	262718	20.00	ng	0.00
21) Naphthalene-d8	7.90	136	1014257	20.00	ng	0.00
39) Acenaphthene-d10	9.64	164	496153	20.00	ng	0.00
64) Phenanthrene-d10	11.11	188	999964	20.00	ng	0.00
76) Chrysene-d12	13.74	240	790999	20.00	ng	-0.01
87) Perylene-d12	15.10	264	823276	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.22	112	1872478	109.99	ng	0.01
7) Phenol-d6	6.25	99	2281464	110.41	ng	0.00
23) Nitrobenzene-d5	7.17	82	1407816	85.38	ng	-0.01
42) 2,4,6-Tribromophenol	10.42	330	633772	121.13	ng	0.00
45) 2-Fluorobiphenyl	8.98	172	2581484	88.38	ng	0.00
79) Terphenyl-d14	12.71	244	2906699	78.13	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115100.D
Acq On : 22 Jun 2019 1:24
Operator : HP/JU
Sample : PB120777BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120777BL

Quant Time: Jun 22 05:28:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 21 17:55:32 2019
Response via : Initial Calibration

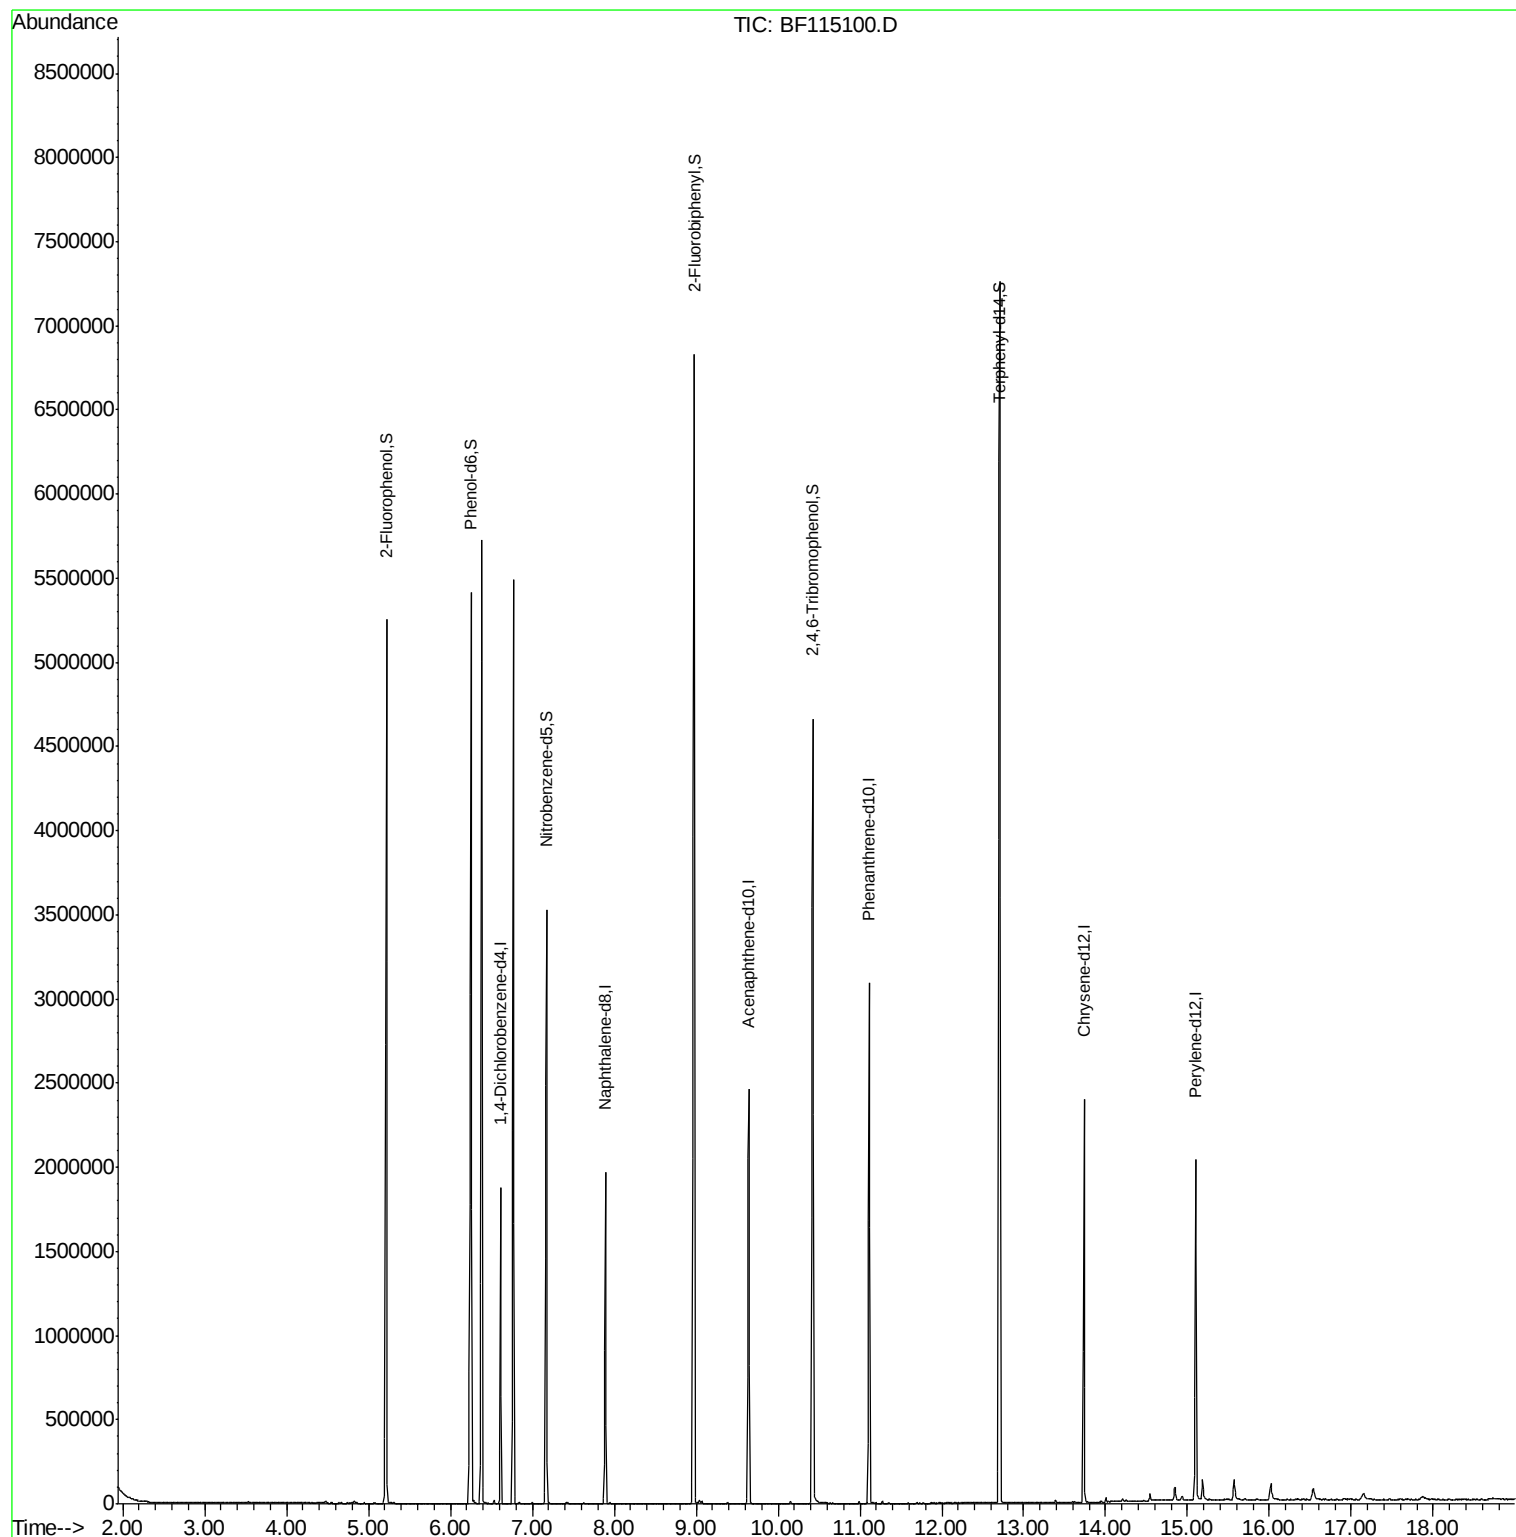

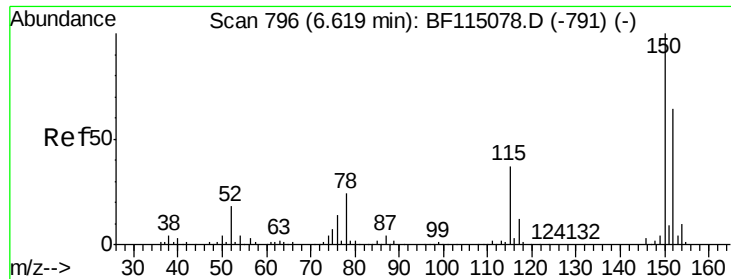


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.61 min Scan# 795
Delta R.T. -0.01 min
Lab File: BF115100.D
Acq: 22 Jun 2019 1:24

Instrument :
BNA_F
ClientSampleId :
PB120777BL

Tot Ion:152 Resp: 262718
Ion Ratio Lower Upper
152 100
150 156.7 124.2 186.2
115 58.0 46.1 69.1

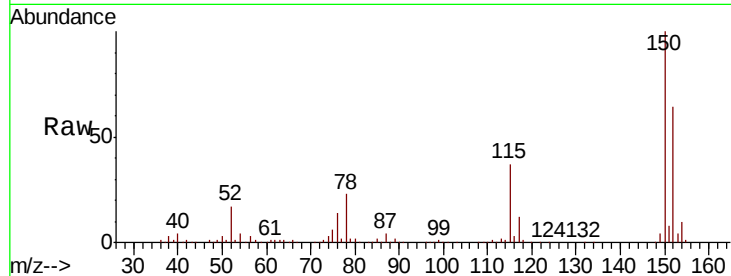


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

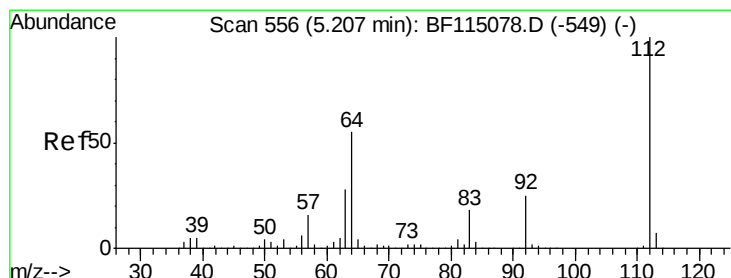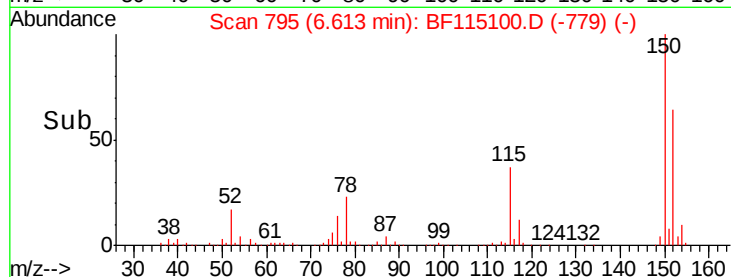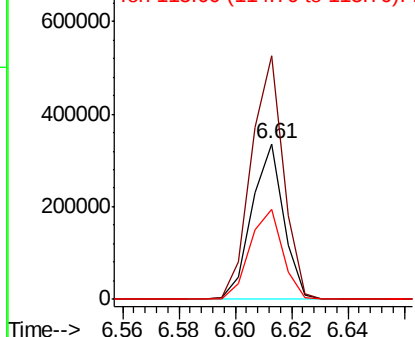



#5


2-Fluorophenol
Concen: 109.987 ng
RT: 5.22 min Scan# 558
Delta R.T. 0.01 min
Lab File: BF115100.D
Acq: 22 Jun 2019 1:24

Tgt Ion:112 Resp: 1872478
Ion Ratio Lower Upper
112 100
64 55.2 43.8 65.6
63 28.4 22.2 33.4

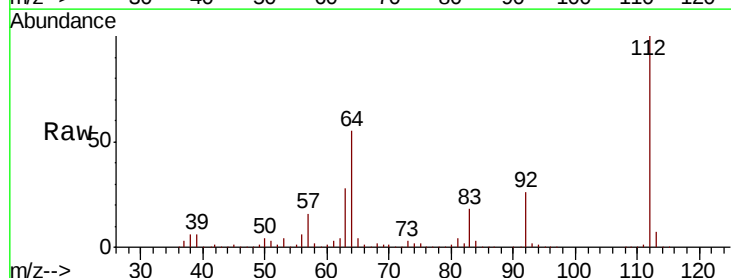

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

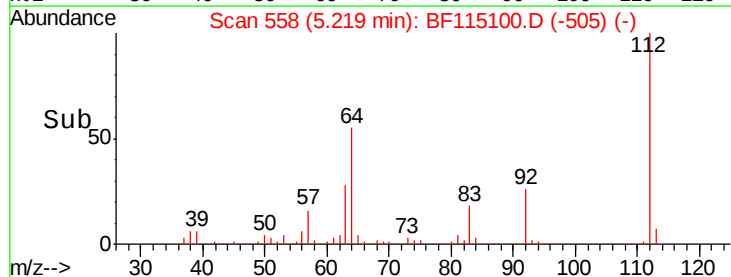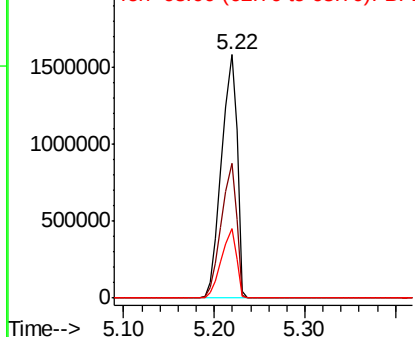

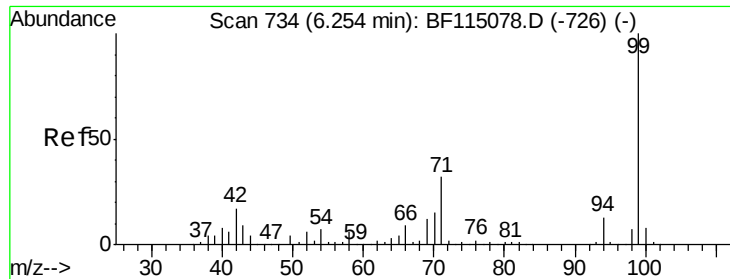

#7

Phenol-d6

Concen: 110.409 ng

RT: 6.25 min Scan# 734

Delta R.T. -0.00 min

Lab File: BF115100.D

Acq: 22 Jun 2019 1:24

Instrument :

BNA_F

ClientSampleId :

PB120777BL


Tot Ion: 99 Resp: 2281464

Ion Ratio Lower Upper




99 100

42 17.3 13.6 20.4

71 33.6 25.5 38.3

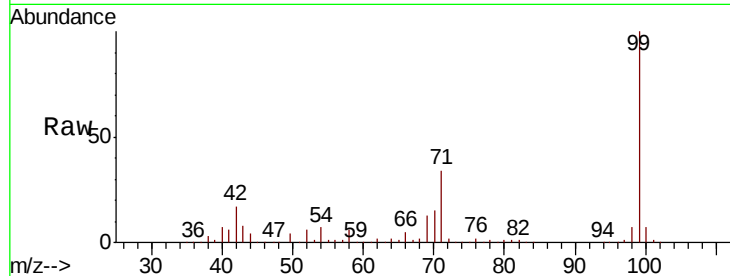

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

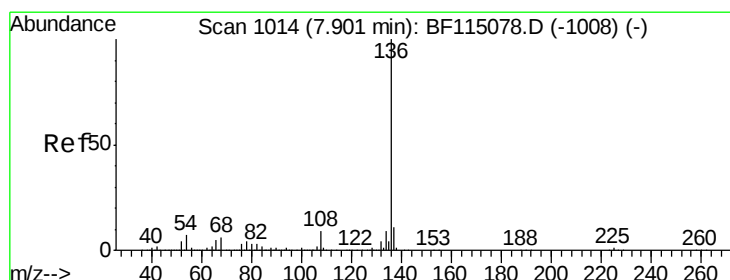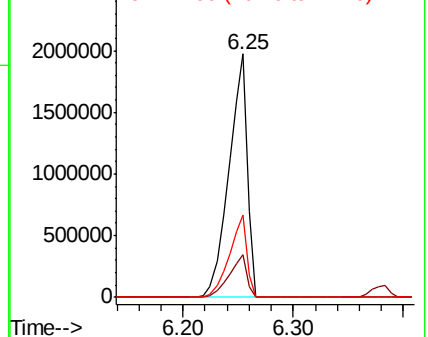

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.90 min Scan# 1013

Delta R.T. -0.01 min

Lab File: BF115100.D

Acq: 22 Jun 2019 1:24

Tgt Ion: 136 Resp: 1014257


Ion Ratio Lower Upper

136 100



137 10.8 8.9 13.3


54 6.3 5.6 8.4

68 5.5 4.8 7.2

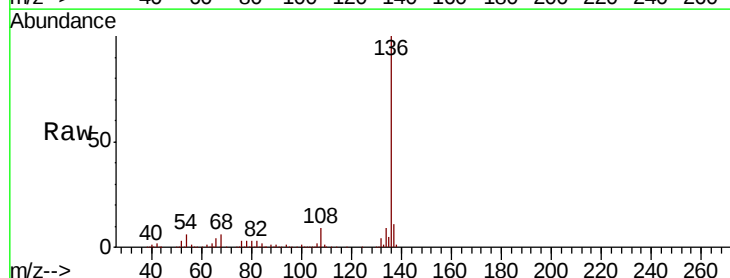

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

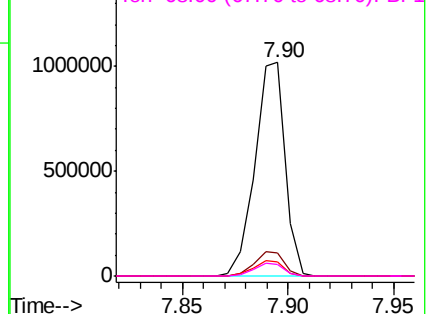







#23
 Nitrobenzene-d5
 Concen: 85.385 ng
 RT: 7.17 min Scan# 890
 Delta R.T. -0.01 min
 Lab File: BF115100.D
 Acq: 22 Jun 2019 1:24

Instrument :
 BNA_F
 ClientSampleId :
 PB120777BL

Tot Ion: 82 Resp: 1407816
 Ion Ratio Lower Upper
 82 100
 128 49.4 40.4 60.6
 54 48.0 37.5 56.3

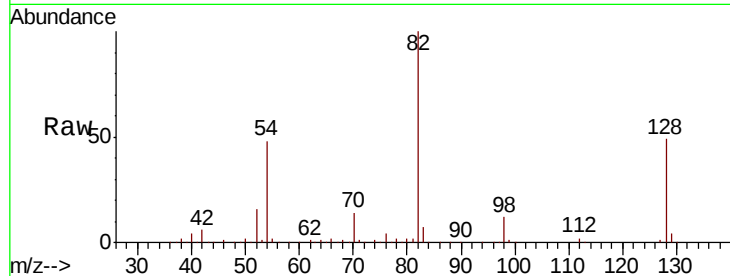


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF1

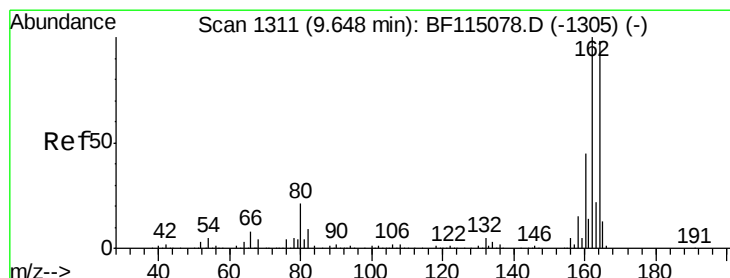
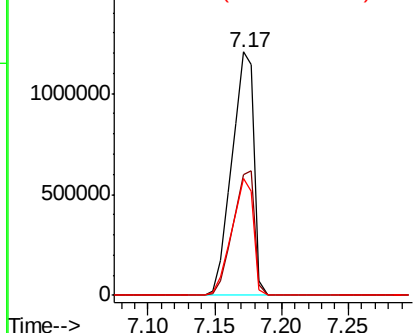



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.64 min Scan# 1310
 Delta R.T. -0.01 min
 Lab File: BF115100.D
 Acq: 22 Jun 2019 1:24

Tgt Ion: 164 Resp: 496153
 Ion Ratio Lower Upper
 164 100
 162 102.4 81.7 122.5
 160 47.6 37.0 55.4

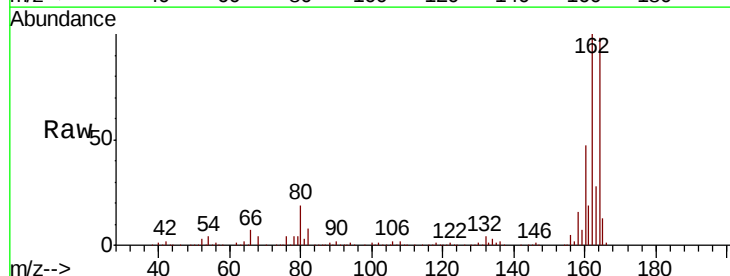

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

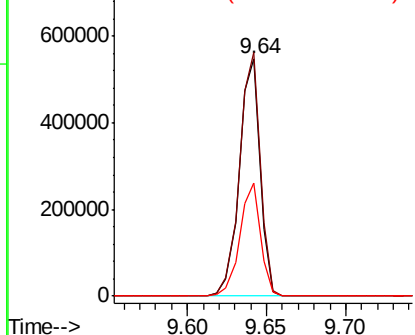



#42

2,4,6-Tribromophenol

Concen: 121.131 ng

RT: 10.42 min Scan# 1443

Delta R.T. -0.01 min

Lab File: BF115100.D

Acq: 22 Jun 2019 1:24

Instrument :

BNA_F

ClientSampleId :

PB120777BL


Tot Ion:330 Resp: 633772

Ion Ratio Lower Upper




330 100

332 95.8 77.3 115.9

141 32.4 28.2 42.2

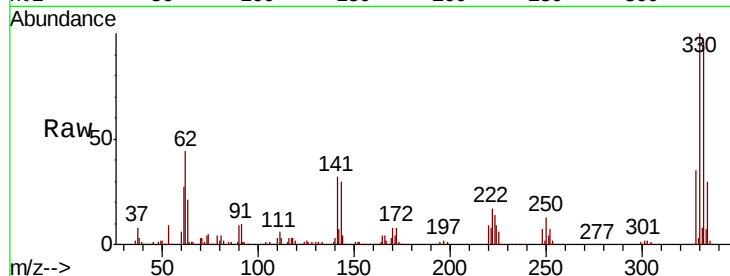

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

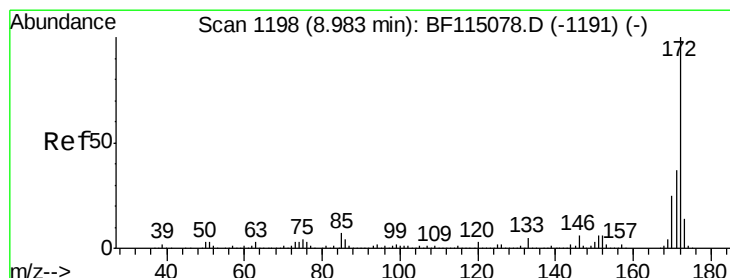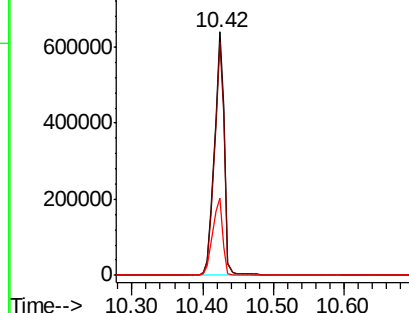

#45

2-Fluorobiphenyl

Concen: 88.379 ng

RT: 8.98 min Scan# 1197

Delta R.T. -0.01 min

Lab File: BF115100.D

Acq: 22 Jun 2019 1:24


Tgt Ion:172 Resp: 2581484

Ion Ratio Lower Upper



172 100


171 38.0 29.8 44.6

170 25.7 20.3 30.5

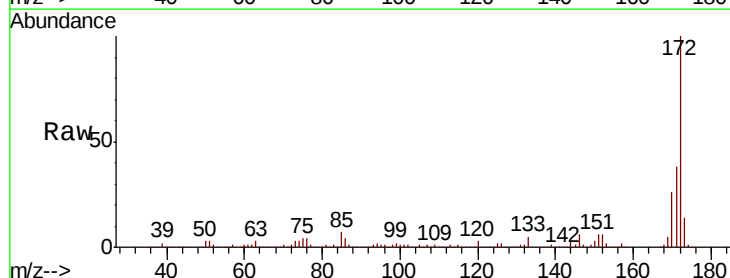

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E



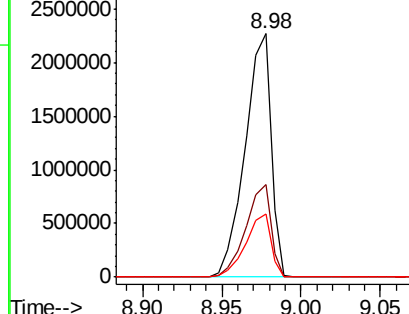





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.11 min Scan# 1560
Delta R.T. -0.01 min
Lab File: BF115100.D
Acq: 22 Jun 2019 1:24




Instrument :
BNA_F
ClientSampleId :
PB120777BL


Tot Ion:188 Resp: 999964
Ion Ratio Lower Upper
188 100
94 10.0 8.6 12.8
80 10.4 8.8 13.2

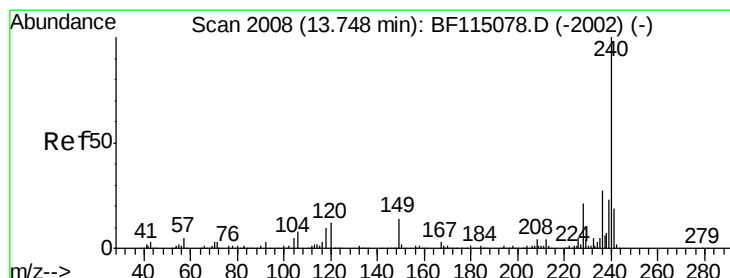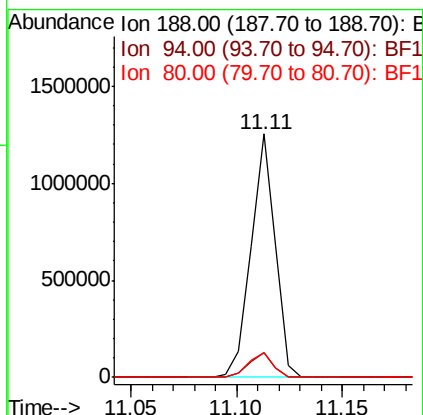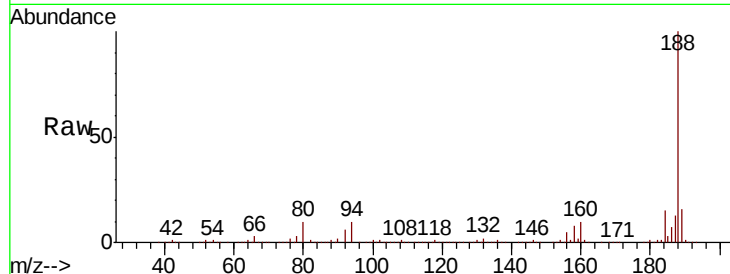

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.74 min Scan# 2006
Delta R.T. -0.01 min
Lab File: BF115100.D
Acq: 22 Jun 2019 1:24

Tgt Ion:240 Resp: 790999
Ion Ratio Lower Upper
240 100
120 11.1 9.4 14.2
236 27.6 21.7 32.5

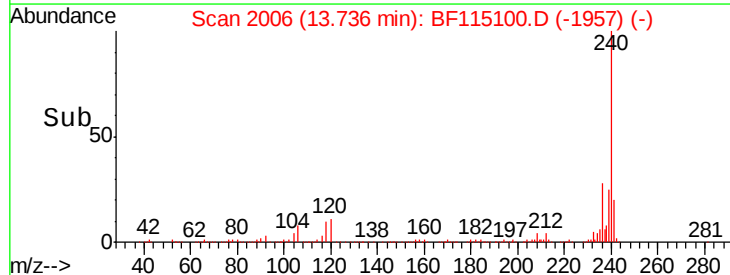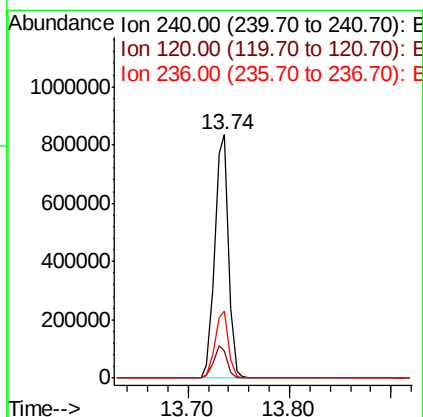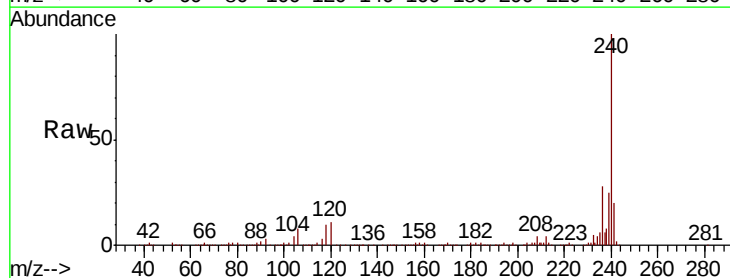

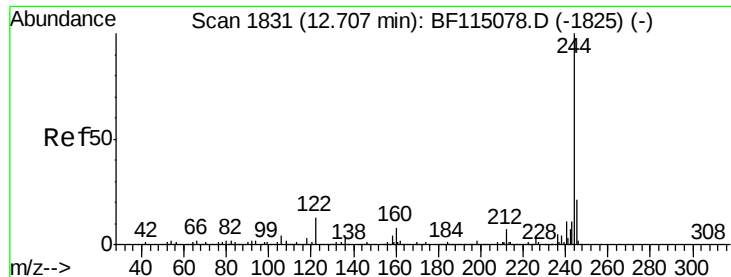

#79

Terphenyl-d14

Concen: 78.130 ng

RT: 12.71 min Scan# 1831

Delta R.T. -0.00 min

Lab File: BF115100.D

Acq: 22 Jun 2019 1:24

Instrument :

BNA_F

ClientSampleId :

PB120777BL


Tot Ion:244 Resp: 2906699

Ion Ratio Lower Upper

244 100

212 7.4 5.8 8.6




122 12.0 10.4 15.6

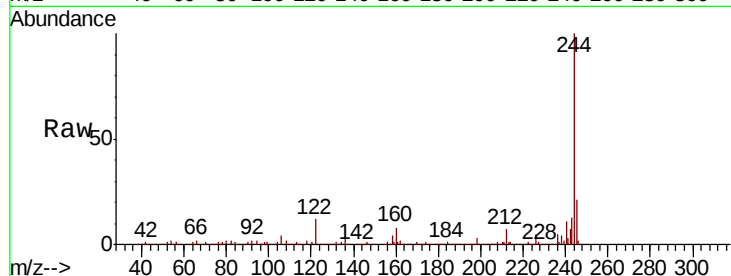

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

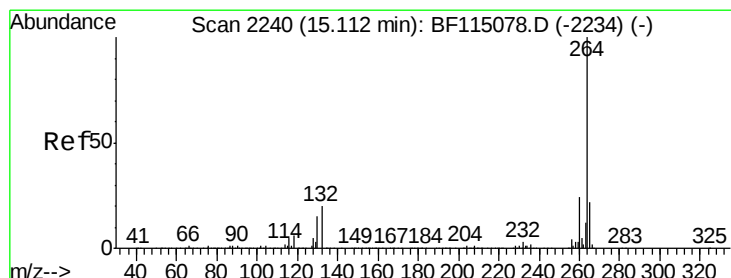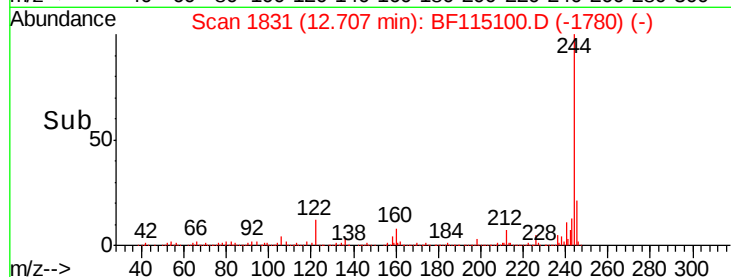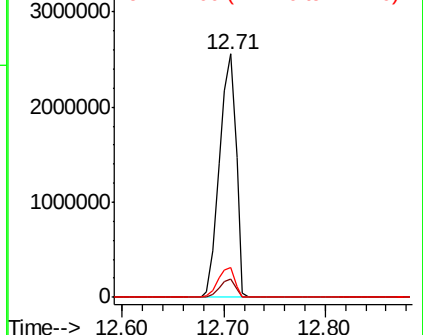

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.10 min Scan# 2238

Delta R.T. -0.01 min

Lab File: BF115100.D

Acq: 22 Jun 2019 1:24


Tgt Ion:264 Resp: 823276

Ion Ratio Lower Upper

264 100

260 24.6 19.6 29.4

265 22.1 17.3 25.9

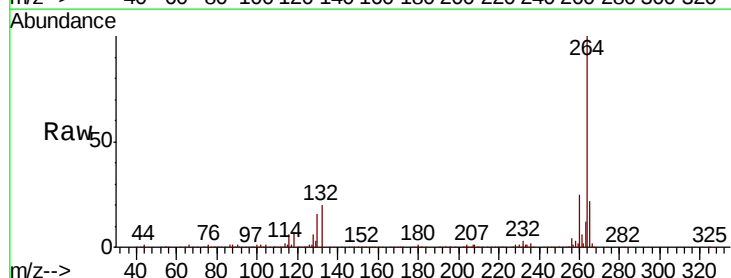

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

