

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
 Data File : BF115090.D
 Acq On : 21 Jun 2019 20:58
 Operator : HP/JU
 Sample : PB120747BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120747BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.219	552	558	561	rBV	5077013	6218760	73.31%	9.875%
2	6.254	727	734	737	rBV	5192508	6366267	75.05%	10.109%
3	6.383	750	756	759	rBV	5828516	6537145	77.07%	10.381%
4	6.613	791	795	798	rBV	1992718	1563405	18.43%	2.483%
5	6.772	817	822	825	rBV	5630119	5223648	61.58%	8.295%
6	7.178	885	891	893	rBV	3573829	4183146	49.32%	6.643%
7	7.895	1008	1013	1016	rBV	2112911	2008392	23.68%	3.189%
8	8.977	1190	1197	1200	rBV	7022345	7658632	90.29%	12.161%
9	9.642	1304	1310	1313	rBV	2606808	2320362	27.35%	3.685%
10	10.424	1437	1443	1446	rBV	4597333	4818208	56.80%	7.651%
11	11.113	1556	1560	1564	rVB	2945185	2562925	30.21%	4.070%
12	12.707	1826	1831	1834	rBV	7125548	8482407	100.00%	13.470%
13	13.736	2002	2006	2010	rBV	2796888	2520369	29.71%	4.002%
14	15.106	2233	2239	2246	rBV	2151286	2510844	29.60%	3.987%


Sum of corrected areas: 62974510

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115090.D
Acq On : 21 Jun 2019 20:58
Operator : HP/JU
Sample : PB120747BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120747BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

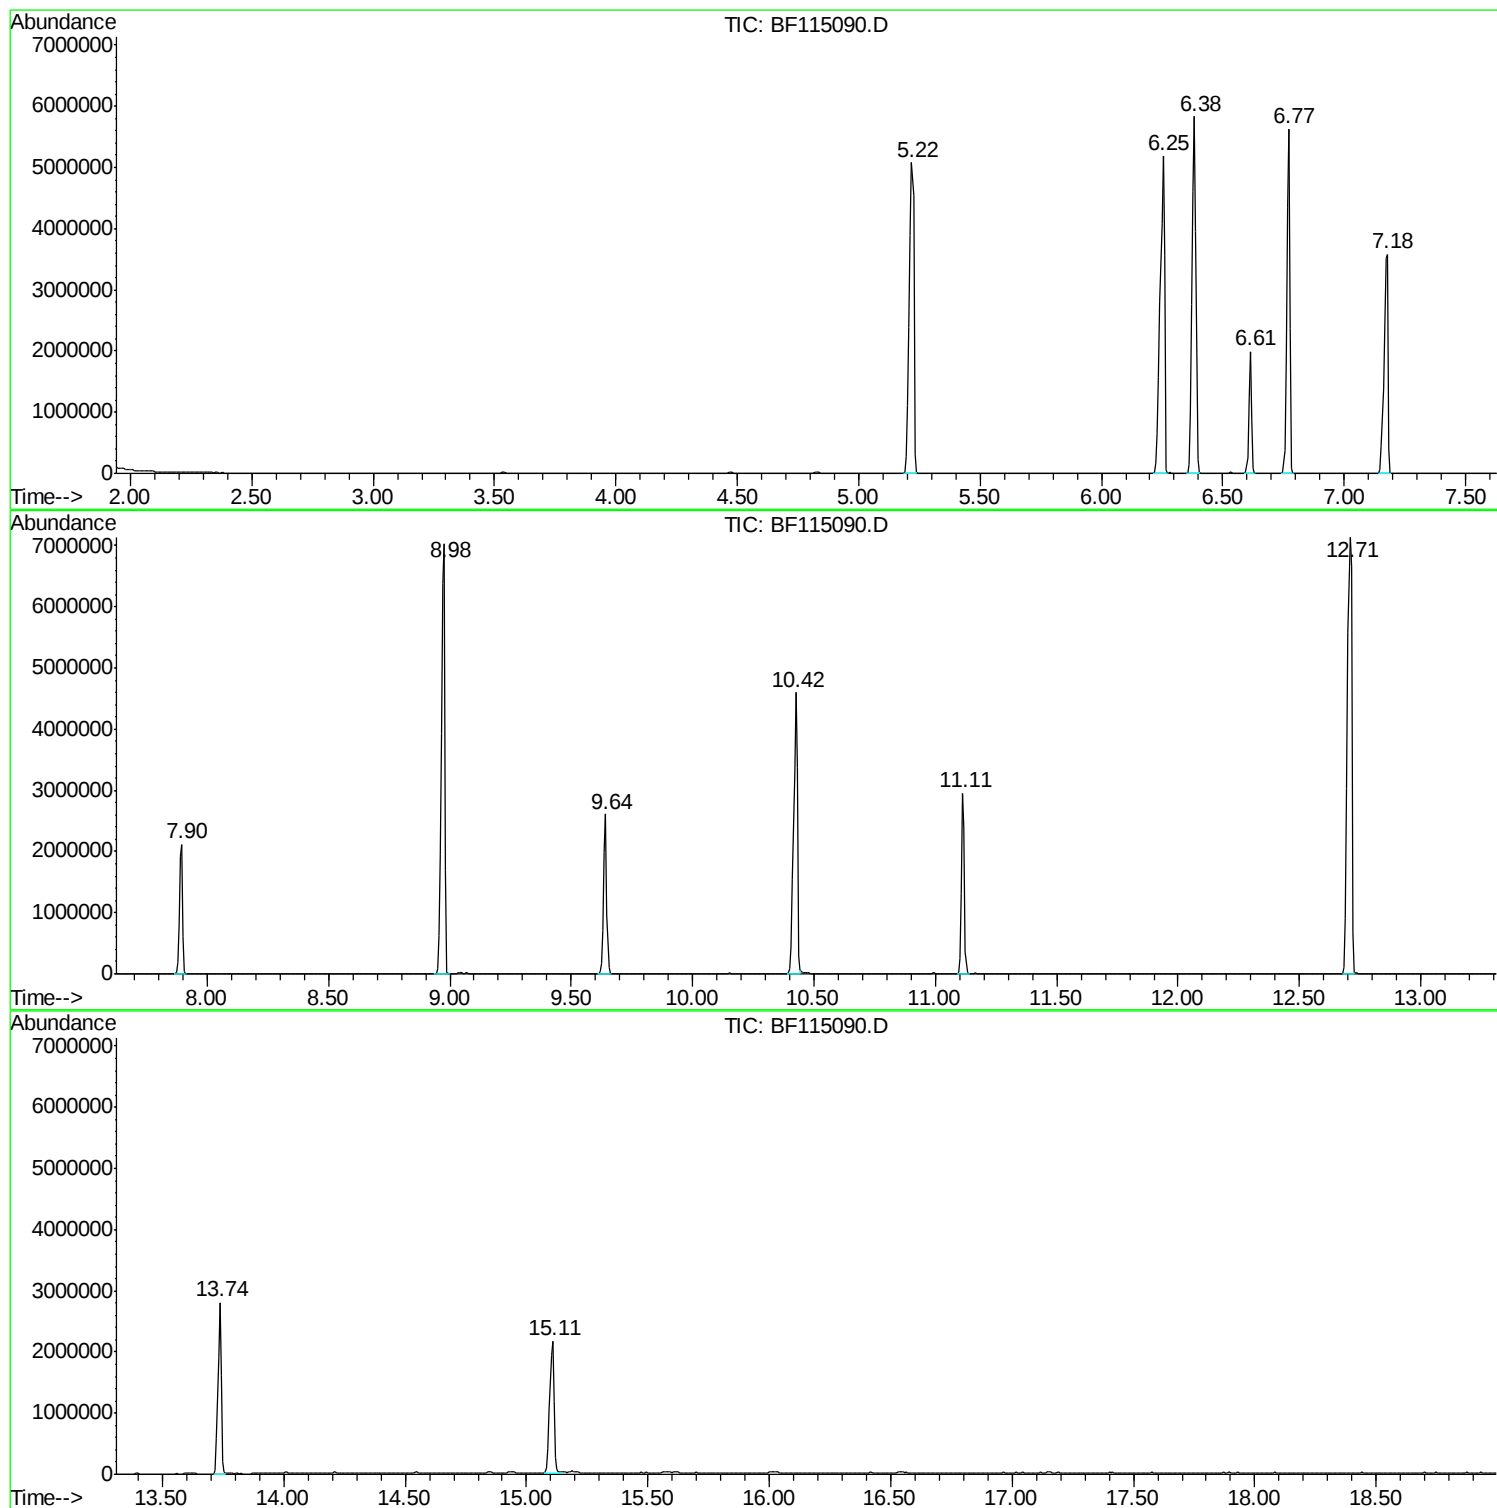

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115090.D
Acq On : 21 Jun 2019 20:58
Operator : HP/JU
Sample : PB120747BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120747BL









Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	83.63 ng	6537150	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	30
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

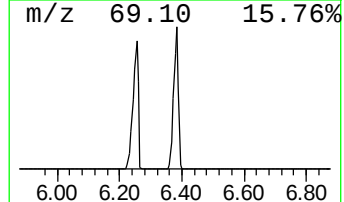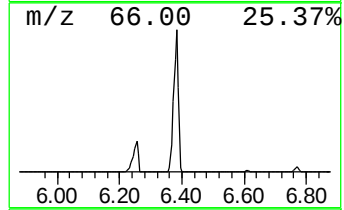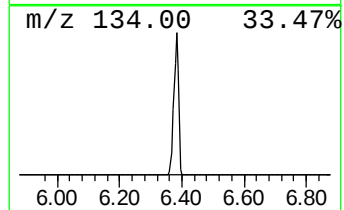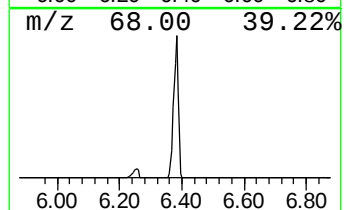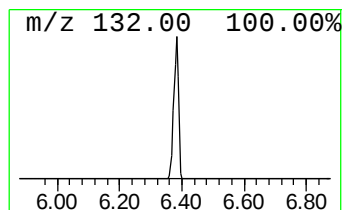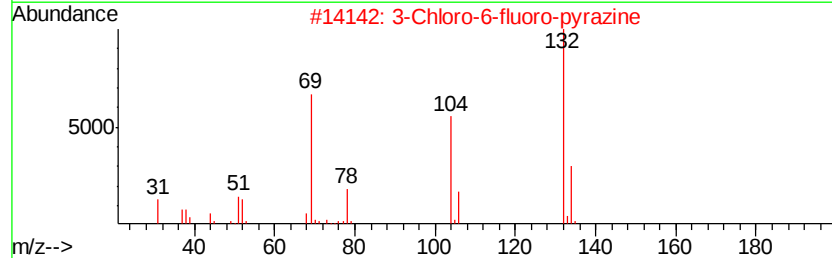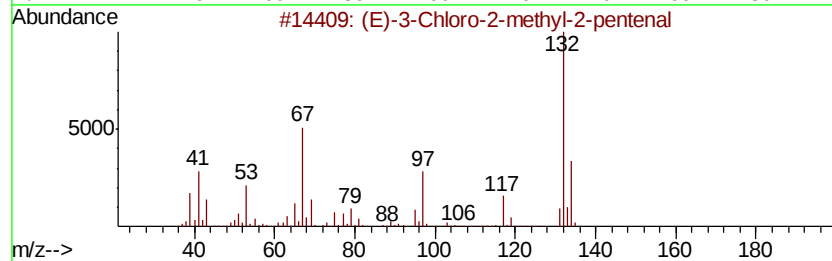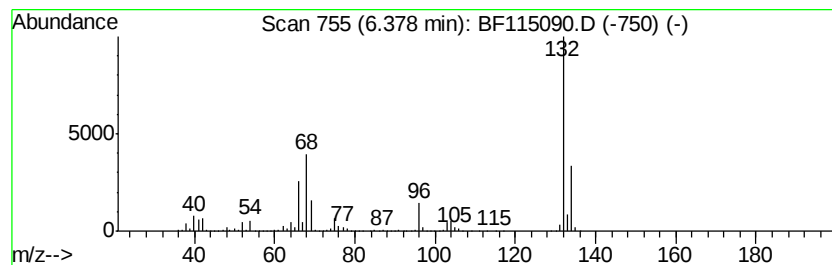

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
Data File : BF115090.D
Acq On : 21 Jun 2019 20:58
Operator : HP/JU
Sample : PB120747BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120747BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.38	6.38	83.6	ng	6537150	1	6.61	1563410	20.0