

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
 Data File : BF115092.D
 Acq On : 21 Jun 2019 21:51
 Operator : HP/JU
 Sample : PB120707BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120707BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.219	552	558	561	rBV	5195089	6173940	75.79%	10.117%
2	6.254	727	734	737	rBV	5206601	6179896	75.87%	10.127%
3	6.384	750	756	759	rBV	5883274	6432019	78.96%	10.540%
4	6.613	791	795	798	rBV	1887686	1485948	18.24%	2.435%
5	6.772	817	822	825	rBV	5554720	5102268	62.64%	8.361%
6	7.172	885	890	893	rBV	3497030	4068721	49.95%	6.668%
7	7.895	1008	1013	1016	rBV	1969326	1919689	23.57%	3.146%
8	8.977	1191	1197	1200	rBV	6836826	7487502	91.92%	12.270%
9	9.642	1304	1310	1313	rBV	2469729	2214430	27.19%	3.629%
10	10.424	1437	1443	1446	rBV	4674258	4805028	58.99%	7.874%
11	11.113	1556	1560	1563	rBV	2864645	2409965	29.59%	3.949%
12	12.707	1826	1831	1834	rBV2	7193332	8145711	100.00%	13.349%
13	13.736	2002	2006	2009	rBV	2719854	2324477	28.54%	3.809%
14	15.101	2233	2238	2248	rBV	1963105	2273439	27.91%	3.726%


Sum of corrected areas: 61023033

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115092.D
Acq On : 21 Jun 2019 21:51
Operator : HP/JU
Sample : PB120707BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120707BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

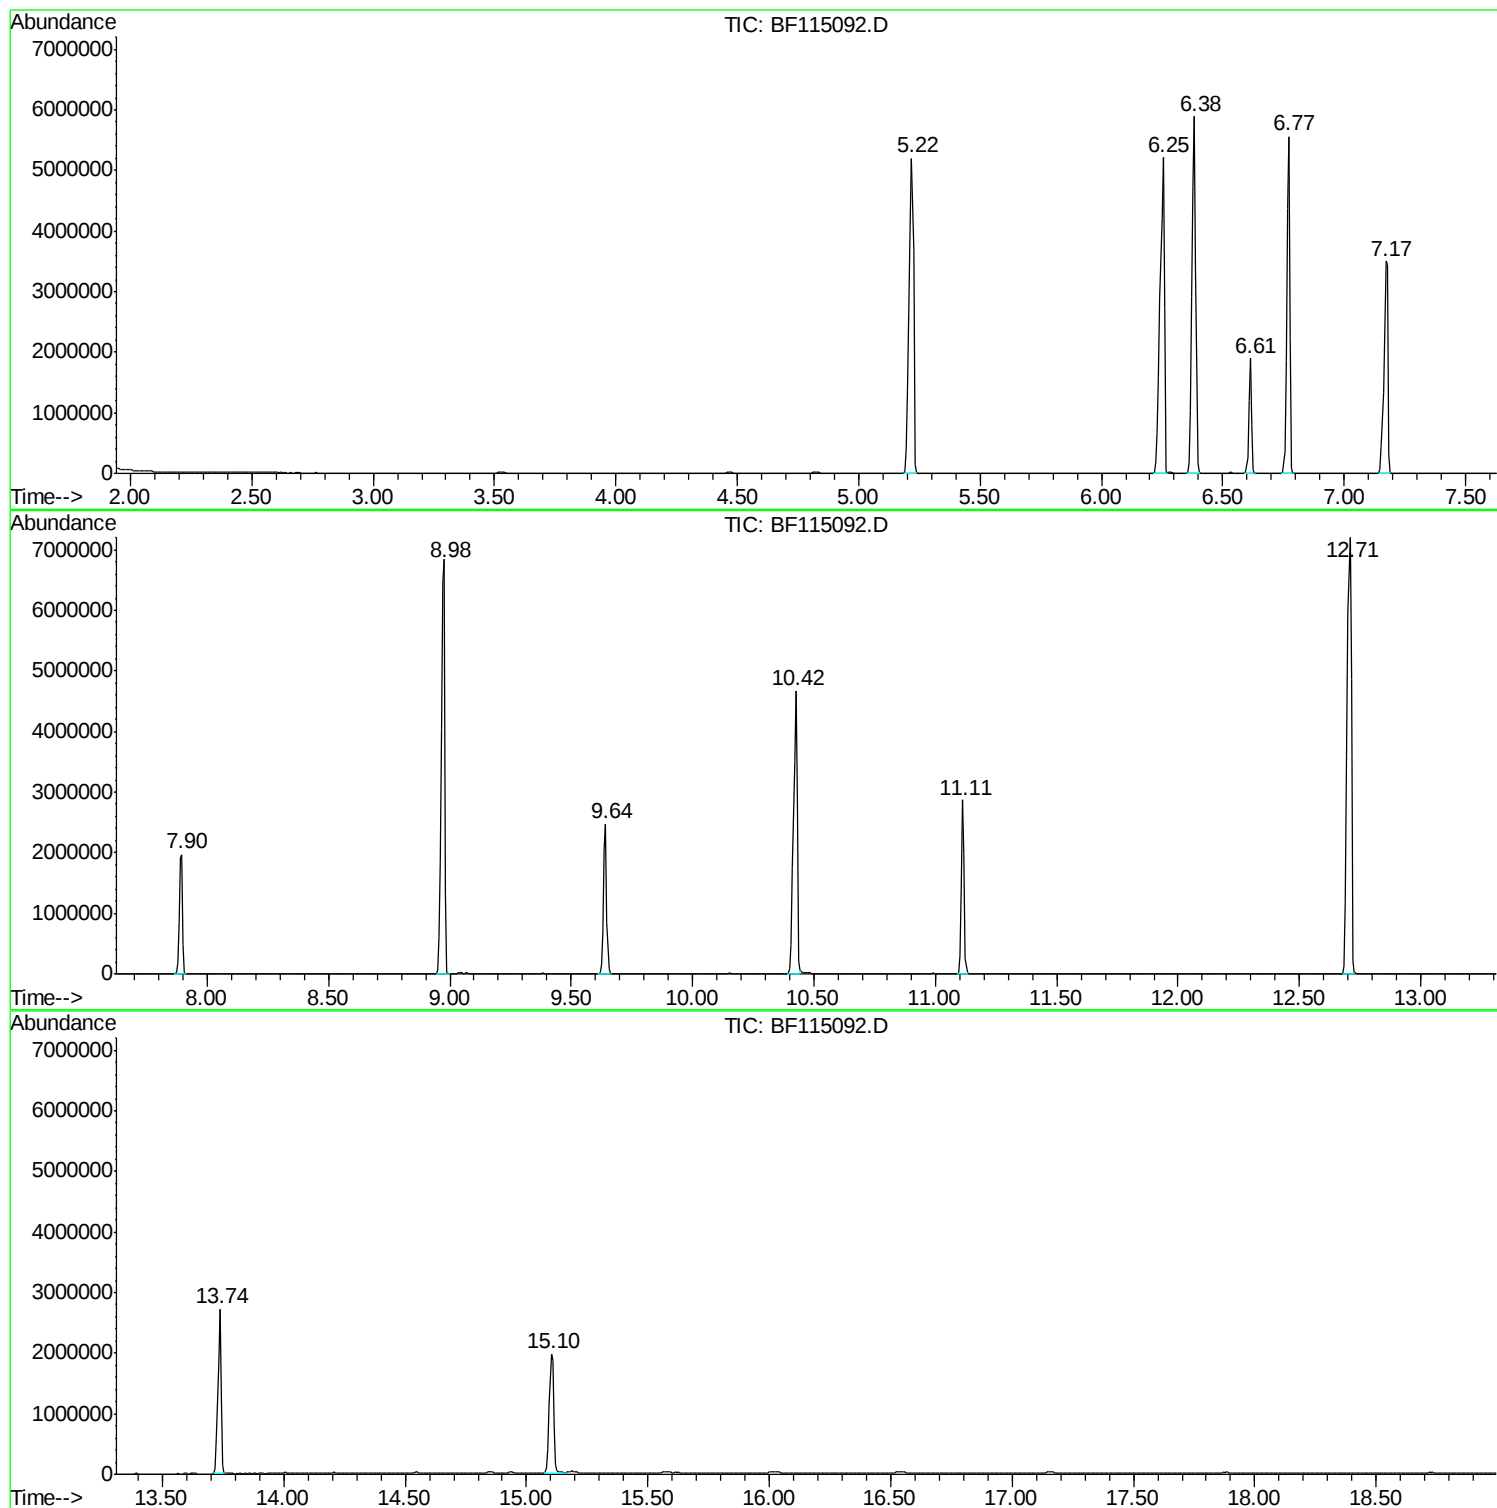

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115092.D
Acq On : 21 Jun 2019 21:51
Operator : HP/JU
Sample : PB120707BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120707BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	86.57 ng	6432020	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	12
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

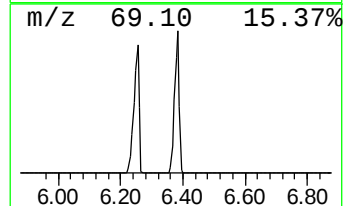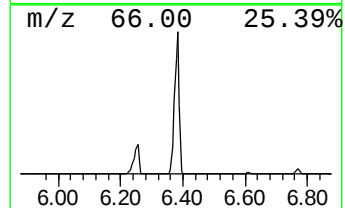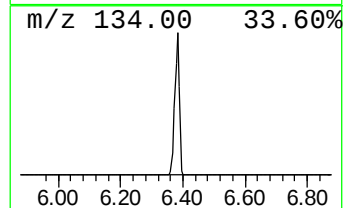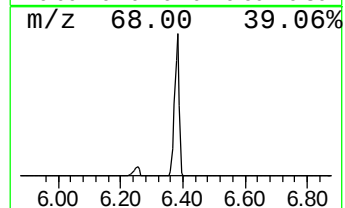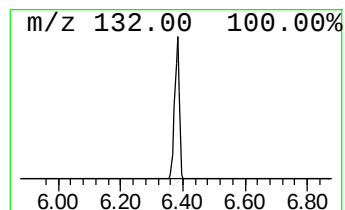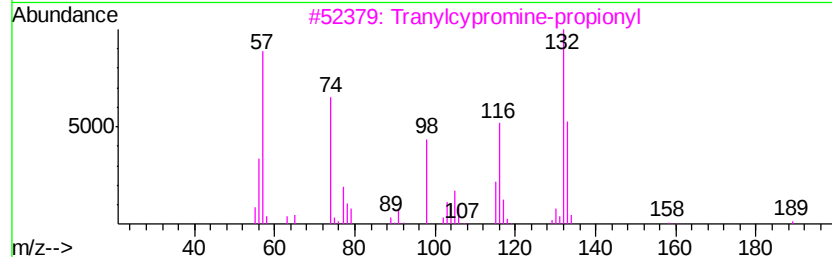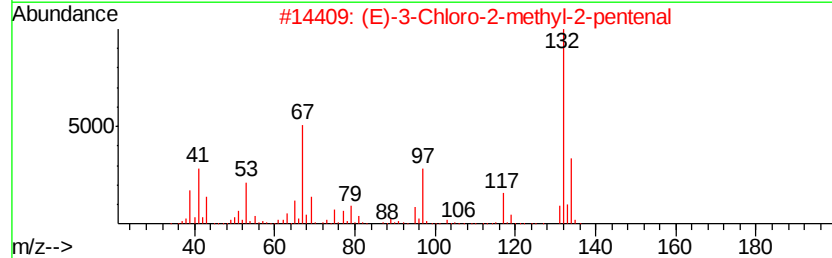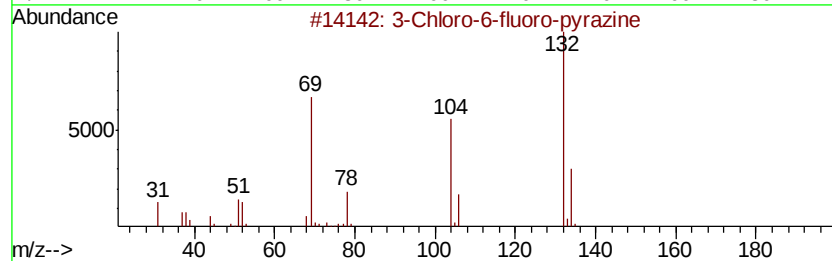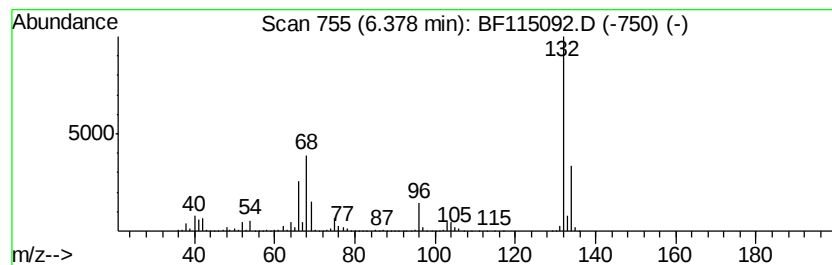

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
Data File : BF115092.D
Acq On : 21 Jun 2019 21:51
Operator : HP/JU
Sample : PB120707BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120707BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.38	6.38	86.6	ng	6432020	1	6.61	1485950	20.0