

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
 Data File : BF115095.D
 Acq On : 21 Jun 2019 23:11
 Operator : HP/JU
 Sample : PB120753BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120753BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.219	552	558	561	rBV	5158598	5607794	73.21%	9.647%
2	6.254	727	734	737	rBV	5038197	5712486	74.57%	9.827%
3	6.384	750	756	759	rBV	5687817	5938833	77.53%	10.216%
4	6.613	791	795	798	rBV	1960632	1549943	20.23%	2.666%
5	6.772	817	822	825	rBV	5058183	4816932	62.88%	8.286%
6	7.172	884	890	893	rBV	3449706	3823076	49.91%	6.577%
7	7.895	1008	1013	1016	rBV	2017835	2014009	26.29%	3.465%
8	8.972	1190	1196	1200	rBV	6405914	7124089	93.00%	12.255%
9	9.642	1304	1310	1313	rBV	2540199	2300698	30.03%	3.958%
10	10.424	1437	1443	1446	rBV	4538659	4325869	56.47%	7.442%
11	11.113	1556	1560	1563	rBV	2996129	2518567	32.88%	4.333%
12	12.707	1825	1831	1834	rBV	7090008	7660285	100.00%	13.178%
13	13.736	2001	2006	2009	rBV	2670502	2393274	31.24%	4.117%
14	15.101	2233	2238	2246	rBV	2105429	2344240	30.60%	4.033%


Sum of corrected areas: 58130095

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115095.D
Acq On : 21 Jun 2019 23:11
Operator : HP/JU
Sample : PB120753BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120753BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

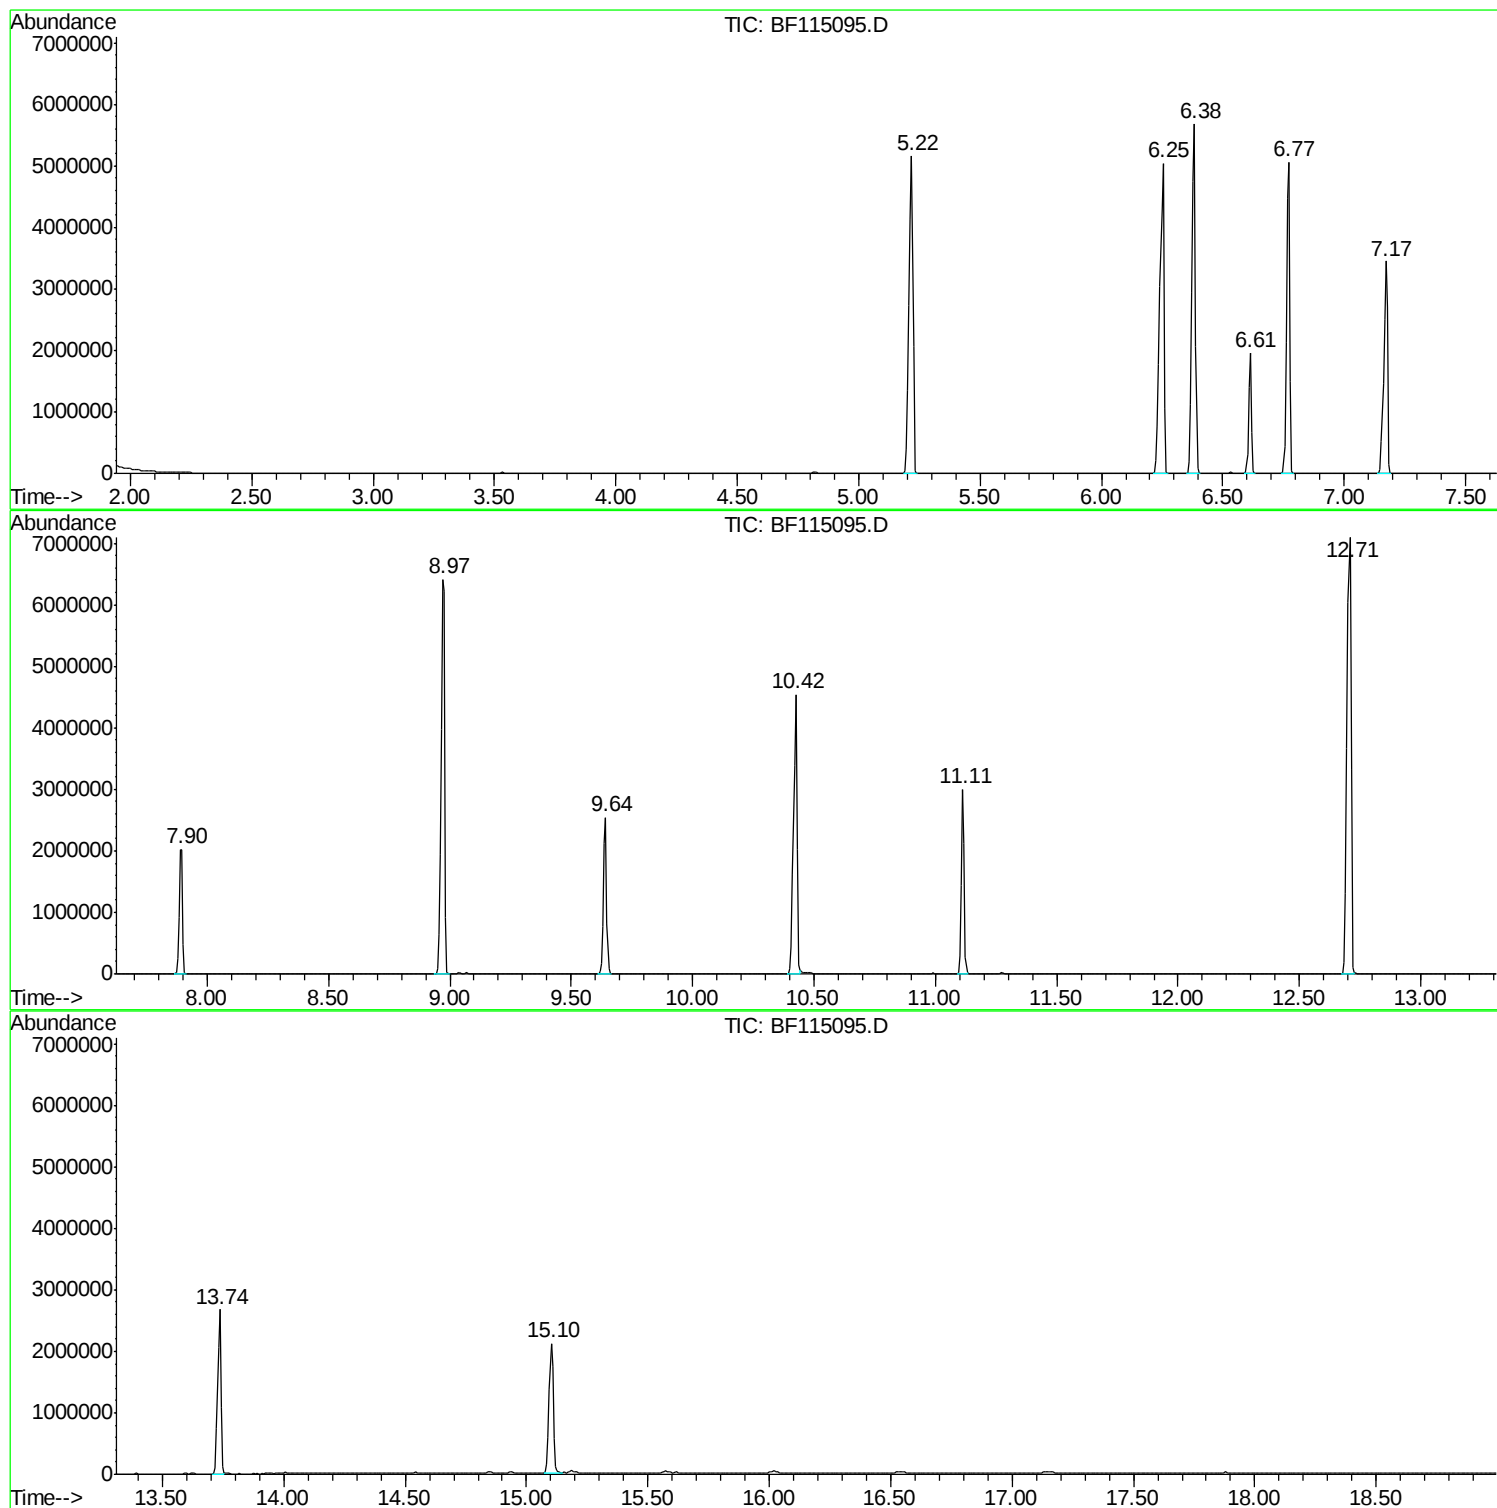

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115095.D
Acq On : 21 Jun 2019 23:11
Operator : HP/JU
Sample : PB120753BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120753BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	76.63 ng	5938830	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	12
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

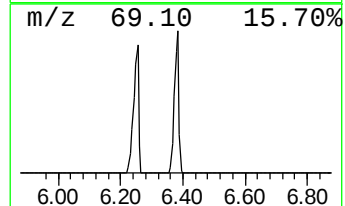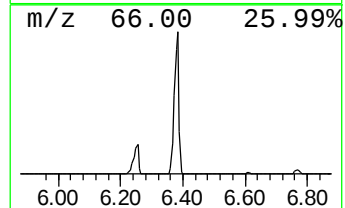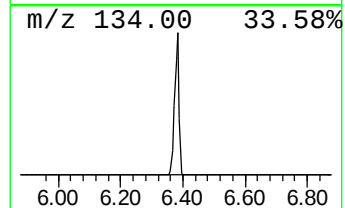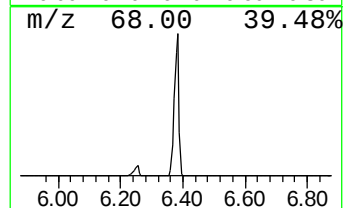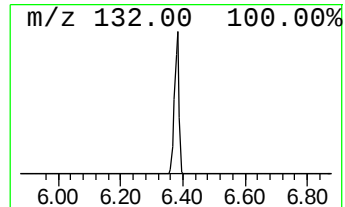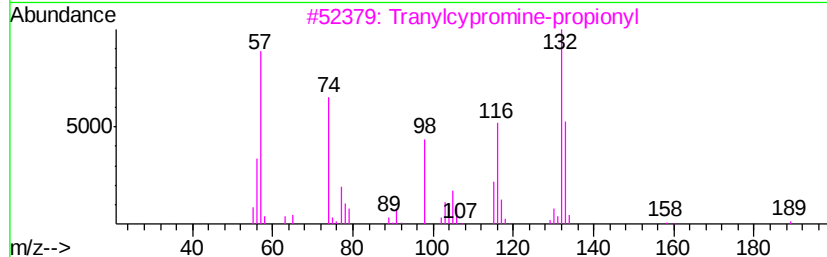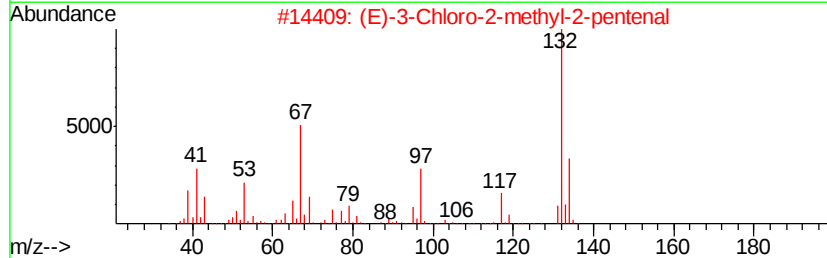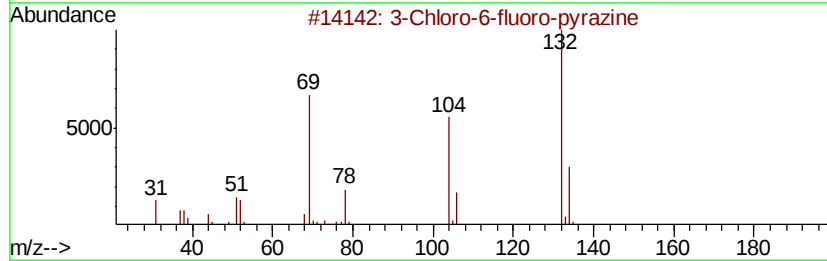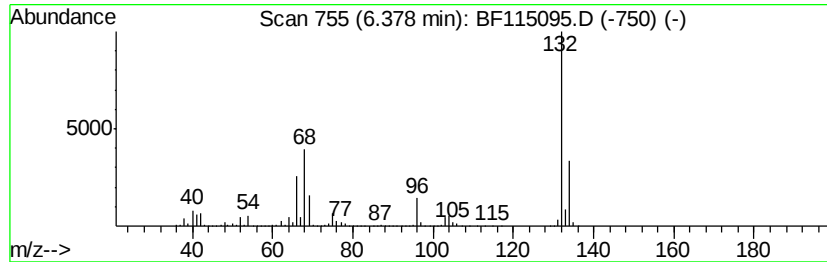

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
Data File : BF115095.D
Acq On : 21 Jun 2019 23:11
Operator : HP/JU
Sample : PB120753BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120753BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.38	6.38	76.6	ng	5938830	1	6.61	1549940	20.0