

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
 Data File : BF115098.D
 Acq On : 22 Jun 2019 00:30
 Operator : HP/JU
 Sample : PB120612BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120612BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.219	552	558	561	rBV	5004062	5350127	75.23%	9.809%
2	6.254	727	734	736	rBV	4525450	5464468	76.84%	10.019%
3	6.384	750	756	759	rBV	5080546	5658704	79.57%	10.375%
4	6.613	791	795	798	rBV	1734814	1434432	20.17%	2.630%
5	6.772	817	822	825	rBV	4578848	4537022	63.80%	8.318%
6	7.172	884	890	893	rBV	3353454	3510094	49.36%	6.435%
7	7.890	1007	1012	1016	rBV	1944071	1871033	26.31%	3.430%
8	8.972	1190	1196	1199	rBV	6292725	6761643	95.08%	12.397%
9	9.636	1304	1309	1313	rBV	2187002	2168184	30.49%	3.975%
10	10.425	1437	1443	1446	rBV	3997725	3993174	56.15%	7.321%
11	11.113	1556	1560	1563	rBV	2979815	2355697	33.13%	4.319%
12	12.707	1825	1831	1834	rBV	6491567	7111372	100.00%	13.038%
13	13.730	2001	2005	2009	rBV	2211114	2208730	31.06%	4.049%
14	15.101	2233	2238	2248	rBV	1978113	2118808	29.79%	3.885%


Sum of corrected areas: 54543488

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115098.D
Acq On : 22 Jun 2019 00:30
Operator : HP/JU
Sample : PB120612BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120612BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

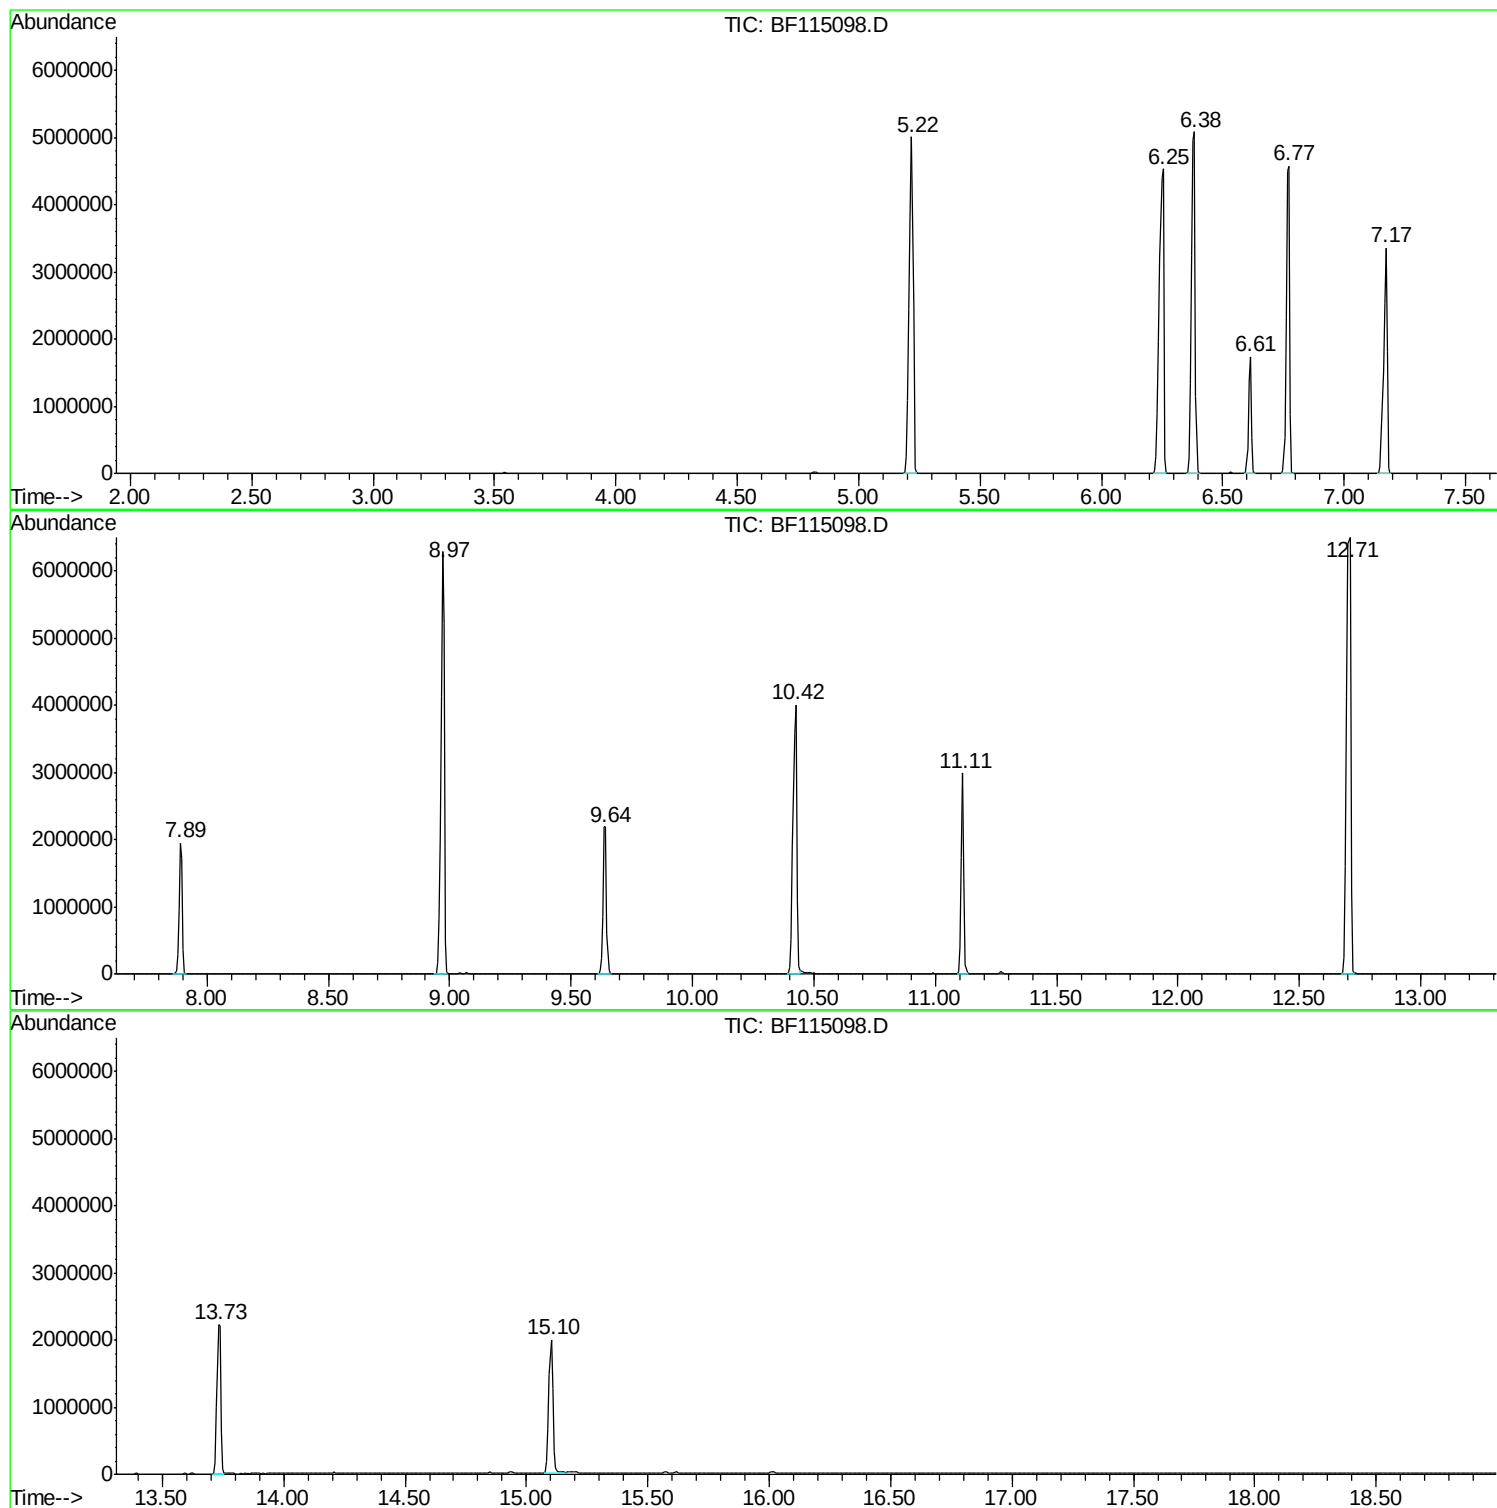

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115098.D
Acq On : 22 Jun 2019 00:30
Operator : HP/JU
Sample : PB120612BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120612BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	78.90 ng	5658700	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	16
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
4		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
5		Cyclopropanamine, 1-phenyl-	133	C9H11N	1000351-26-2	9

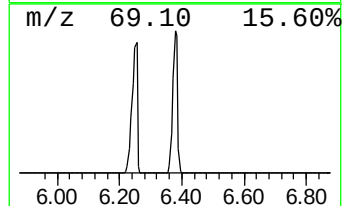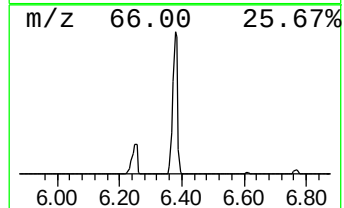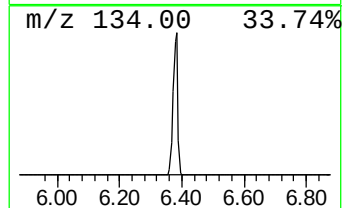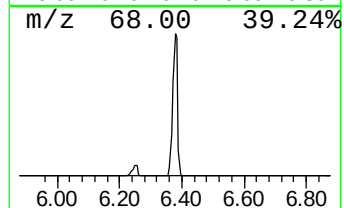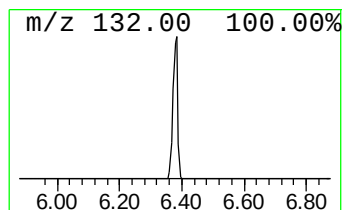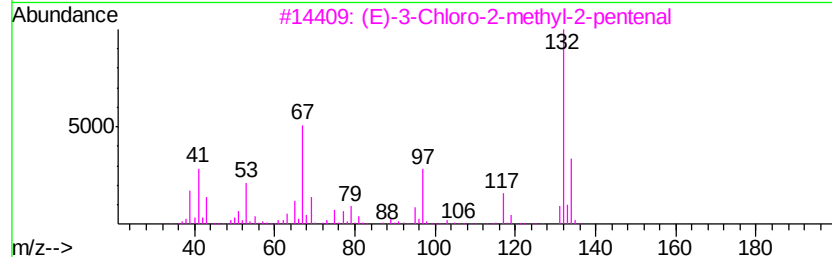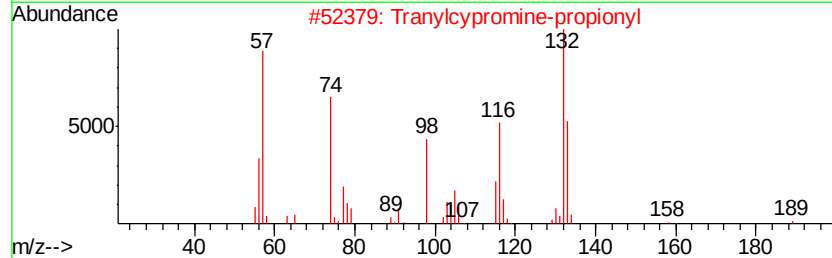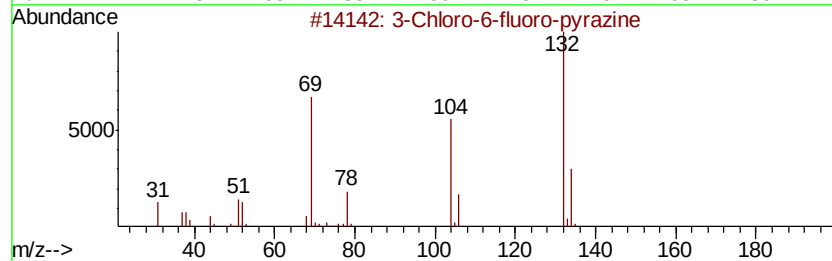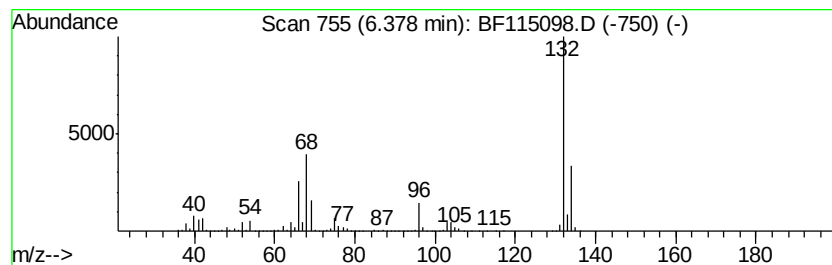

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
Data File : BF115098.D
Acq On : 22 Jun 2019 00:30
Operator : HP/JU
Sample : PB120612BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120612BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.38	6.38	78.9	ng	5658700	1	6.61	1434430	20.0