

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
 Data File : BF115100.D
 Acq On : 22 Jun 2019 1:24
 Operator : HP/JU
 Sample : PB120777BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120777BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.219	552	558	561	rBV	5249863	6073444	75.83%	9.868%
2	6.254	727	734	737	rBV	5415152	6116749	76.37%	9.939%
3	6.383	750	756	759	rBV	5721256	6366605	79.49%	10.345%
4	6.613	791	795	798	rVB	1878974	1521077	18.99%	2.471%
5	6.772	817	822	825	rBV	5493032	5154145	64.35%	8.375%
6	7.172	884	890	893	rBV	3529104	4111835	51.34%	6.681%
7	7.889	1008	1012	1016	rBV	1970784	1962208	24.50%	3.188%
8	8.977	1190	1197	1200	rBV	6829154	7655397	95.58%	12.439%
9	9.642	1304	1310	1313	rBV	2459030	2249931	28.09%	3.656%
10	10.424	1437	1443	1446	rBV	4663691	4579855	57.18%	7.441%
11	11.113	1556	1560	1563	rBV	3089112	2450597	30.60%	3.982%
12	12.707	1825	1831	1834	rBV	7258715	8009179	100.00%	13.014%
13	13.736	2001	2006	2009	rBV	2398336	2282541	28.50%	3.709%
14	14.848	2191	2195	2203	rBV	74587	81575	1.02%	0.133%
15	15.101	2233	2238	2248	rBV	2020129	2223296	27.76%	3.612%
16	15.183	2248	2252	2261	rVB	119964	148102	1.85%	0.241%
17	15.571	2313	2318	2323	rBV	121566	168741	2.11%	0.274%
18	16.018	2388	2394	2404	rBV	97700	175899	2.20%	0.286%
19	16.536	2476	2482	2495	rVB3	62683	130262	1.63%	0.212%
20	17.148	2581	2586	2599	rVB3	33960	83406	1.04%	0.136%


Sum of corrected areas: 61544844

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115100.D
Acq On : 22 Jun 2019 1:24
Operator : HP/JU
Sample : PB120777BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120777BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

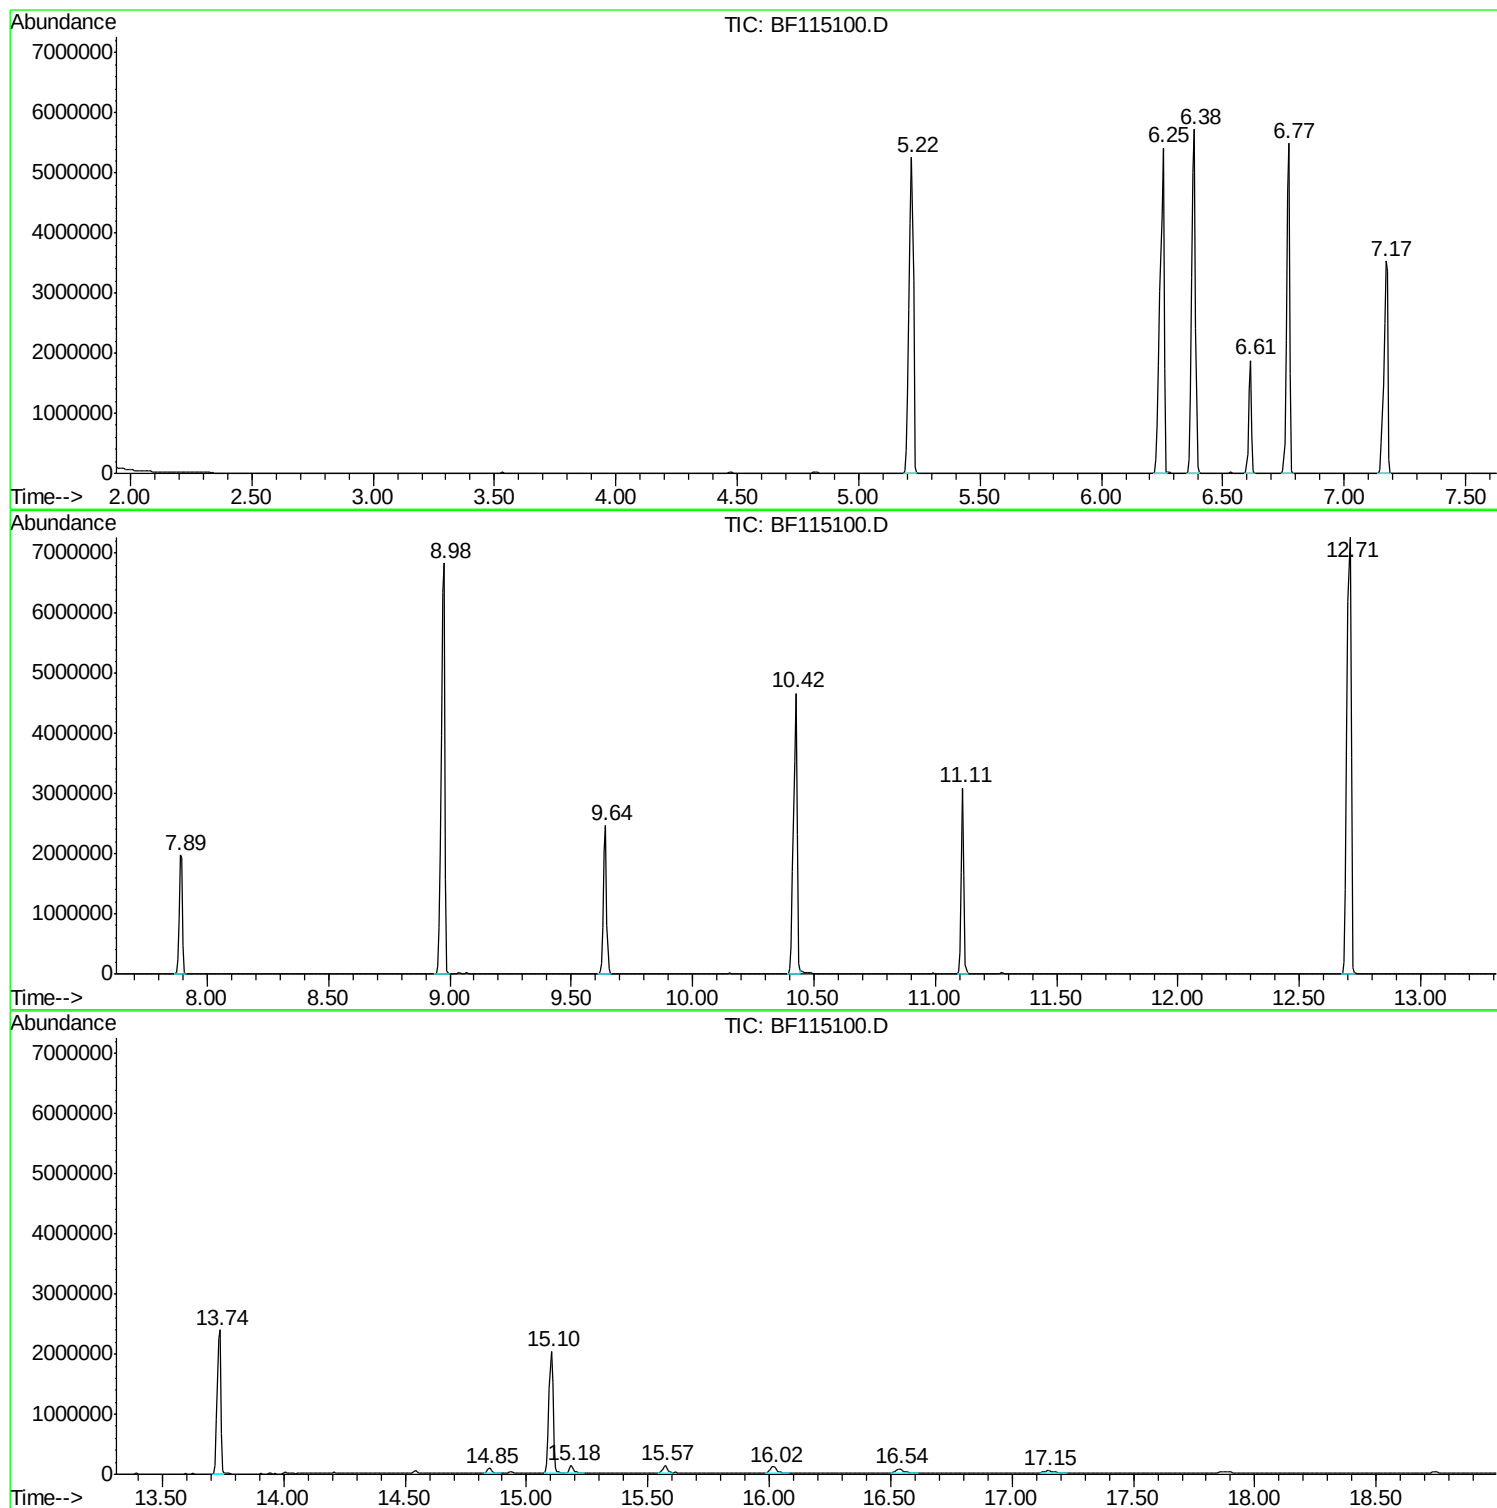

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115100.D
Acq On : 22 Jun 2019 1:24
Operator : HP/JU
Sample : PB120777BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120777BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	83.71 ng	6366610	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

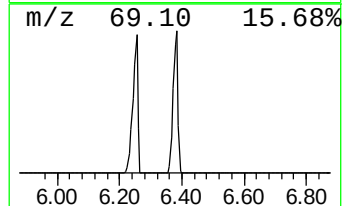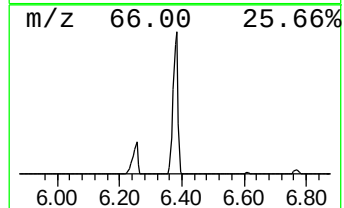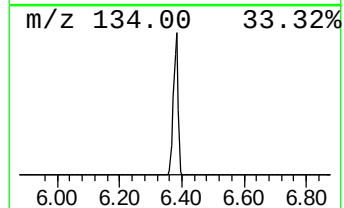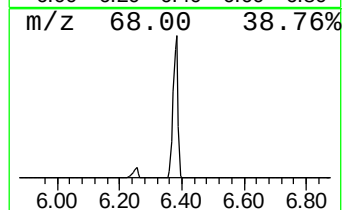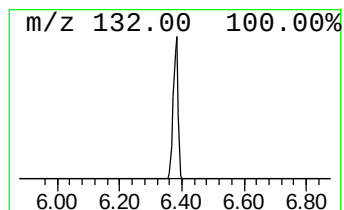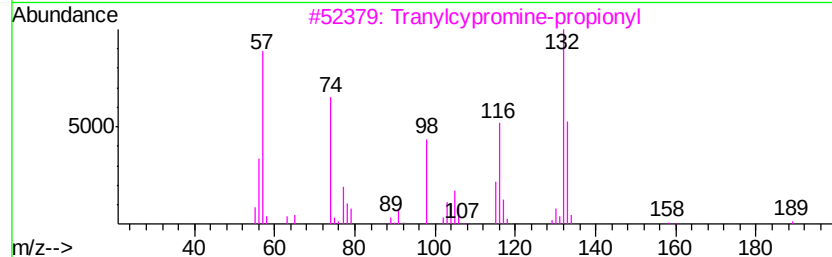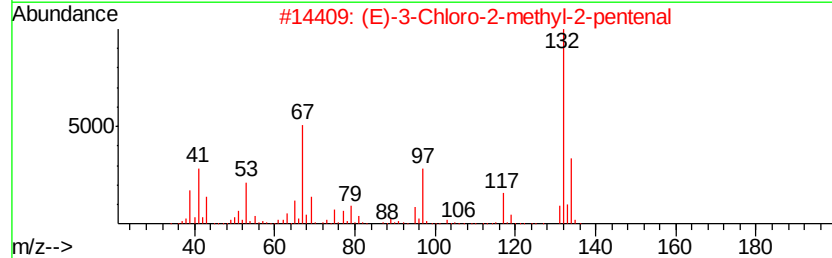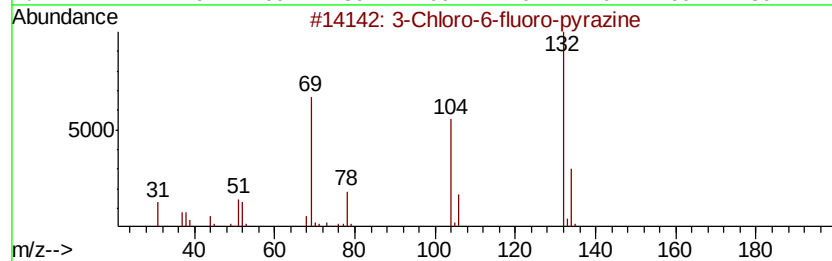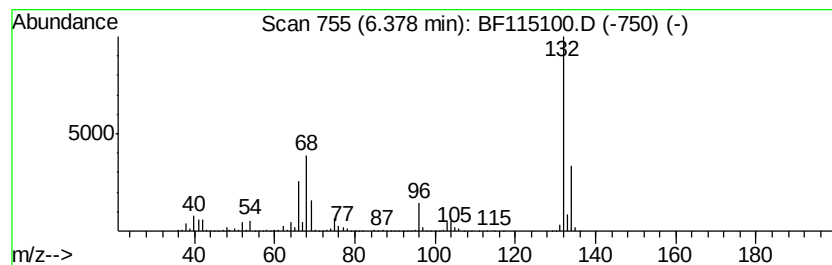

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
Data File : BF115100.D
Acq On : 22 Jun 2019 1:24
Operator : HP/JU
Sample : PB120777BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120777BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.38	6.38	83.7	ng	6366610	1	6.61	1521080	20.0