

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
 Data File : BF115102.D
 Acq On : 22 Jun 2019 2:16
 Operator : HP/JU
 Sample : PB120818BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120818BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.219	552	558	561	rBV	4977502	5415325	73.11%	9.709%
2	6.254	727	734	736	rBV	4754888	5595813	75.55%	10.033%
3	6.384	750	756	759	rBV	5167811	5780134	78.04%	10.364%
4	6.613	791	795	798	rBV	1726961	1462494	19.75%	2.622%
5	6.772	817	822	825	rVB	4722950	4681401	63.20%	8.394%
6	7.172	884	890	893	rBV	3508079	3662543	49.45%	6.567%
7	7.889	1008	1012	1016	rBV	1908028	1881733	25.41%	3.374%
8	8.972	1190	1196	1199	rBV	6389237	6961637	93.99%	12.482%
9	9.642	1304	1310	1313	rBV	2218340	2174183	29.35%	3.898%
10	10.425	1437	1443	1446	rBV	4352363	4116301	55.58%	7.380%
11	11.113	1556	1560	1563	rBV	2987348	2356667	31.82%	4.225%
12	12.707	1825	1831	1834	rBV	6974541	7406709	100.00%	13.280%
13	13.730	2001	2005	2009	rBV	2314258	2205865	29.78%	3.955%
14	15.101	2233	2238	2248	rBV	1958498	2072890	27.99%	3.717%


Sum of corrected areas: 55773695

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115102.D
Acq On : 22 Jun 2019 2:16
Operator : HP/JU
Sample : PB120818BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120818BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

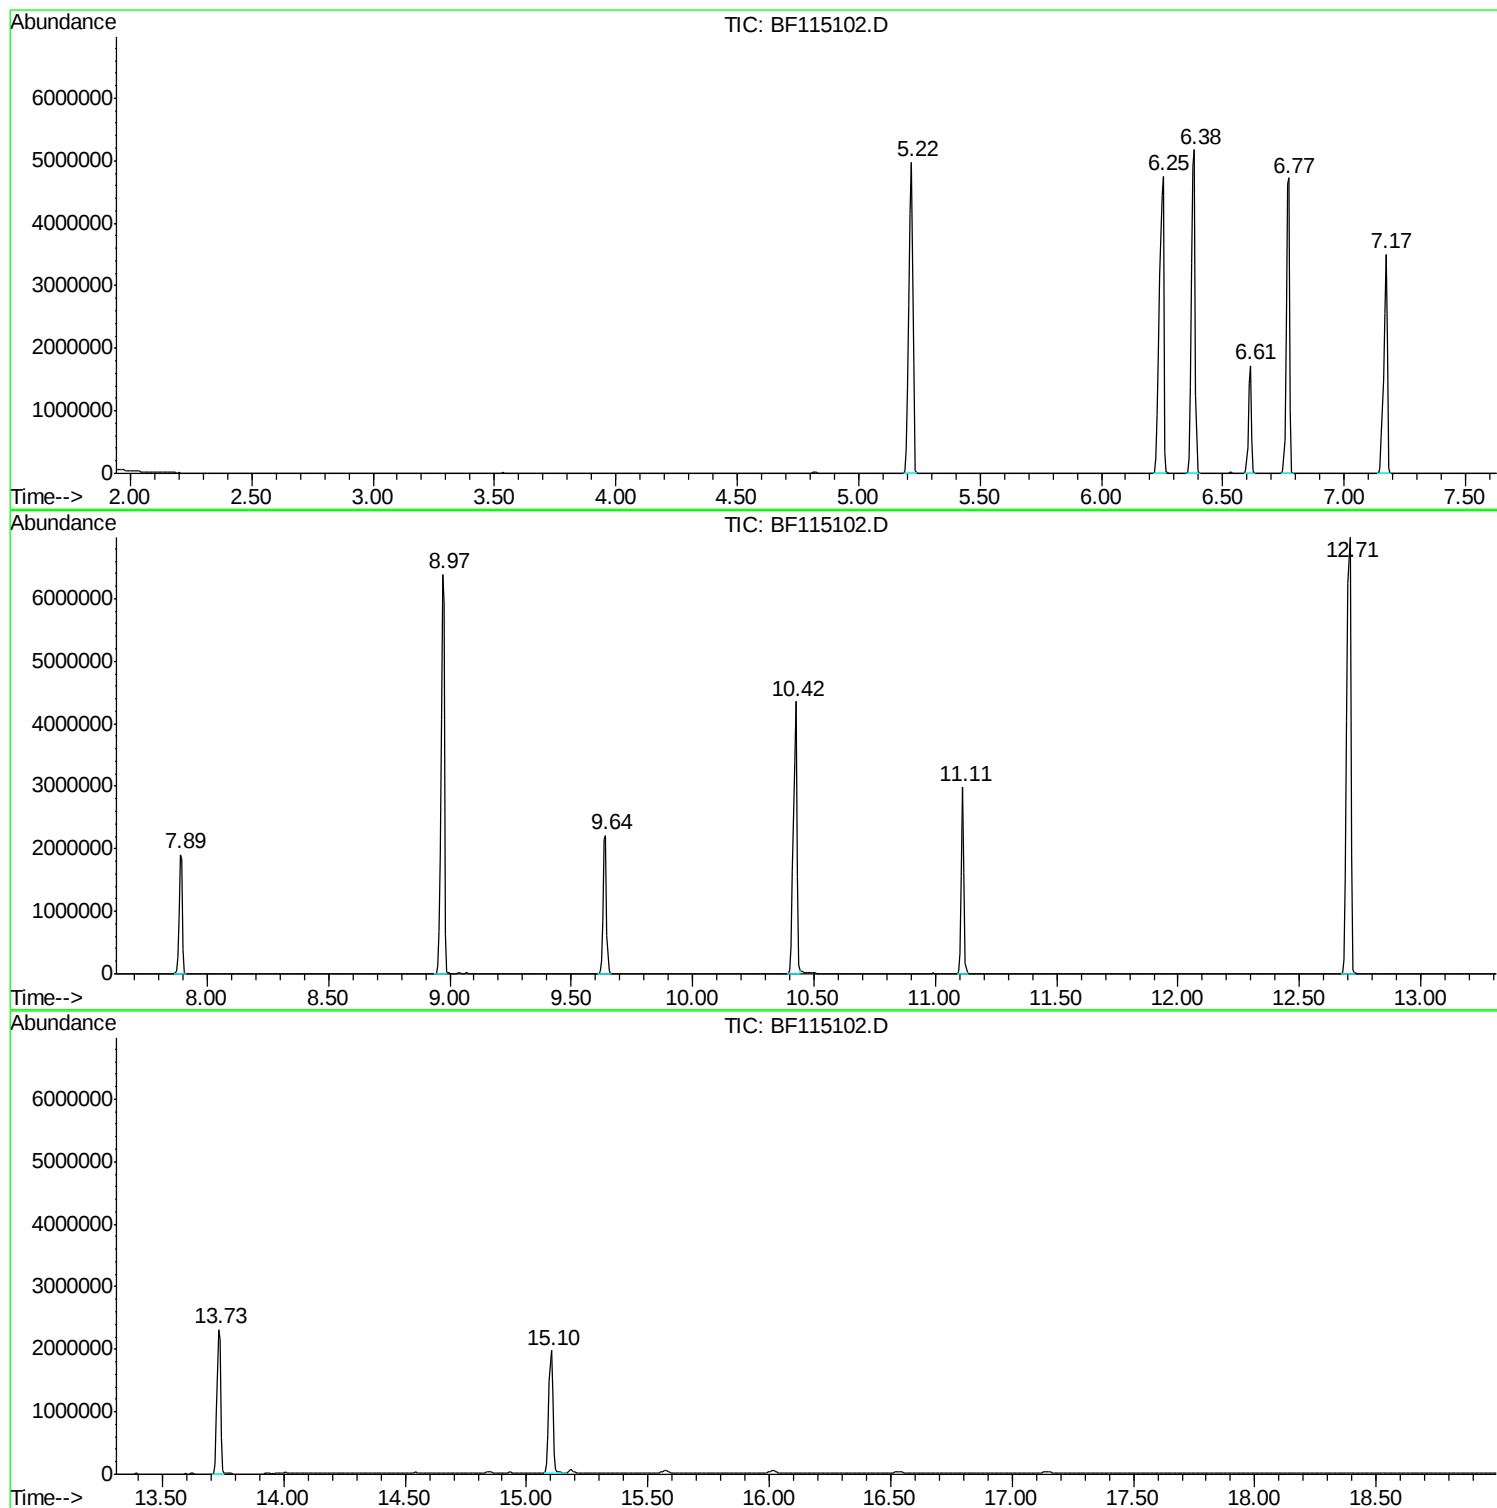

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062119\
Data File : BF115102.D
Acq On : 22 Jun 2019 2:16
Operator : HP/JU
Sample : PB120818BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120818BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	79.04 ng	5780130	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	16
4		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
5		Xenon	132	Xe	007440-63-3	9

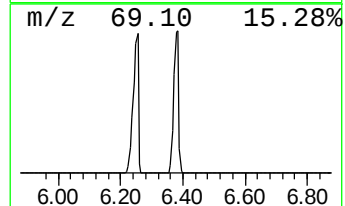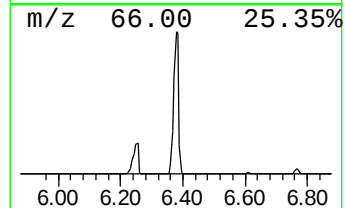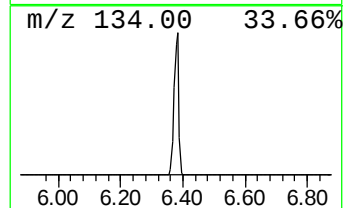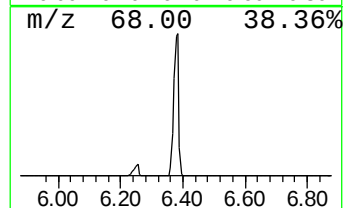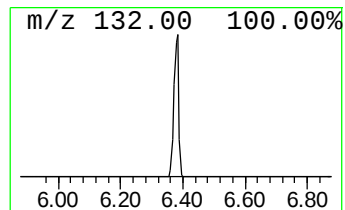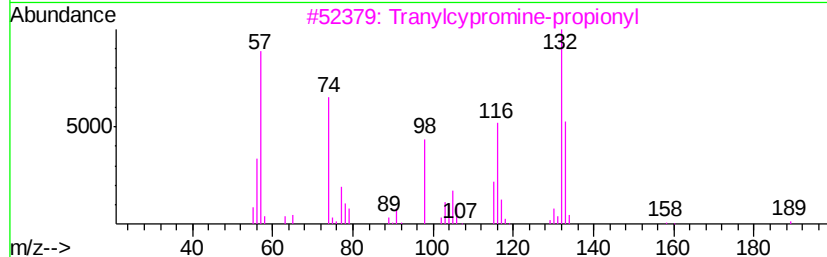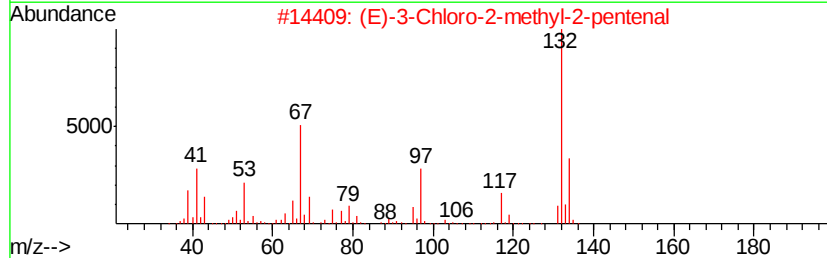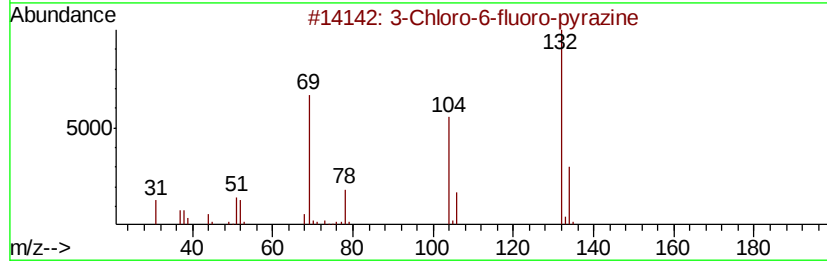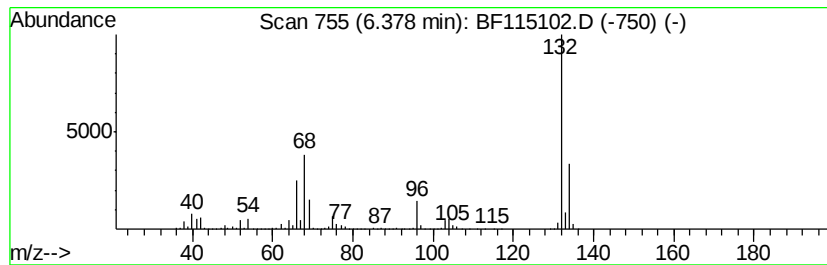

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
Data File : BF115102.D
Acq On : 22 Jun 2019 2:16
Operator : HP/JU
Sample : PB120818BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120818BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.38	6.38	79.0	ng	5780130	1	6.61	1462490	20.0