


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062119\
 Data File : BF115075.D
 Acq On : 21 Jun 2019 13:19
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 24 04:21:29 2019

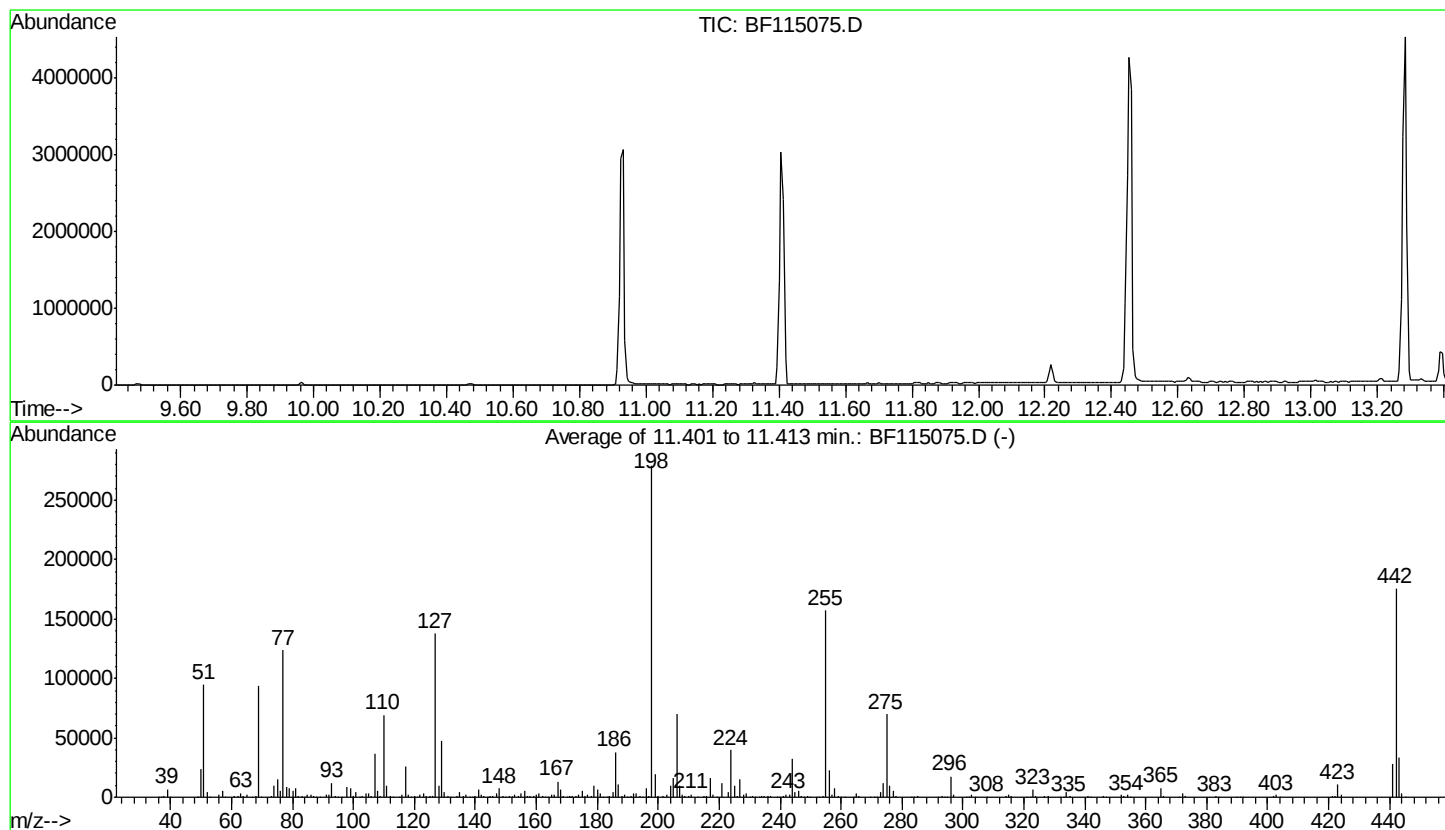

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	94746	PASS
68	69	0.00	2	1.3	1205	PASS
69	198	0.00	100	33.8	94240	PASS
70	69	0.00	2	0.2	155	PASS
127	198	10	80	49.3	137648	PASS
197	198	0.00	2	0.5	1320	PASS
198	198	100	100	100.0	279189	PASS
199	198	5	9	6.8	18959	PASS
275	198	10	60	25.0	69672	PASS
365	198	1	100	2.8	7745	PASS
441	198	0.01	100	10.0	27784	PASS
442	198	50	100	62.8	175309	PASS
443	442	15	24	19.0	33382	PASS