
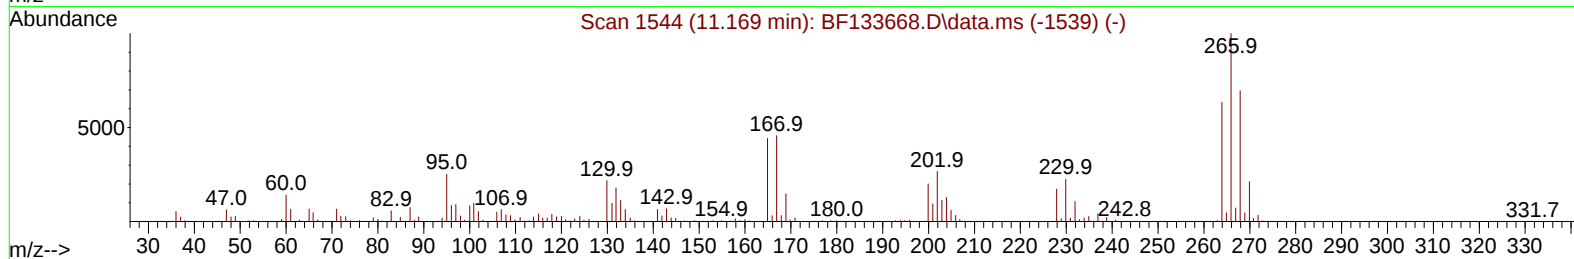
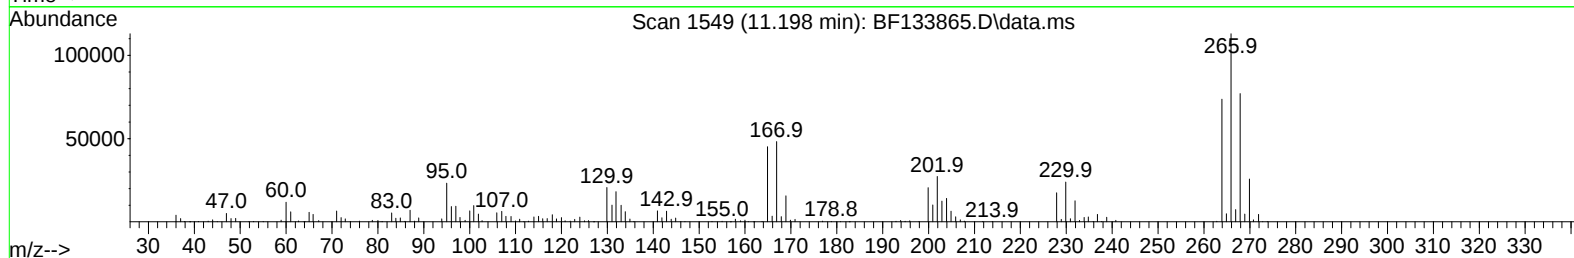


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062123\
Data File : BF133865.D
Acq On : 21 Jun 2023 12:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 12:59:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 13:43:46 2023
Response via : Initial Calibration

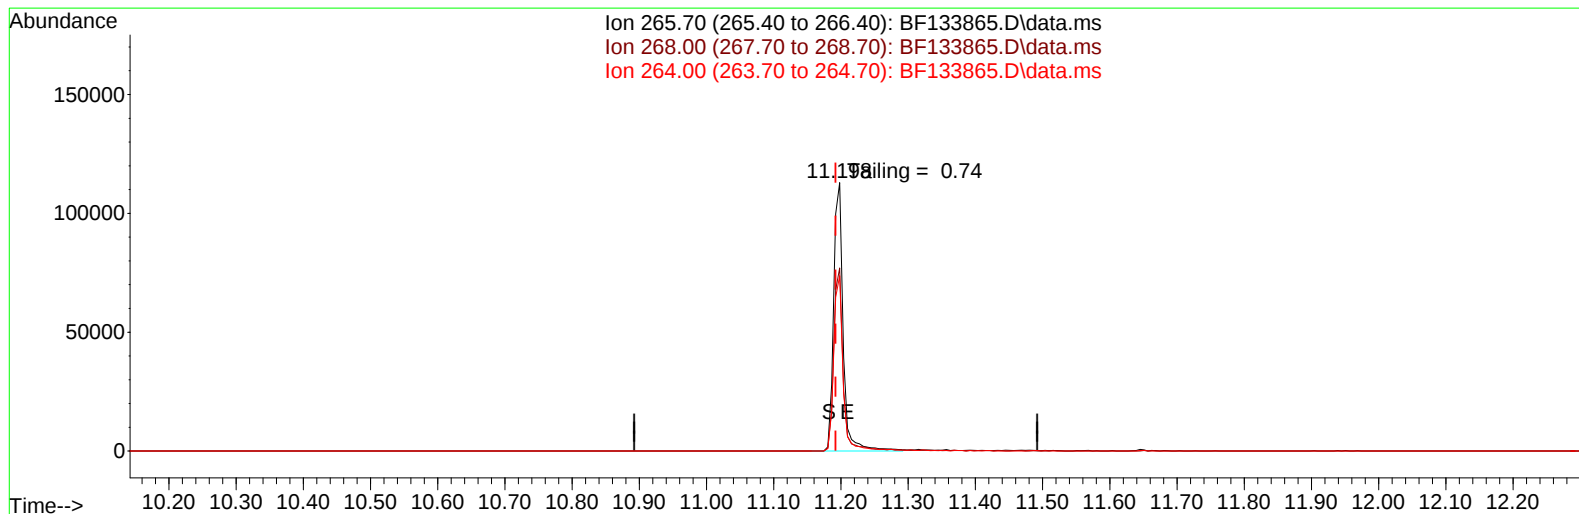

TIC: BF133865.D\data.ms

(70) Pentachlorophenol (C)




11.198min (+ 0.006) 21503.48 ng

response 111081

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	68.20
264.00	63.40	65.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062123\
Data File : BF133865.D
Acq On : 21 Jun 2023 12:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 21 12:59:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 13:43:46 2023
Response via : Initial Calibration

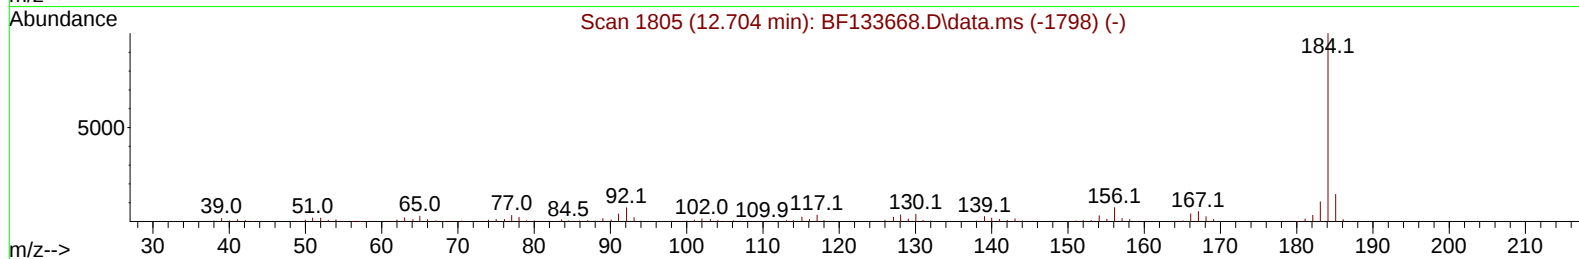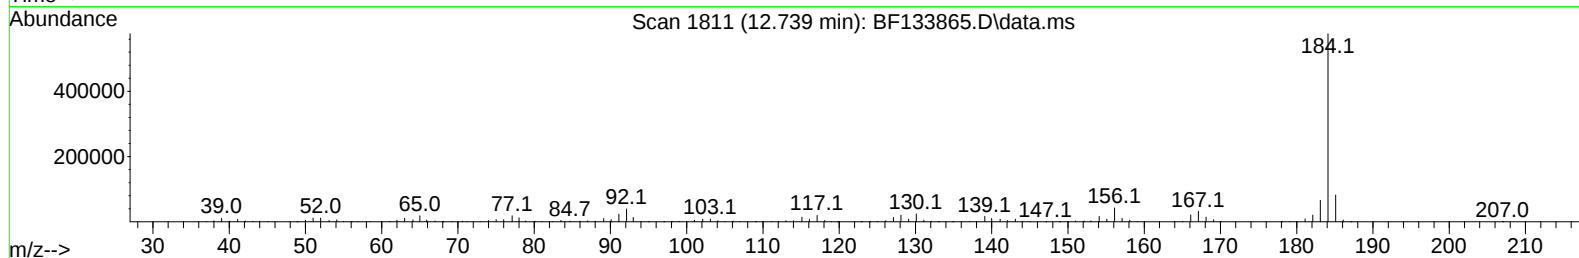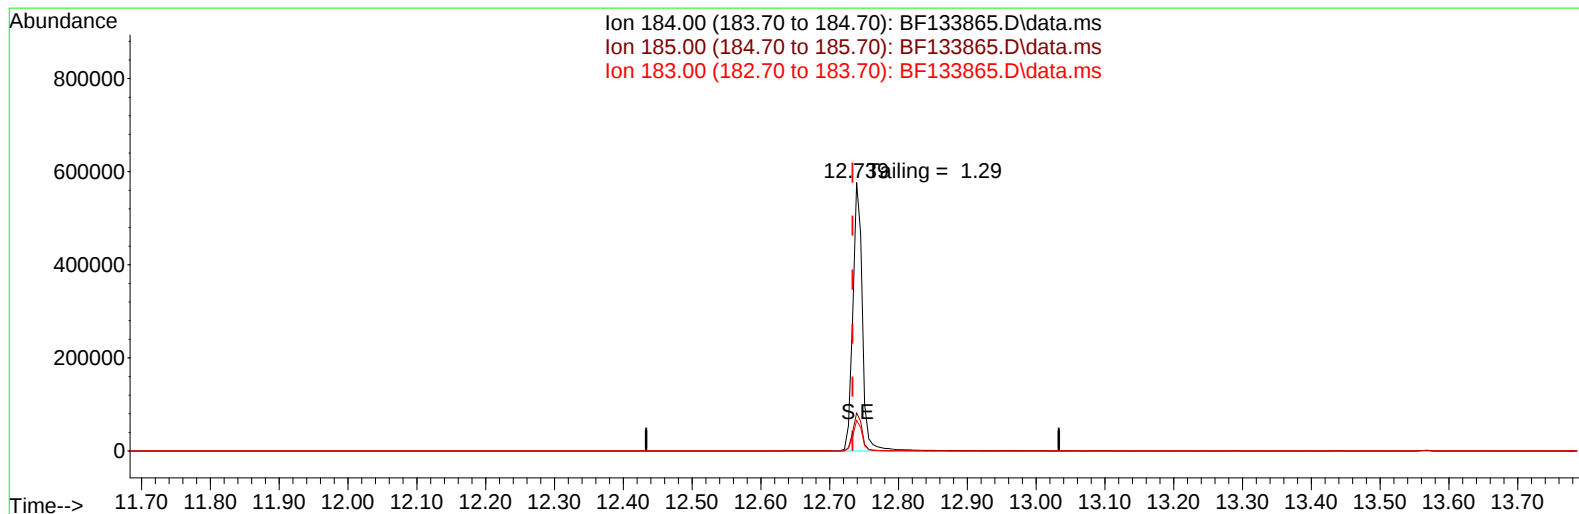

TIC: BF133865.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 65842.37 ng m

response 545723

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.28
183.00	10.50	11.47
0.00	0.00	0.00