
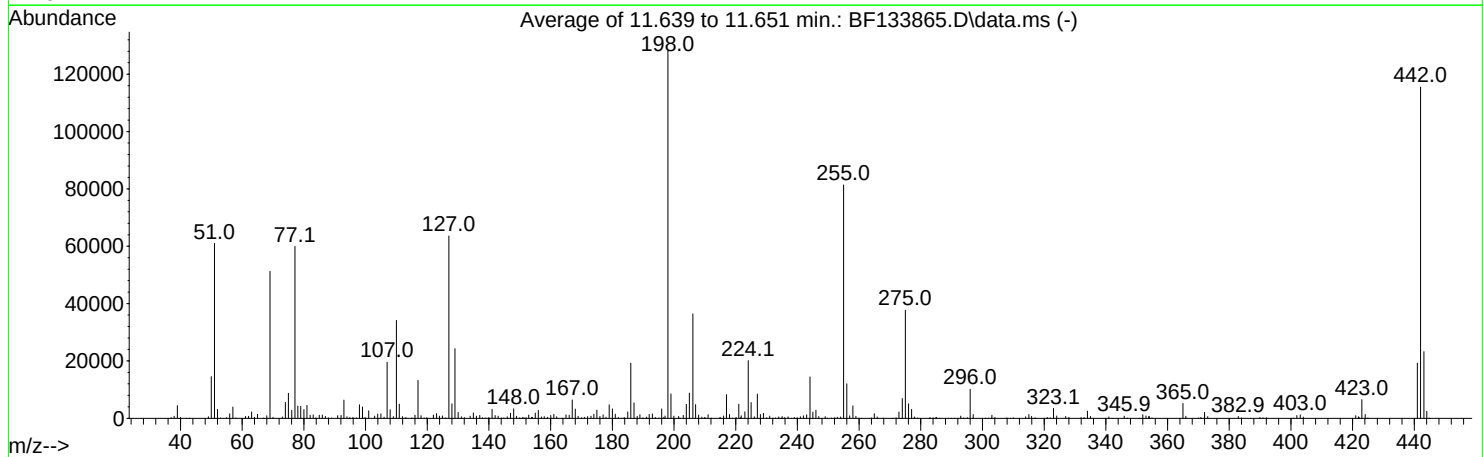


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062123\
Data File : BF133865.D
Acq On : 21 Jun 2023 12:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\BFDDTBREAKDOWN-8270.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 01 16:14:27 2010

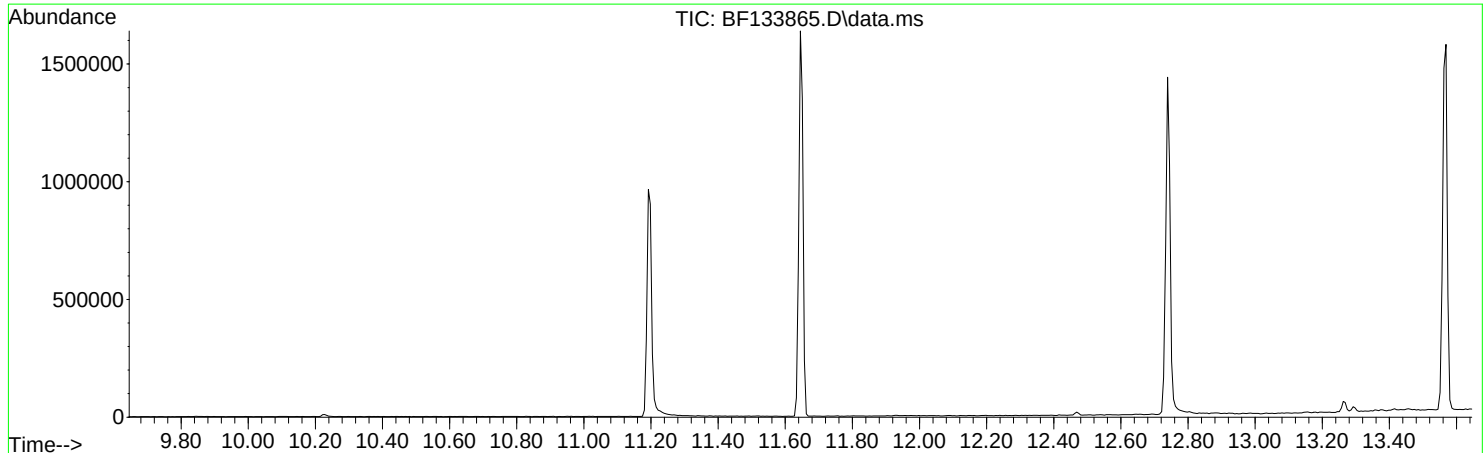




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.6	61029	PASS
68	69	0.00	2	1.7	890	PASS
69	198	0.00	100	39.9	51238	PASS
70	69	0.00	2	0.7	340	PASS
127	198	10	80	49.5	63568	PASS
197	198	0.00	2	0.6	830	PASS
198	198	100	100	100.0	128299	PASS
199	198	5	9	6.6	8489	PASS
275	198	10	60	29.4	37713	PASS
365	198	1	100	4.0	5139	PASS
441	442	0.01	24	16.6	19229	PASS
442	198	50	100	90.0	115507	PASS
443	442	15	24	20.1	23266	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062123\
 Data File : BF133865.D
 Acq On : 21 Jun 2023 12:01
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 21 12:59:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 13:43:46 2023
 Response via : Initial Calibration

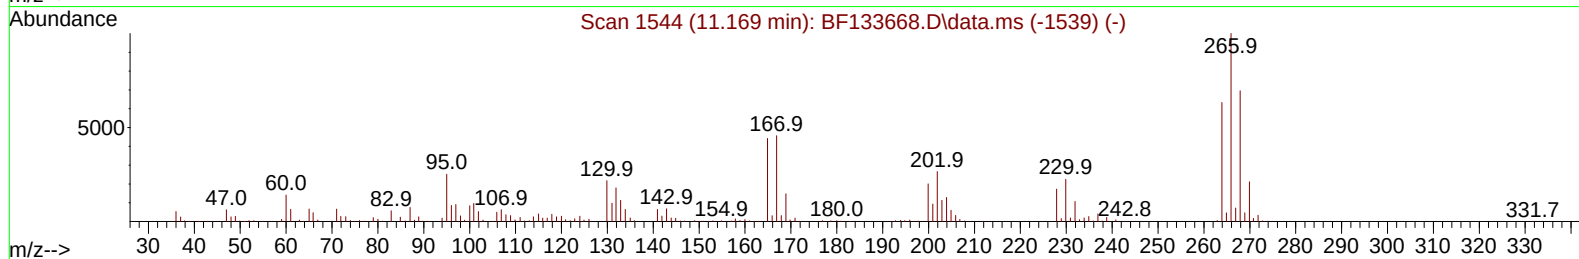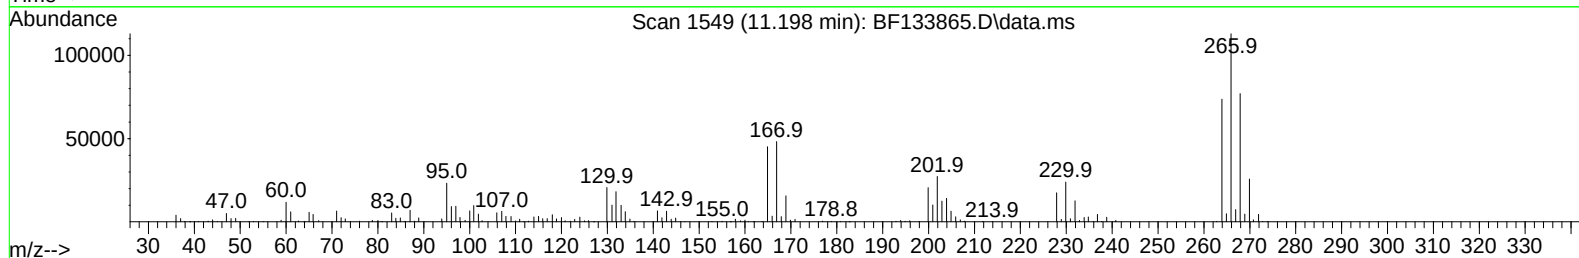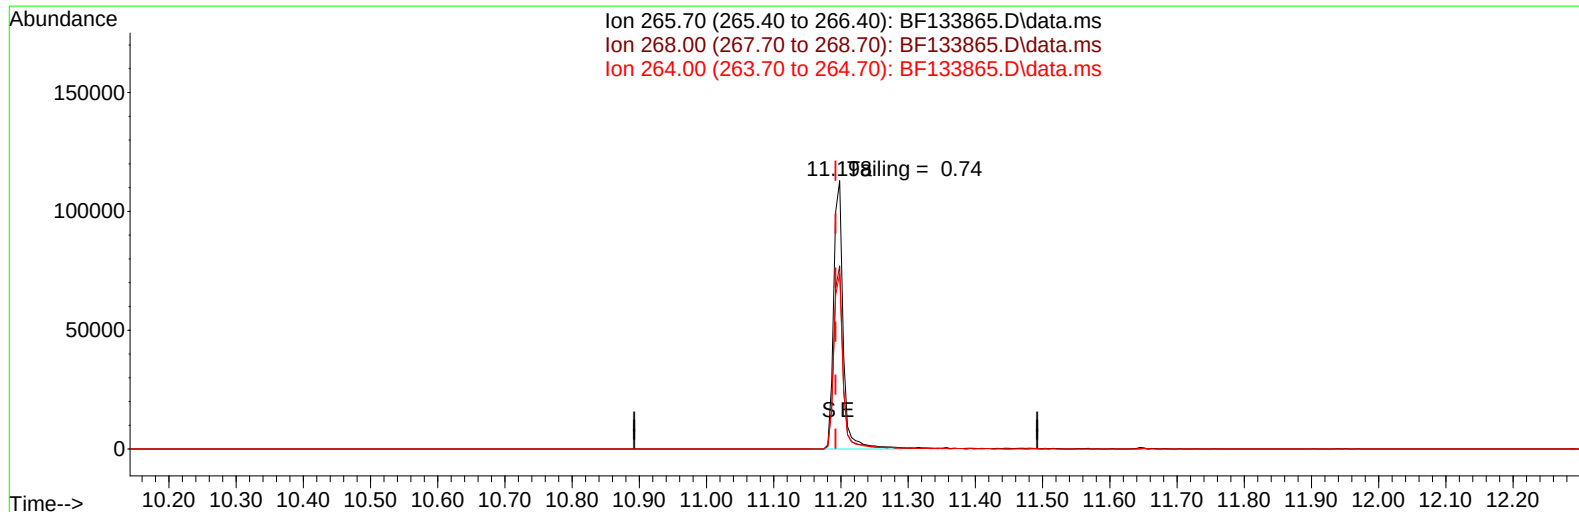

TIC: BF133865.D\data.ms

(70) Pentachlorophenol (C)

11.198min (+ 0.006) 21503.48 ng




response 111081

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	68.20
264.00	63.40	65.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062123\
Data File : BF133865.D
Acq On : 21 Jun 2023 12:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 21 12:59:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 13:43:46 2023
Response via : Initial Calibration

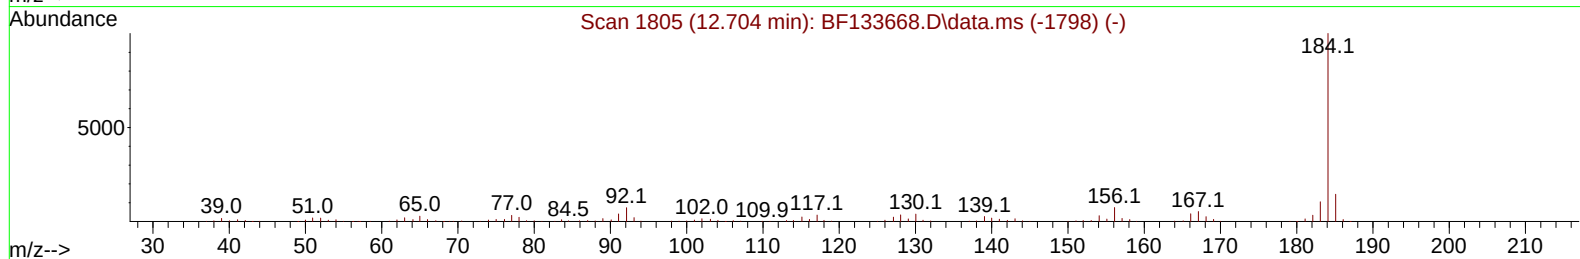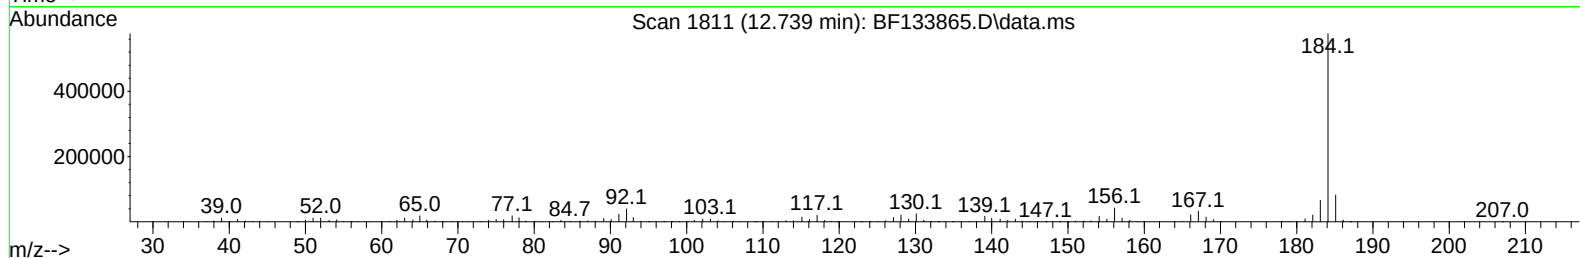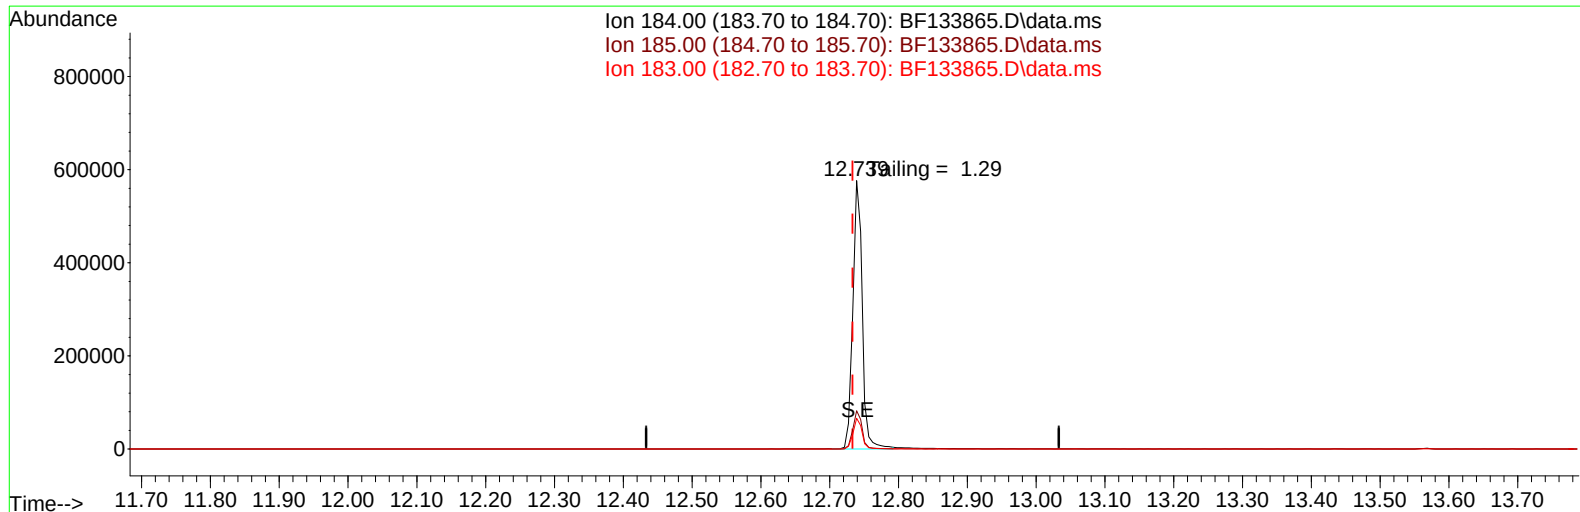

TIC: BF133865.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 65842.37 ng m

response 545723

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.28
183.00	10.50	11.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/21/2023	BNA_F	<u>BF133865.D</u>
Compound Name	Response	Retention Time
DDT	284208	13.568
DDD	11530	13.268
DDE	243	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11773	295981	3.98

Instrument :
BNA_F
ClientSampleId :
DFTPP