

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062218\
 Data File : BF106729.D
 Acq On : 23 Jun 2018 00:34
 Operator : JU/SJ
 Sample : J3573-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-49-COMP

Quant Time: Jun 23 01:21:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 22 11:34:03 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.96	152	48104	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	174812	20.00	ng	0.00
38) Acenaphthene-d10	10.00	164	81366	20.00	ng	0.00
63) Phenanthrene-d10	11.49	188	134273	20.00	ng	-0.01
75) Chrysene-d12	14.14	240	132871	20.00	ng	-0.01
86) Perylene-d12	15.68	264	115372	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	364328	128.25	ng	0.00
7) Phenol-d6	6.60	99	464115	130.82	ng	0.00
23) Nitrobenzene-d5	7.52	82	303995	96.64	ng	0.00
41) 2,4,6-Tribromophenol	10.80	330	130105	137.96	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	540142	118.11	ng	0.00
78) Terphenyl-d14	13.08	244	513890	93.68	ng	0.00
Target Compounds						
9) Benzaldehyde	6.74	77	8219	2.743	ng	Qvalue 85
10) Phenol	6.61	94	8884	2.194	ng	85
19) n-Nitroso-di-n-propylamine	7.52	70	39147	16.740	ng	# 73
25) Isophorone	7.52	82	303991	54.842	ng	# 64
49) Dimethylphthalate	9.71	163	72114	11.817	ng	99
56) 2,4-Dinitrotoluene	10.00	165	10220	6.059	ng	# 21
66) 4-Bromophenyl-phenylether	10.80	248	7941	4.955	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062218\
Data File : BF106729.D
Acq On : 23 Jun 2018 00:34
Operator : JU/SJ
Sample : J3573-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-49-COMP

Quant Time: Jun 23 01:21:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 22 11:34:03 2018
Response via : Initial Calibration

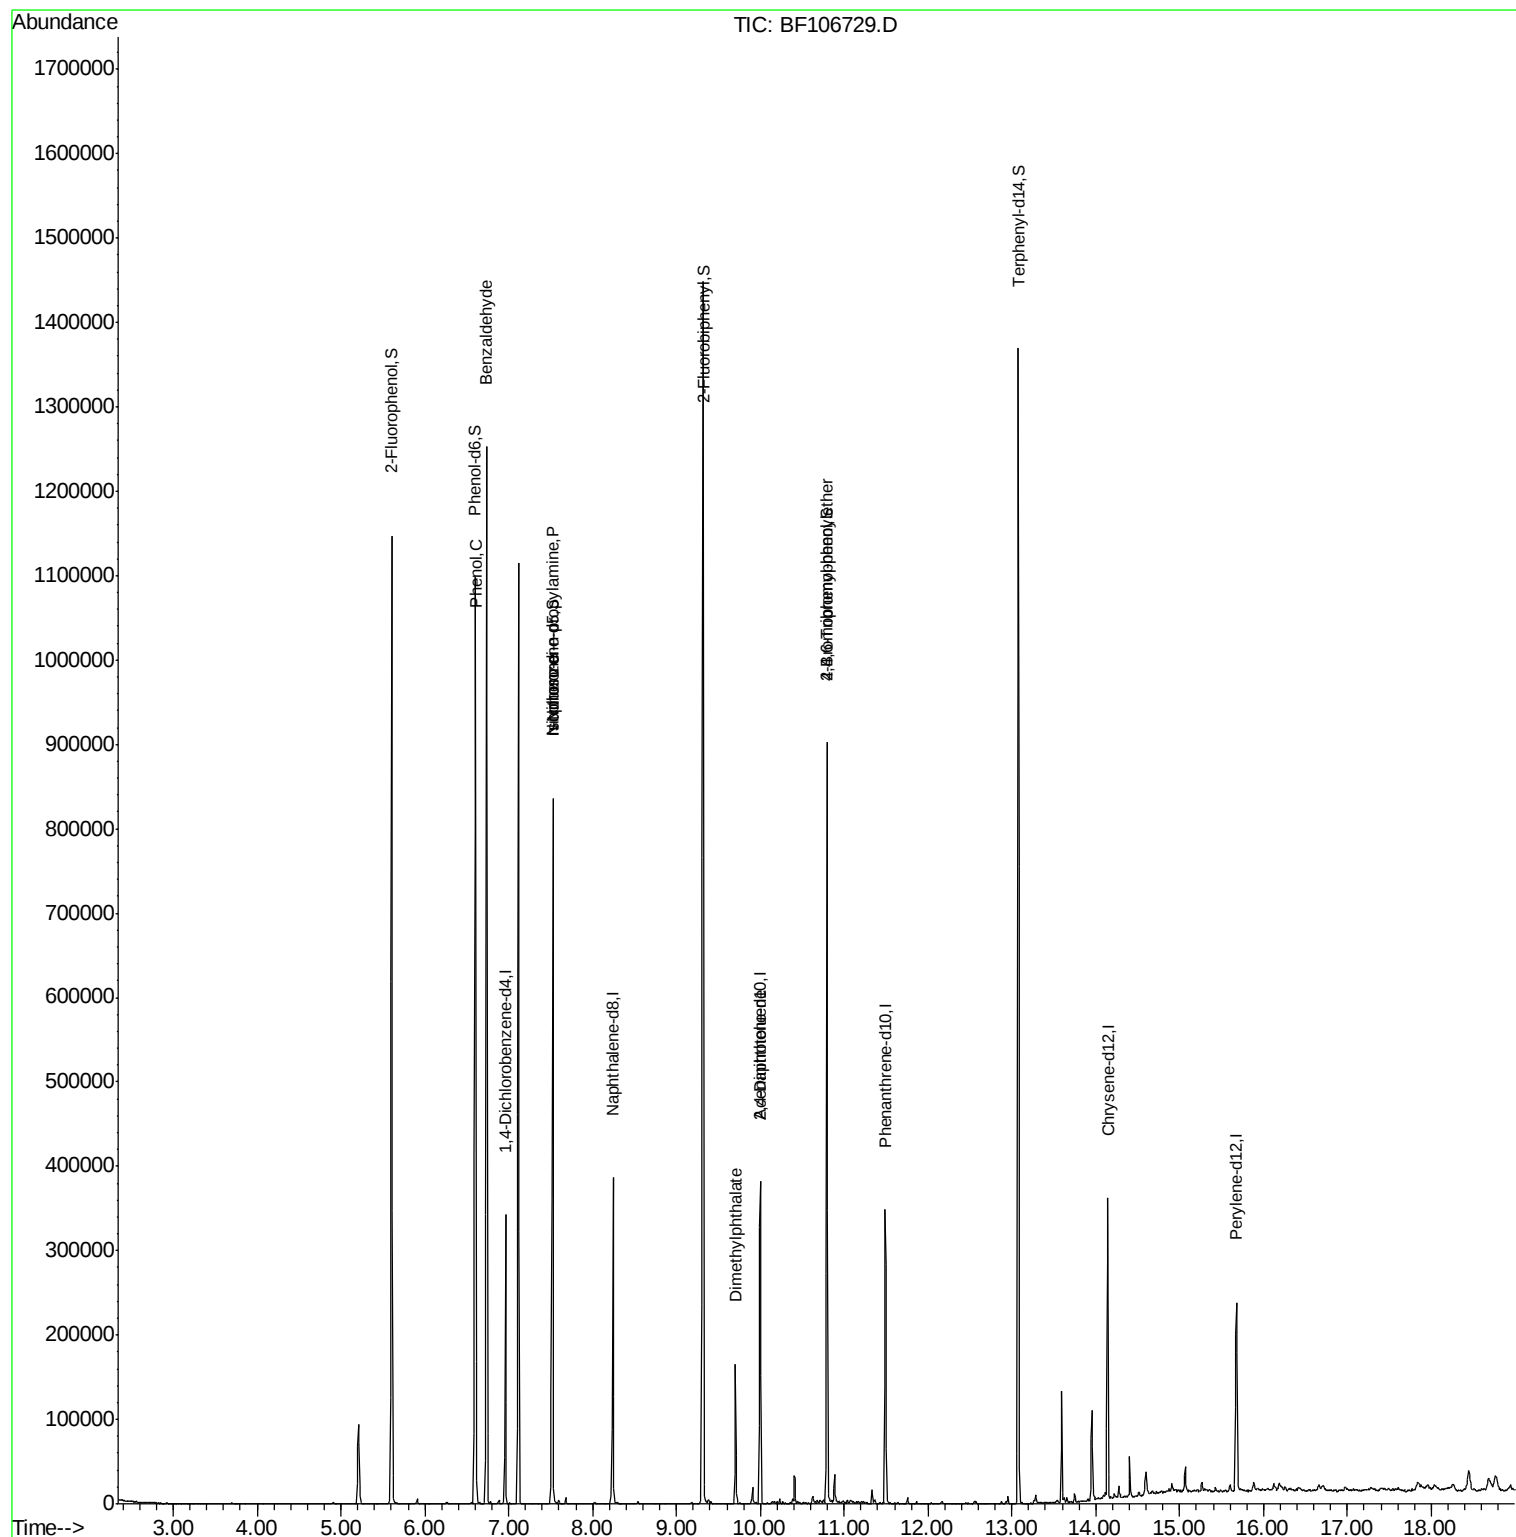

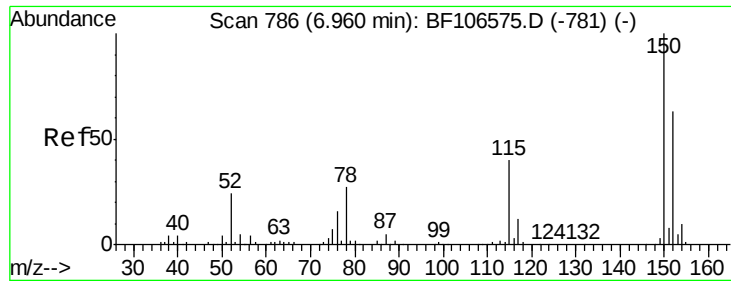


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.96 min Scan# 786
Delta R.T. -0.00 min
Lab File: BF106729.D
Acq: 23 Jun 2018 00:34

Instrument :
BNA_F
ClientSampleId :
SB-49-COMP

Tgt Ion:152 Resp: 48104
Ion Ratio Lower Upper
152 100
150 155.4 124.6 186.8
115 57.6 50.1 75.1

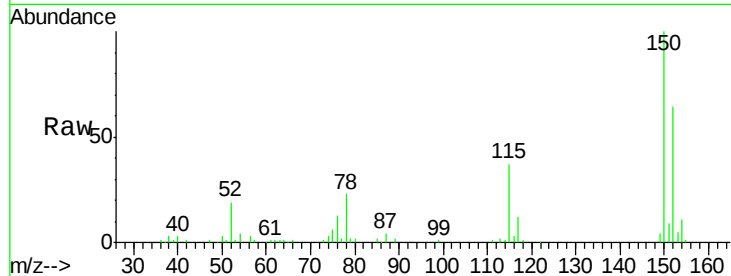


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

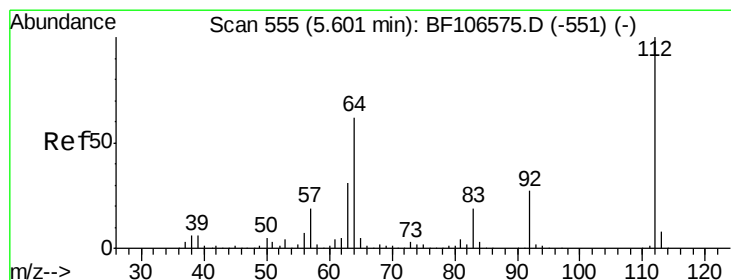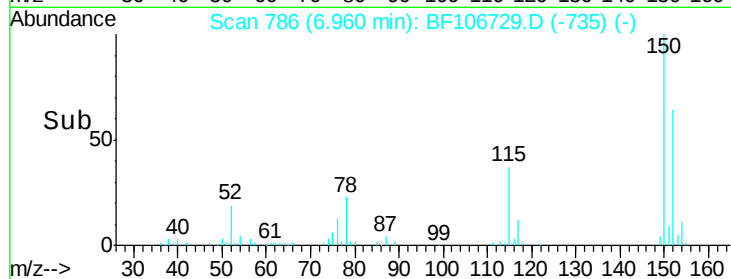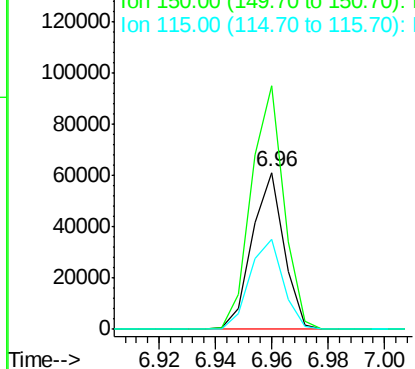



#5


2-Fluorophenol
Concen: 128.248 ng
RT: 5.61 min Scan# 556
Delta R.T. 0.01 min
Lab File: BF106729.D
Acq: 23 Jun 2018 00:34

Tgt Ion:112 Resp: 364328
Ion Ratio Lower Upper
112 100
64 55.8 47.9 71.9
63 27.8 23.7 35.5

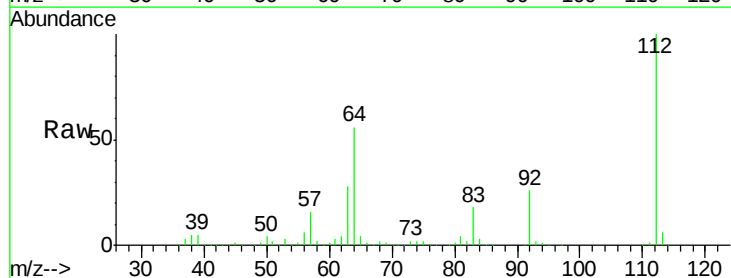

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

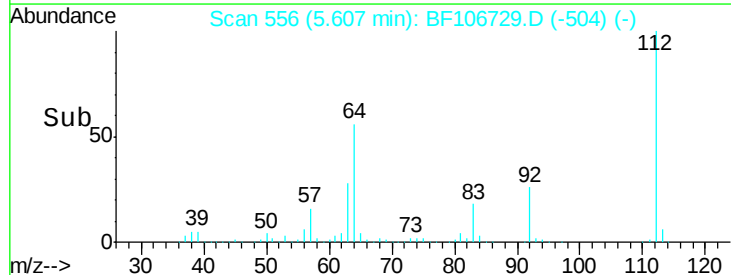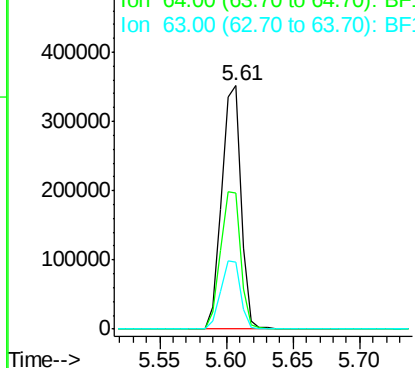

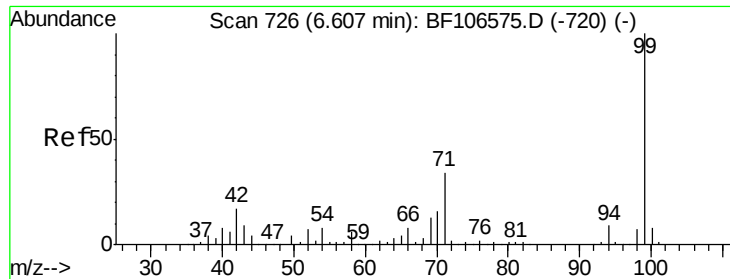

#7

Phenol-d6

Concen: 130.824 ng

RT: 6.60 min Scan# 725

Delta R.T. -0.01 min

Lab File: BF106729.D

Acq: 23 Jun 2018 00:34

Instrument :

BNA_F

ClientSampleId :

SB-49-COMP


Tgt Ion: 99 Resp: 464115

Ion Ratio Lower Upper

99 100

42 16.6 14.5 21.7




71 34.4 25.4 38.0

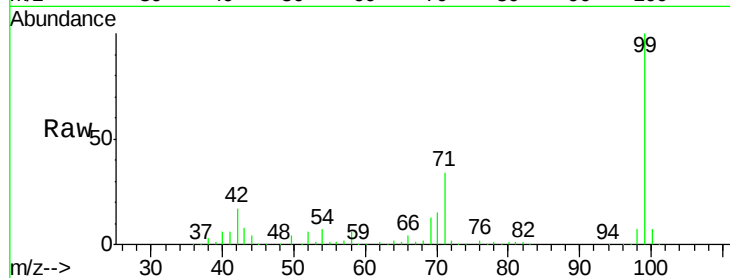

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

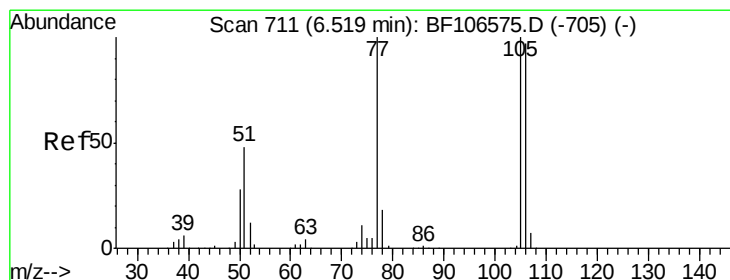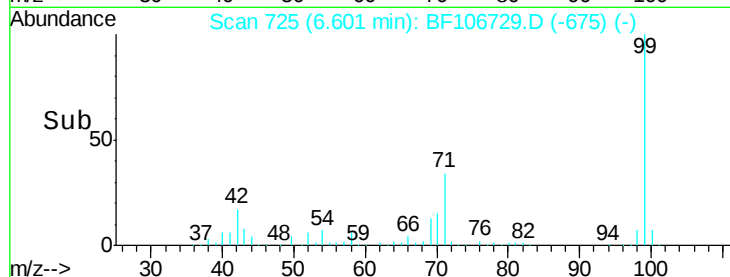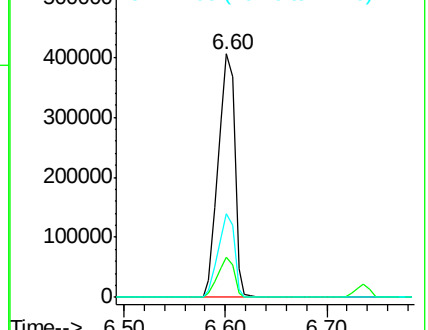

#9

Benzaldehyde

Concen: 2.743 ng

RT: 6.74 min Scan# 748

Delta R.T. 0.22 min

Lab File: BF106729.D

Acq: 23 Jun 2018 00:34


Tgt Ion: 77 Resp: 8219

Ion Ratio Lower Upper

77 100

105 84.0 81.1 121.1



106 81.6 74.5 114.5

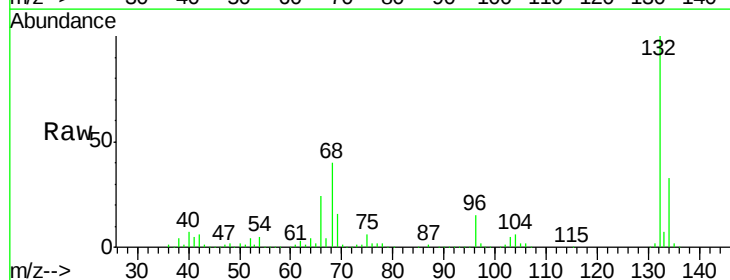


Abundance Ion 77.00 (76.70 to 77.70): BF1

Ion 105.00 (104.70 to 105.70): BF1

Ion 106.00 (105.70 to 106.70): BF1

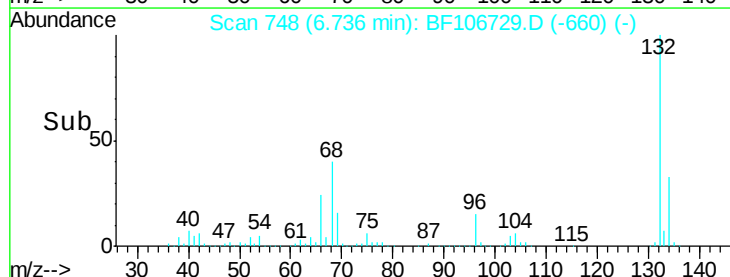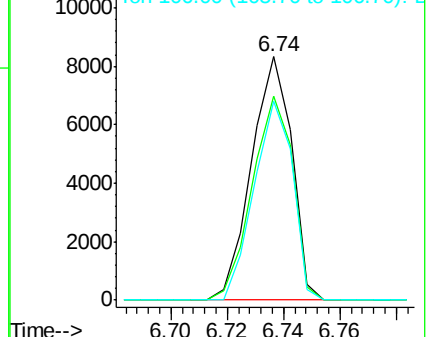

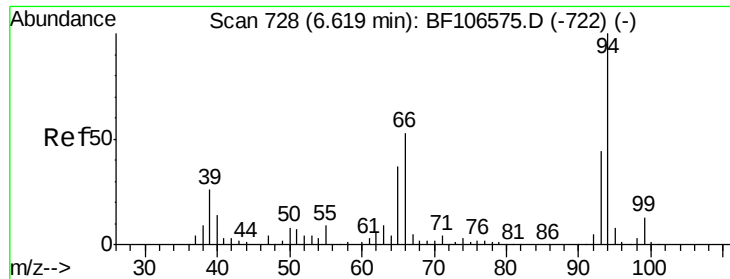

#10

Phenol

Concen: 2.194 ng

RT: 6.61 min Scan# 727

Delta R.T. -0.01 min

Lab File: BF106729.D

Acq: 23 Jun 2018 00:34

Instrument :

BNA_F

ClientSampleId :

SB-49-COMP


Tgt Ion: 94 Resp: 8884

Ion Ratio Lower Upper

94 100

65 31.4 7.9 47.9




66 49.2 16.2 56.2

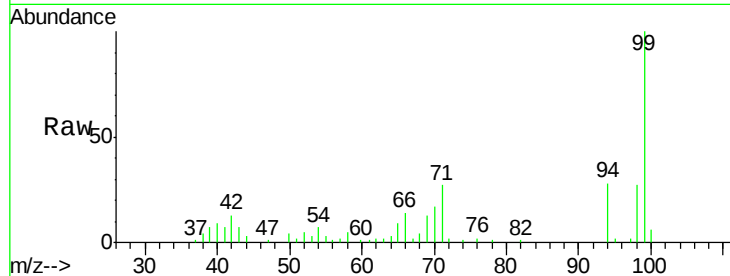

Abundance Ion 94.00 (93.70 to 94.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

Ion 66.00 (65.70 to 66.70): BF1

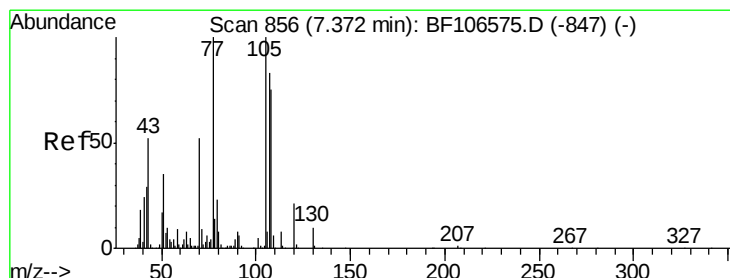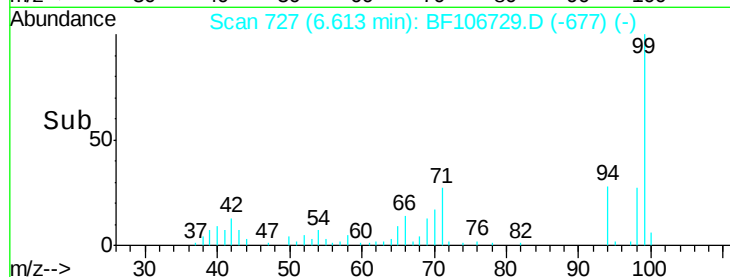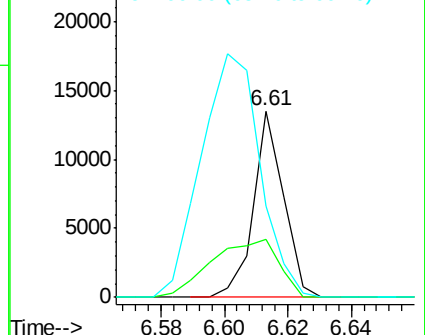

#19

n-Nitroso-di-n-propylamine

Concen: 16.740 ng

RT: 7.52 min Scan# 882

Delta R.T. 0.15 min

Lab File: BF106729.D

Acq: 23 Jun 2018 00:34

Tgt Ion: 70 Resp: 39147


Ion Ratio Lower Upper

70 100

42 42.2 47.5 71.3#

101 0.0 7.4 11.2#

130 2.4 16.6 25.0#


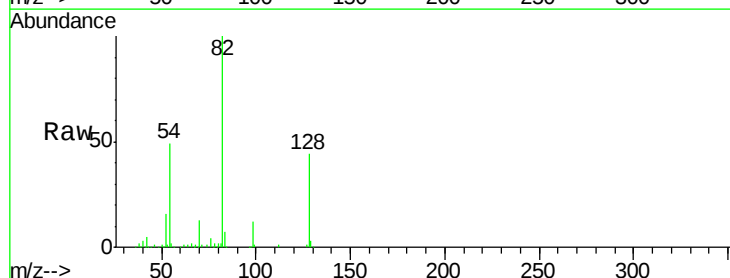



Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

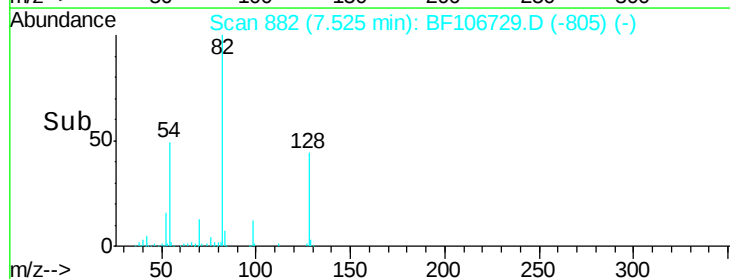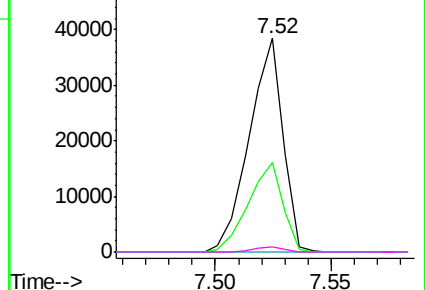


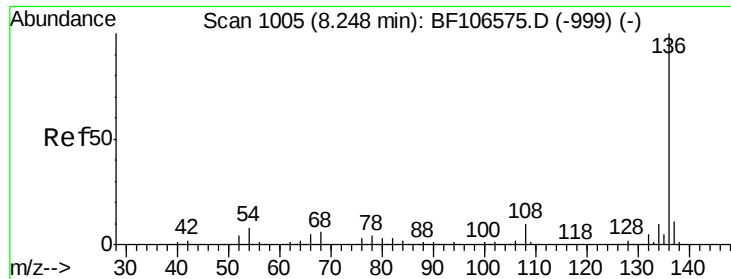




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.24 min Scan# 1004
Delta R.T. -0.01 min
Lab File: BF106729.D
Acq: 23 Jun 2018 00:34

Instrument :
BNA_F
ClientSampleId :
SB-49-COMP

Tgt Ion: 136 Resp: 174812
Ion Ratio Lower Upper
136 100
137 10.6 8.9 13.3
54 7.7 6.6 9.8
68 5.9 5.0 7.4

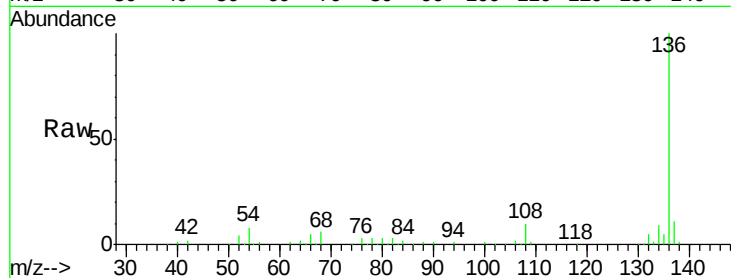


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

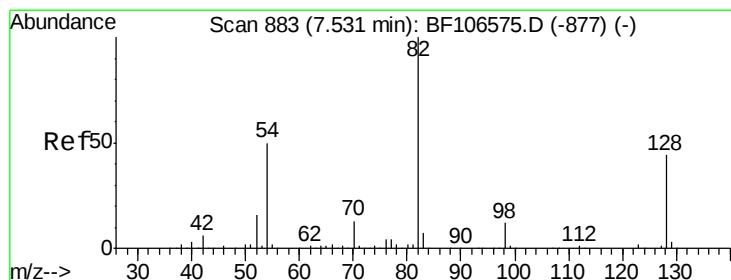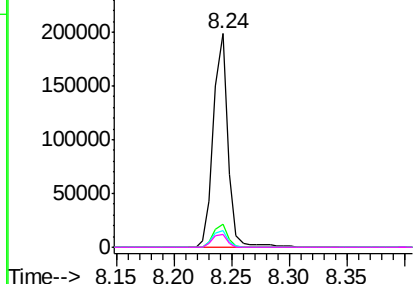
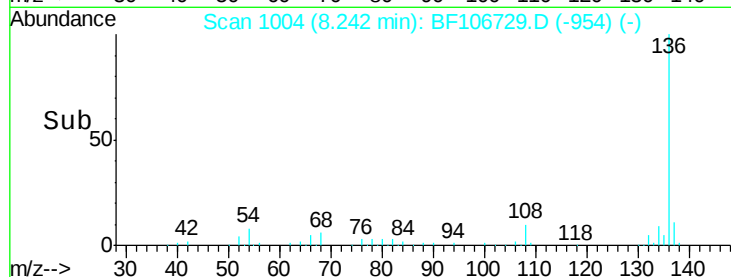



#23
Nitrobenzene-d5
Concen: 96.641 ng
RT: 7.52 min Scan# 882
Delta R.T. -0.01 min
Lab File: BF106729.D
Acq: 23 Jun 2018 00:34

Tgt Ion: 82 Resp: 303995
Ion Ratio Lower Upper
82 100
128 44.4 36.1 54.1
54 48.7 41.4 62.2

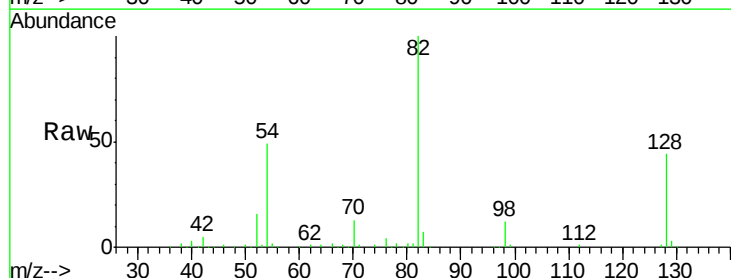

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

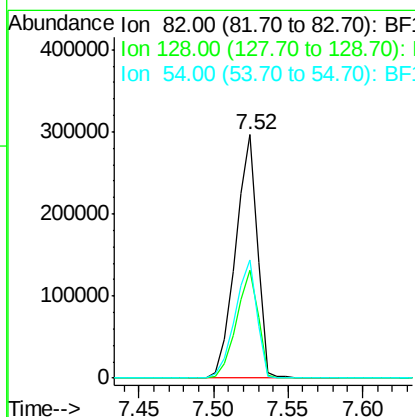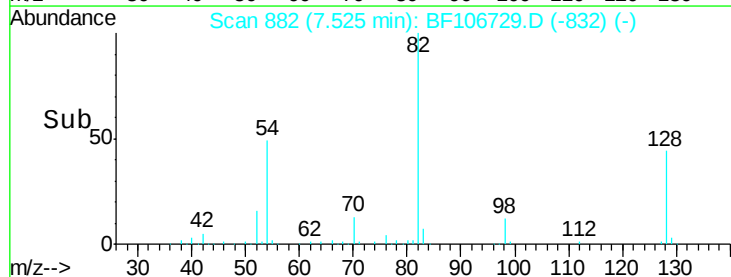

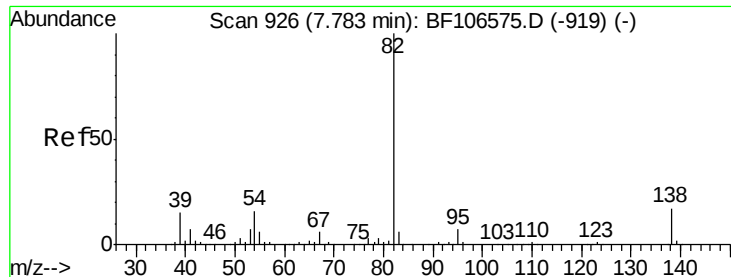

#25

Isophorone

Concen: 54.842 ng

RT: 7.52 min Scan# 882

Delta R.T. -0.26 min

Lab File: BF106729.D

Acq: 23 Jun 2018 00:34

Instrument :

BNA_F

ClientSampleId :

SB-49-COMP





Tgt Ion: 82 Resp: 303991

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

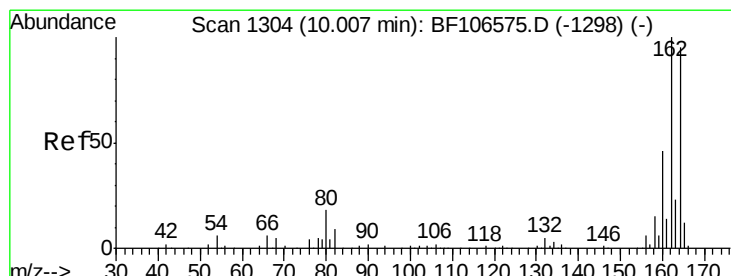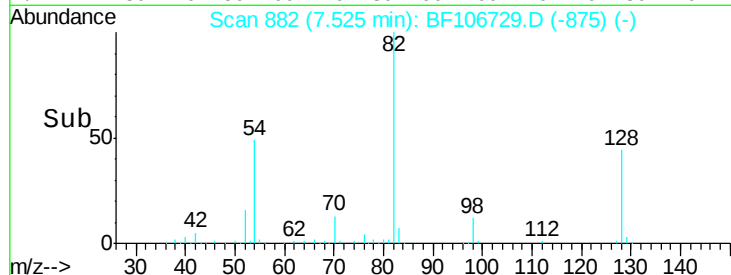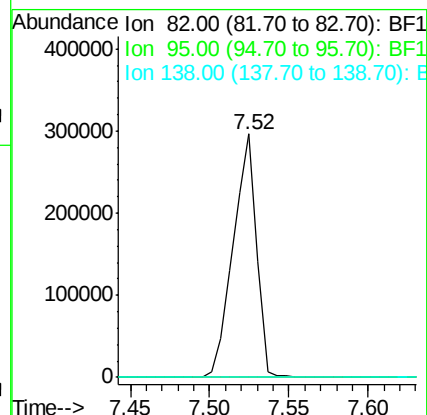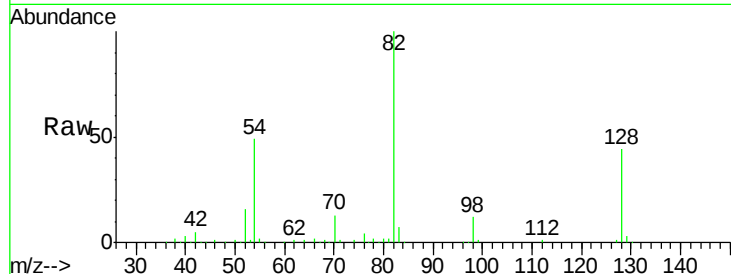

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.00 min Scan# 1303

Delta R.T. -0.01 min

Lab File: BF106729.D

Acq: 23 Jun 2018 00:34




Tgt Ion: 164 Resp: 81366


Ion Ratio Lower Upper

164 100

162 95.9 86.1 129.1

160 45.2 38.3 57.5

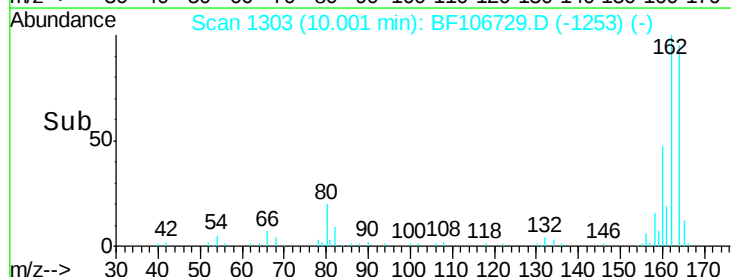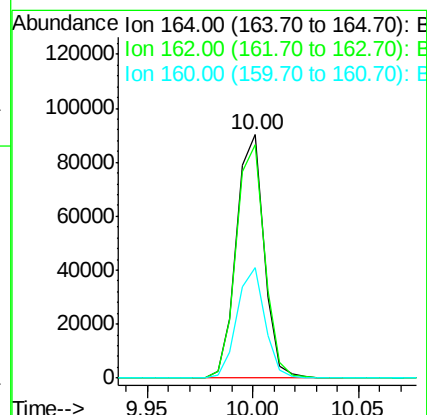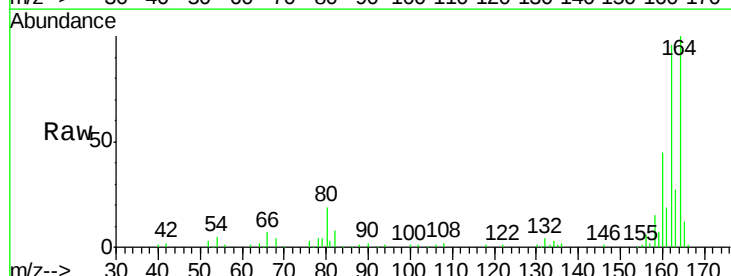


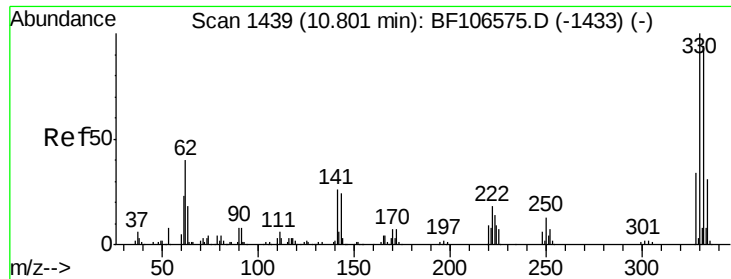




#41
 2,4,6-Tribromophenol
 Concen: 137.961 ng
 RT: 10.80 min Scan# 1438
 Delta R.T. -0.01 min
 Lab File: BF106729.D
 Acq: 23 Jun 2018 00:34

Instrument :
 BNA_F
 ClientSampleId :
 SB-49-COMP

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.3	77.0	115.6
141	22.9	29.9	44.9#

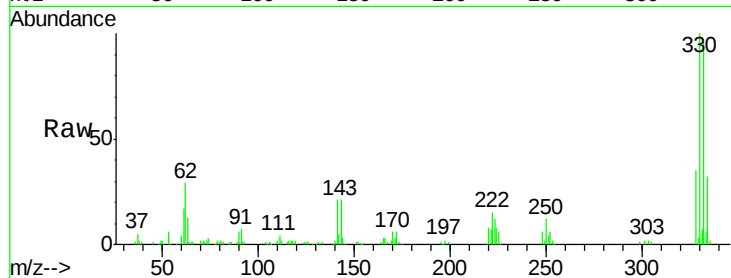


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

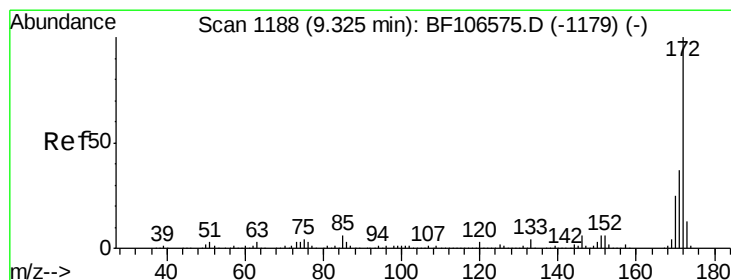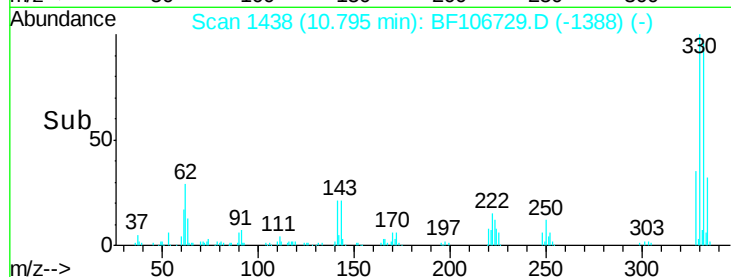
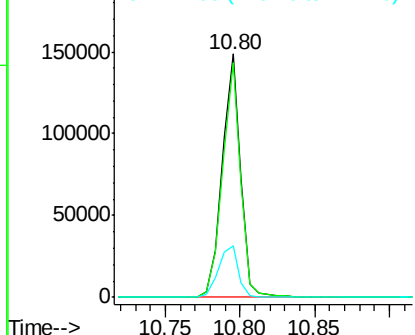



#44
 2-Fluorobiphenyl
 Concen: 118.110 ng
 RT: 9.32 min Scan# 1187
 Delta R.T. -0.01 min
 Lab File: BF106729.D
 Acq: 23 Jun 2018 00:34

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	29.7	44.5
170	24.7	19.6	29.4

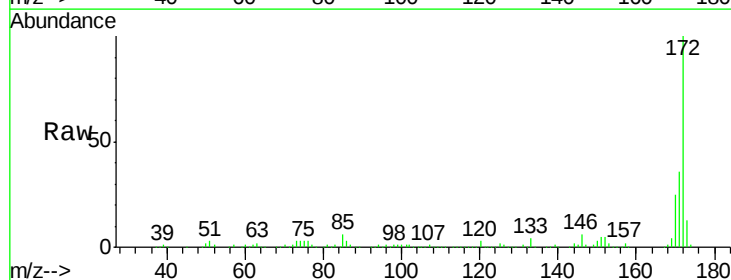

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

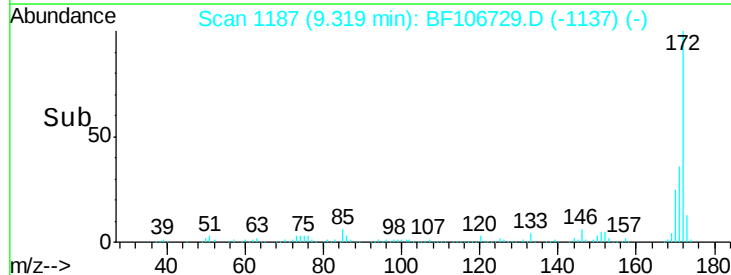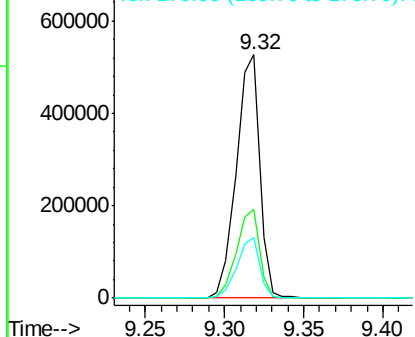


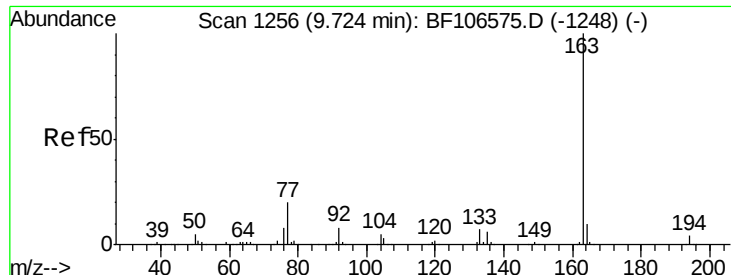




#49
Dimethylphthalate
Concen: 11.817 ng
RT: 9.71 min Scan# 1253
Delta R.T. -0.02 min
Lab File: BF106729.D
Acq: 23 Jun 2018 00:34

Instrument :
BNA_F
ClientSampleId :
SB-49-COMP

Tgt Ion:163 Resp: 72114
Ion Ratio Lower Upper
163 100
194 3.5 2.7 4.1
164 10.6 8.2 12.2

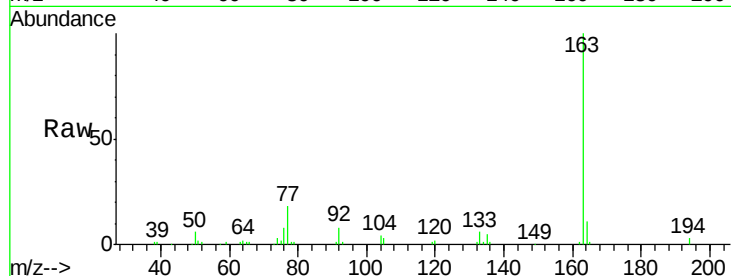


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

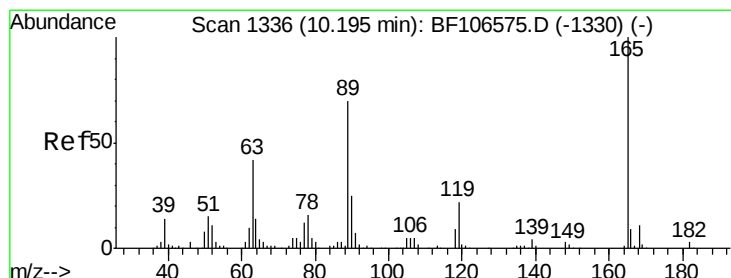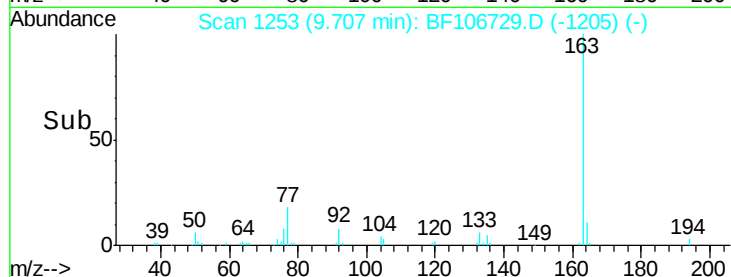
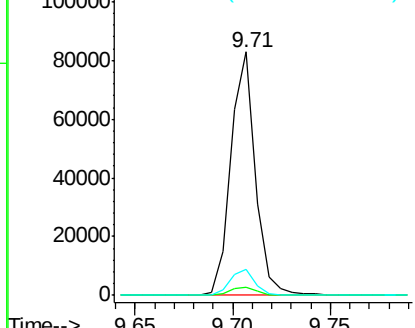



#56
2,4-Dinitrotoluene
Concen: 6.059 ng
RT: 10.00 min Scan# 1303
Delta R.T. -0.19 min
Lab File: BF106729.D
Acq: 23 Jun 2018 00:34

Tgt Ion:165 Resp: 10220
Ion Ratio Lower Upper
165 100
63 0.0 36.4 54.6#
89 0.0 57.8 86.6#
182 0.0 1.6 2.4#

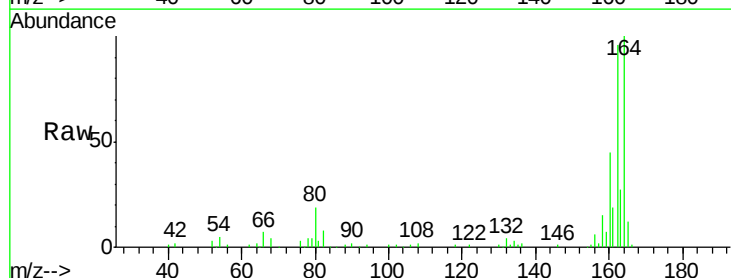

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1
Ion 182.00 (181.70 to 182.70): E



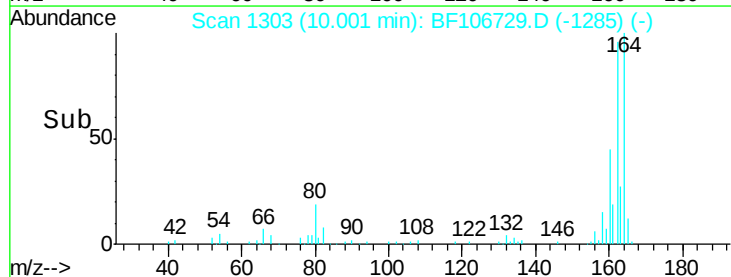
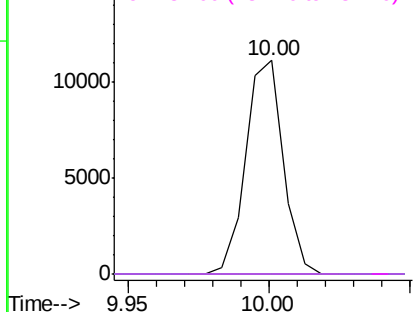


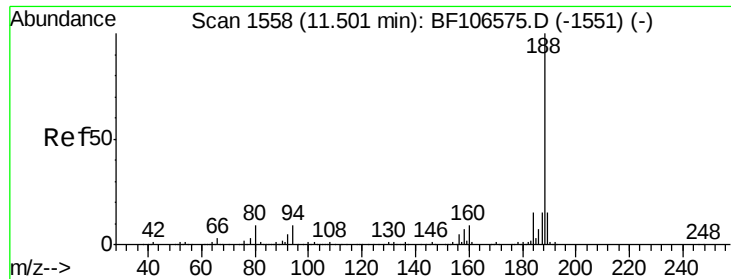

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.49 min Scan# 1556
Delta R.T. -0.01 min
Lab File: BF106729.D
Acq: 23 Jun 2018 00:34




Instrument :
BNA_F
ClientSampleId :
SB-49-COMP


Tgt Ion:188 Resp: 134273
Ion Ratio Lower Upper
188 100
94 9.2 8.5 12.7
80 10.0 9.2 13.8

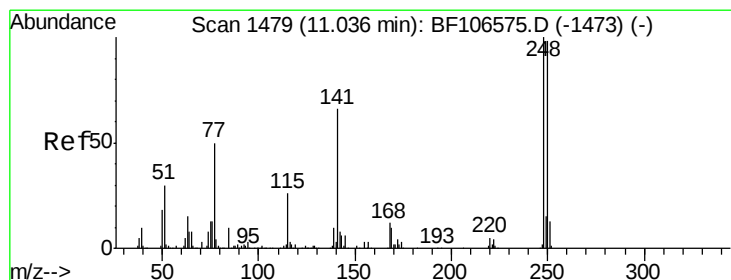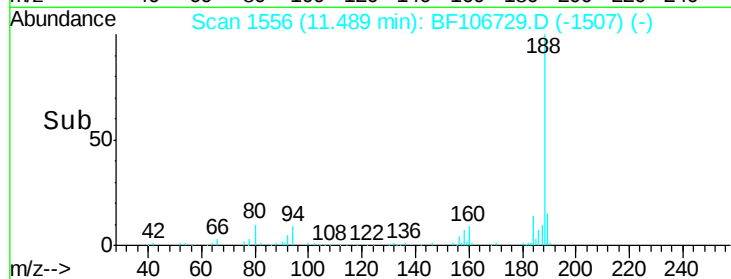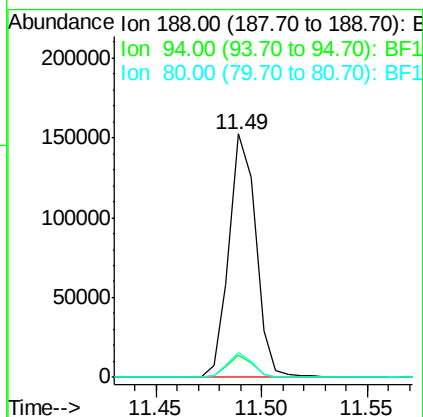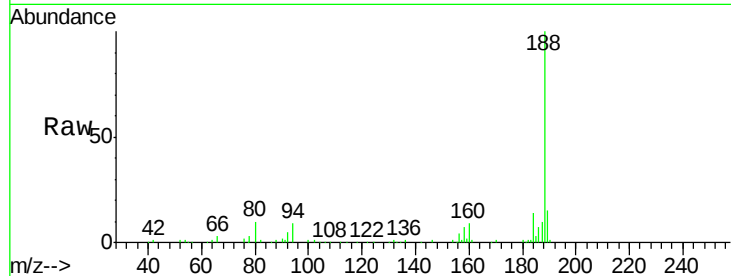

#66
4-Bromophenyl-phenylether
Concen: 4.955 ng
RT: 10.80 min Scan# 1438
Delta R.T. -0.24 min
Lab File: BF106729.D
Acq: 23 Jun 2018 00:34

Tgt Ion:248 Resp: 7941
Ion Ratio Lower Upper
248 100
250 200.4 76.9 115.3#
141 352.1 74.4 111.6#


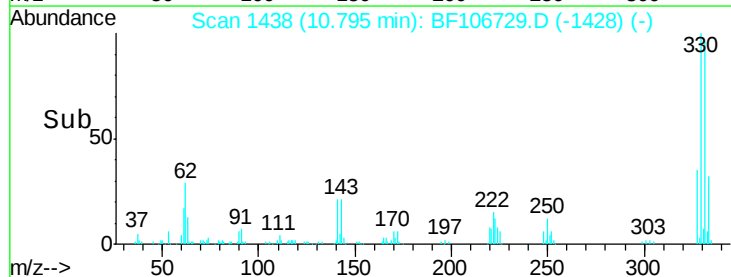
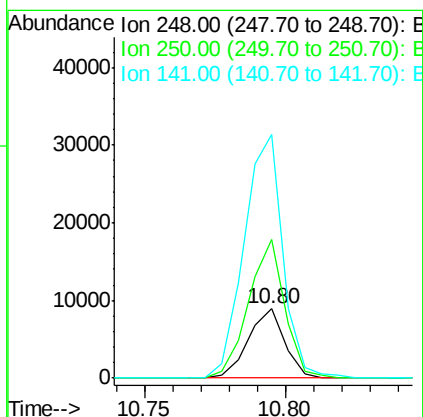
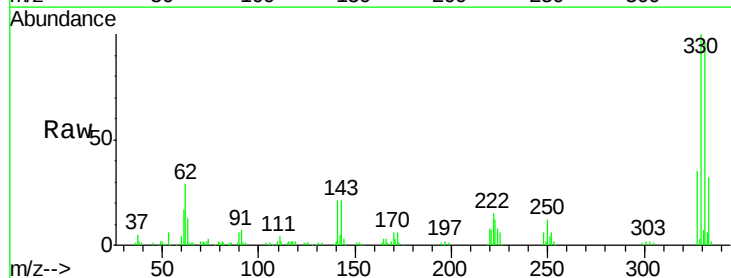


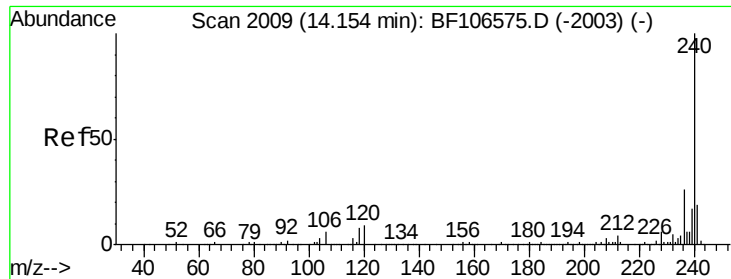

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.14 min Scan# 2007
Delta R.T. -0.01 min
Lab File: BF106729.D
Acq: 23 Jun 2018 00:34




Instrument :
BNA_F
ClientSampleId :
SB-49-COMP


Tgt Ion: 240 Resp: 132871
Ion Ratio Lower Upper
240 100
120 8.9 9.5 14.3#
236 26.2 20.7 31.1

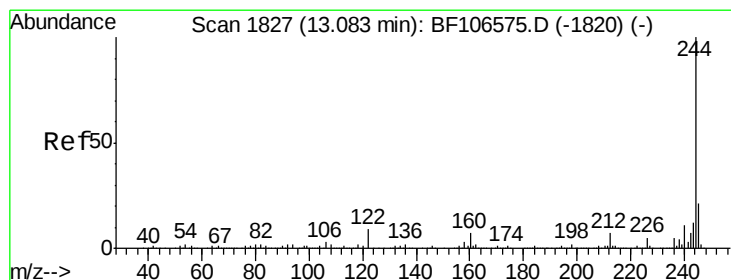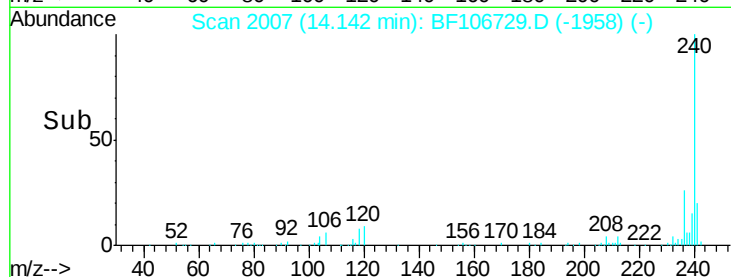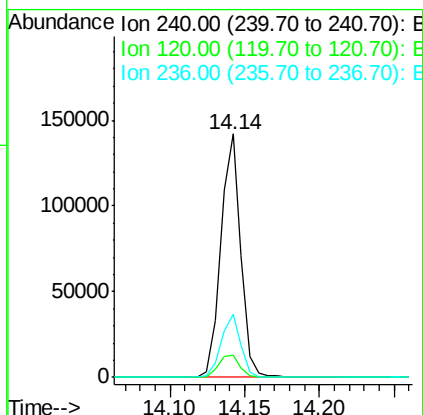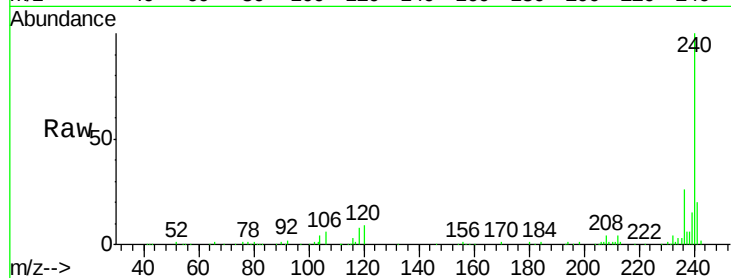

#78
Terphenyl-d14
Concen: 93.684 ng
RT: 13.08 min Scan# 1826
Delta R.T. -0.01 min
Lab File: BF106729.D
Acq: 23 Jun 2018 00:34

Tgt Ion: 244 Resp: 513890
Ion Ratio Lower Upper
244 100
212 6.6 5.4 8.0
122 8.7 11.0 16.4#

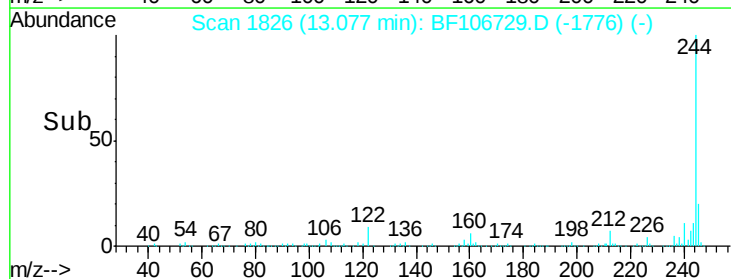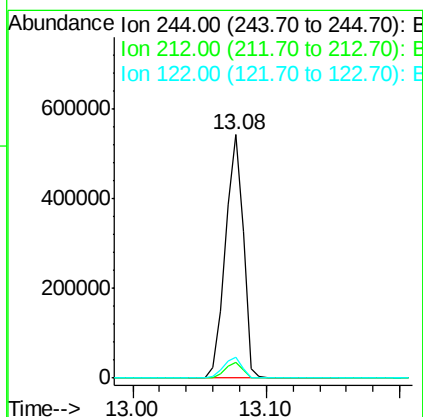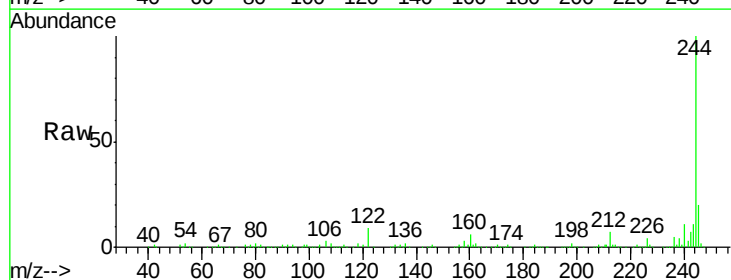

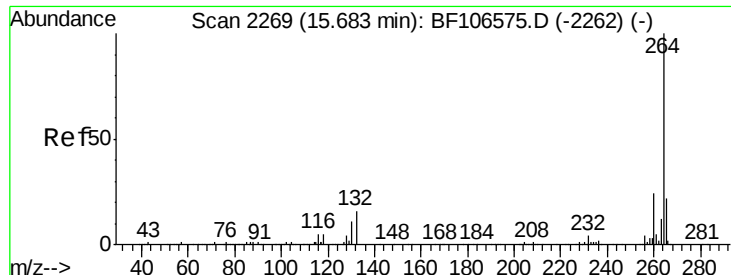

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.68 min Scan# 2268
Delta R.T. -0.01 min
Lab File: BF106729.D
Acq: 23 Jun 2018 00:34

Instrument :
BNA_F
ClientSampleId :
SB-49-COMP

Tgt Ion: 264 Resp: 115372

Ion	Ratio	Lower	Upper
264	100		
260	22.7	19.2	28.8
265	21.4	17.5	26.3

