


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062218\
 Data File : BF106695.D
 Acq On : 22 Jun 2018 9:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 22 11:34:03 2018

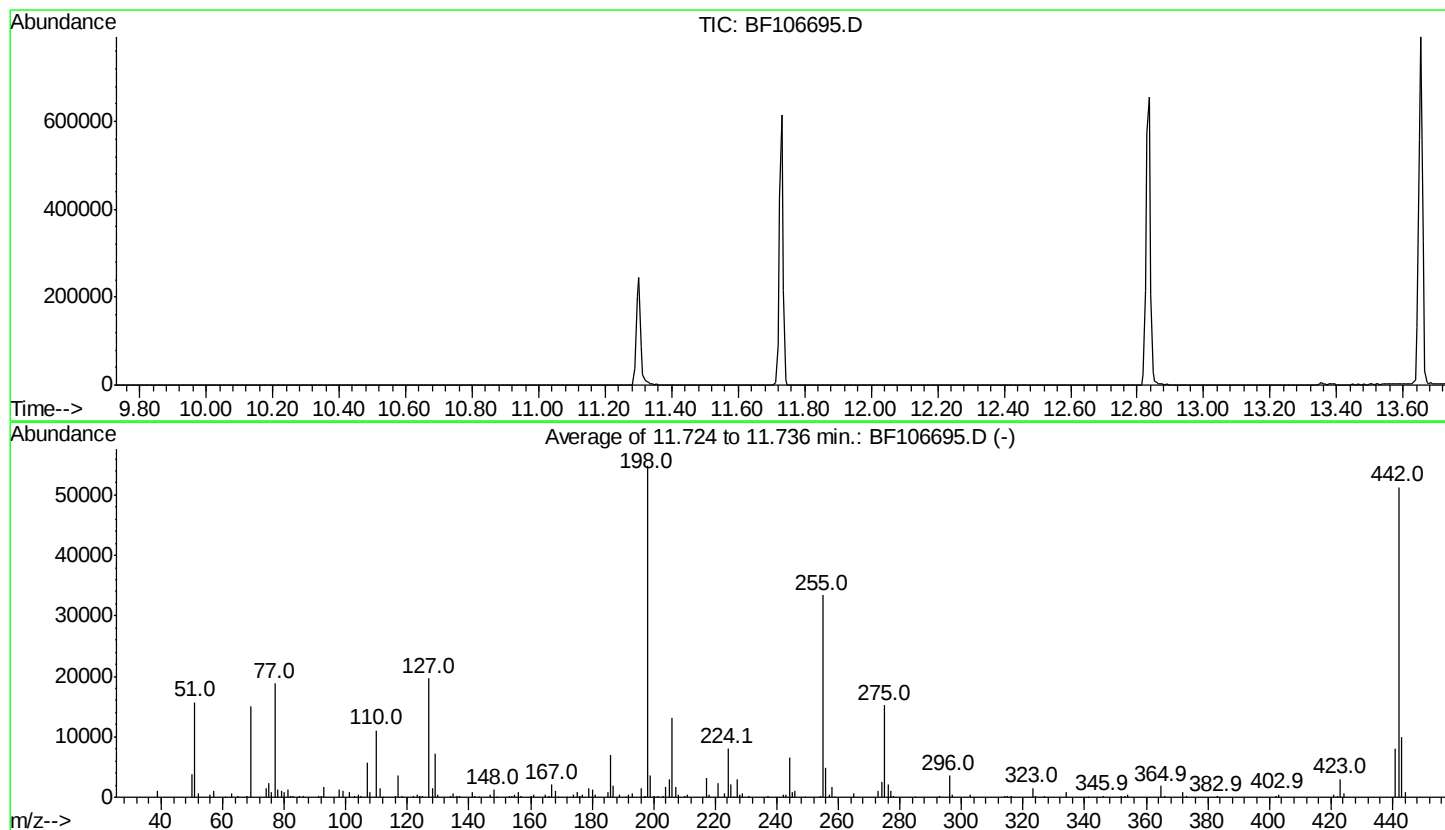

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	15763	PASS
68	69	0.00	2	0.8	121	PASS
69	198	0.00	100	27.3	14960	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.8	19621	PASS
197	198	0.00	2	0.3	163	PASS
198	198	100	100	100.0	54842	PASS
199	198	5	9	6.5	3555	PASS
275	198	10	60	27.6	15148	PASS
365	198	1	100	3.3	1829	PASS
441	443	0.01	100	79.6	7983	PASS
442	198	50	100	93.5	51293	PASS
443	442	15	24	19.5	10026	PASS