


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062218\
 Data File : BF106709.D
 Acq On : 22 Jun 2018 15:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 22 11:34:03 2018

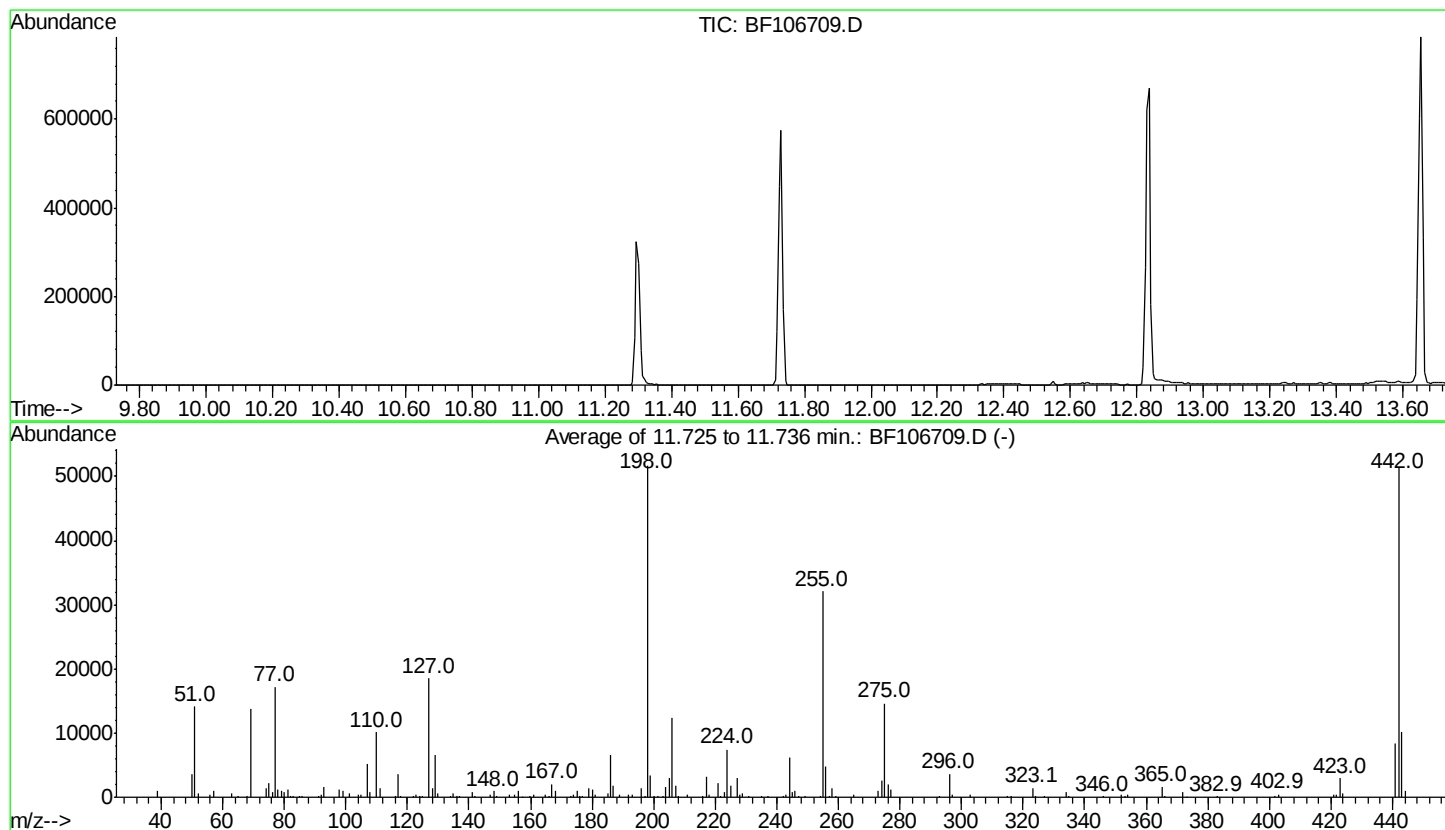

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	14152	PASS
68	69	0.00	2	1.7	235	PASS
69	198	0.00	100	26.7	13815	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.8	18509	PASS
197	198	0.00	2	0.6	298	PASS
198	198	100	100	100.0	51680	PASS
199	198	5	9	6.6	3428	PASS
275	198	10	60	28.2	14584	PASS
365	198	1	100	3.3	1680	PASS
441	443	0.01	100	83.0	8410	PASS
442	198	50	100	99.7	51533	PASS
443	442	15	24	19.7	10130	PASS