


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062218\
 Data File : BF106736.D
 Acq On : 23 Jun 2018 4:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 22 11:34:03 2018

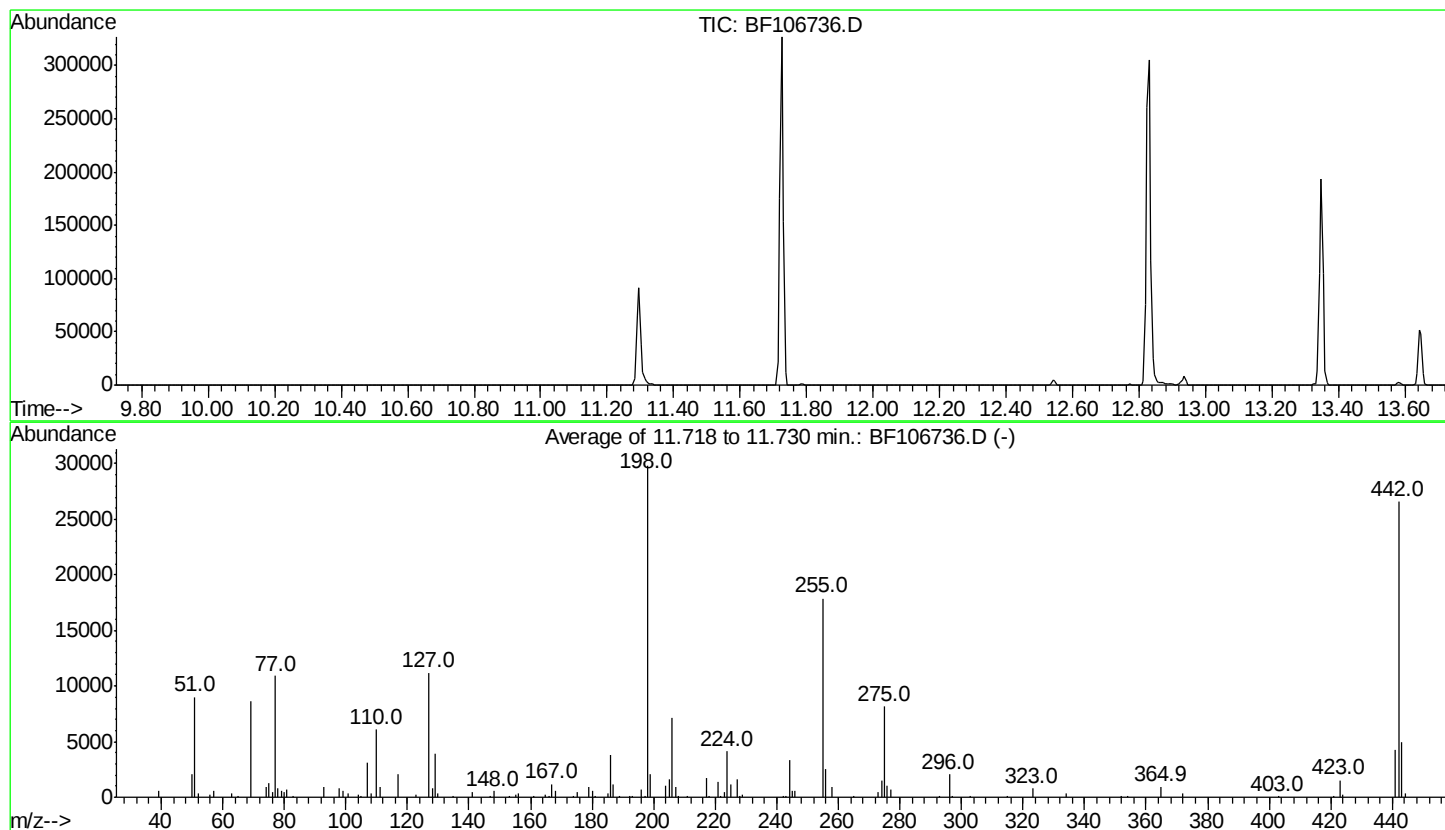

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	9025	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.8	8596	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.5	11177	PASS
197	198	0.00	2	0.4	106	PASS
198	198	100	100	100.0	29826	PASS
199	198	5	9	7.0	2083	PASS
275	198	10	60	27.3	8147	PASS
365	198	1	100	3.2	954	PASS
441	443	0.01	100	85.6	4273	PASS
442	198	50	100	89.1	26585	PASS
443	442	15	24	18.8	4990	PASS