
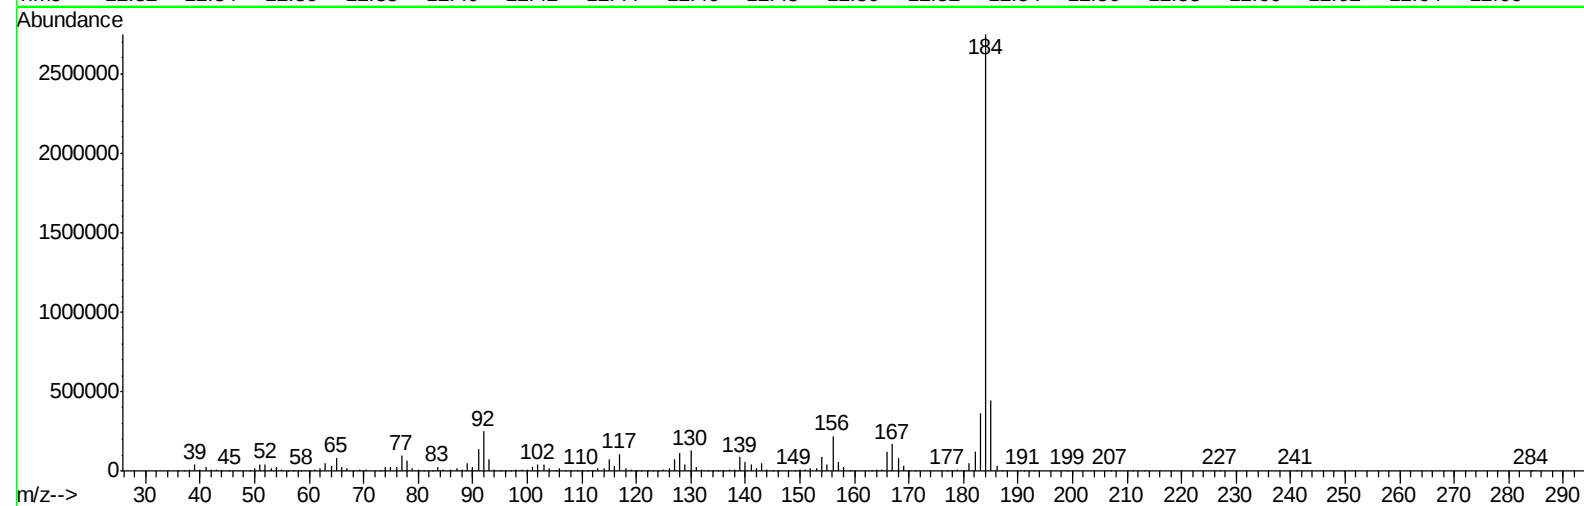


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062219\
Data File : BF115106.D
Acq On : 22 Jun 2019 8:23
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 07:12:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

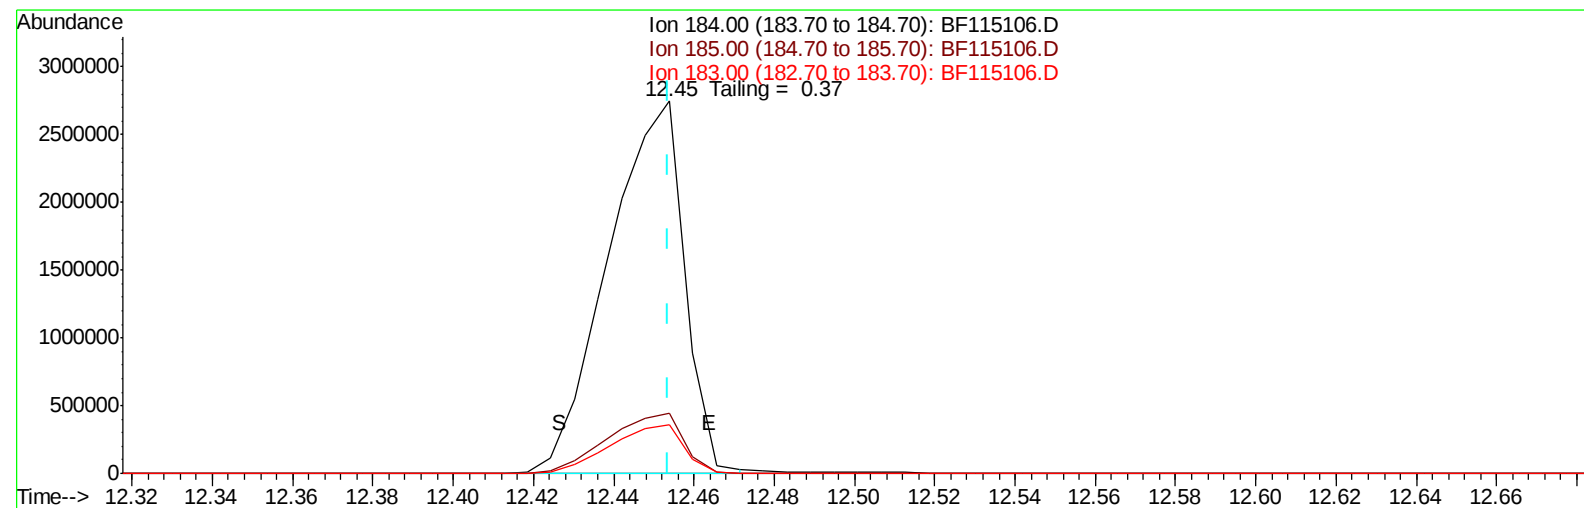

TIC: BF115106.D

(77) Benzidine



12.454min (-0.000) 84814.74ng

response 3645598

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	16.06
183.00	12.00	13.13
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062219\
Data File : BF115106.D
Acq On : 22 Jun 2019 8:23
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 07:12:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

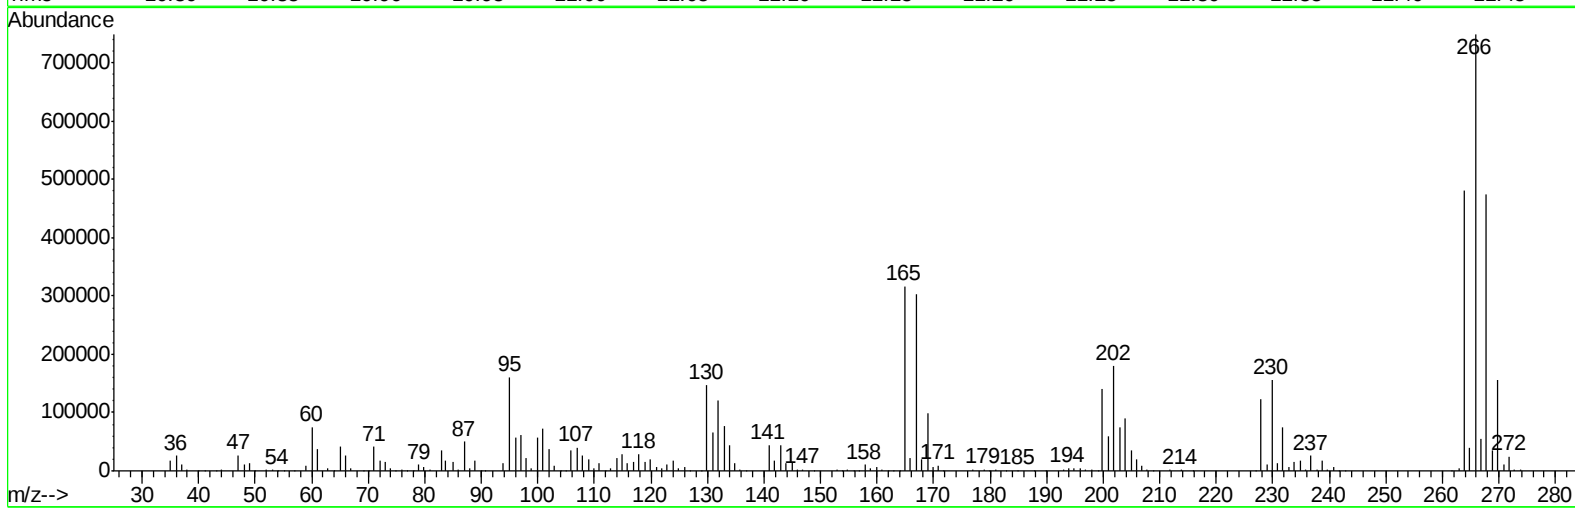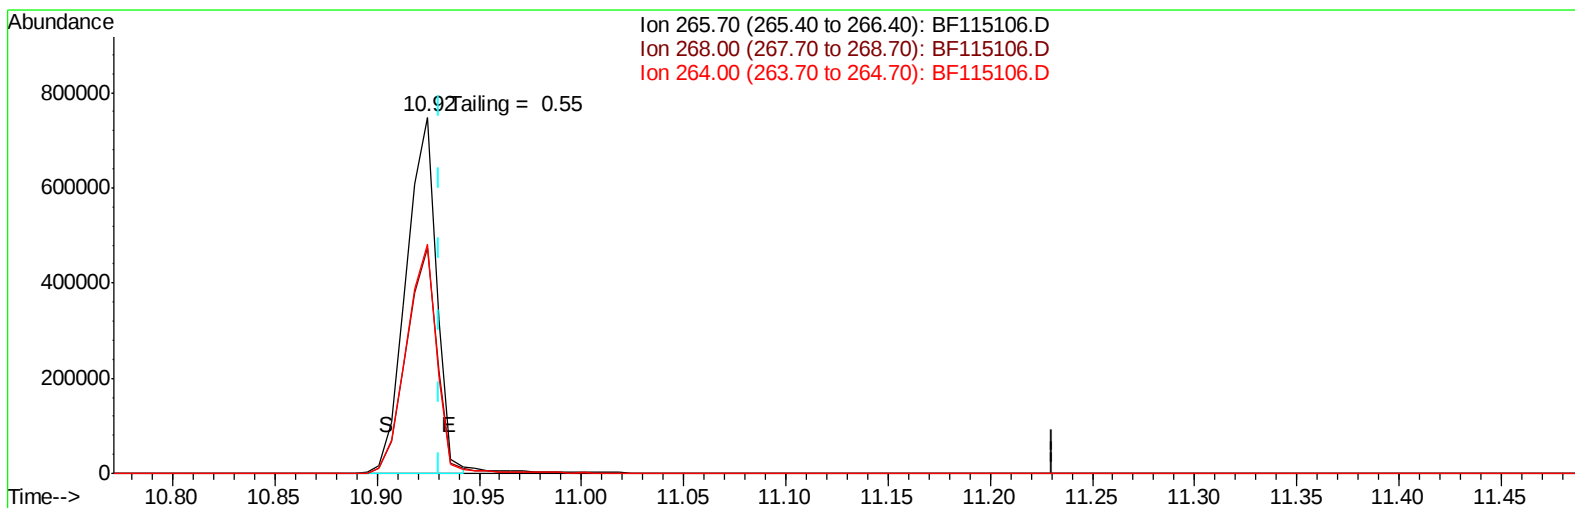

TIC: BF115106.D

(70) Pentachlorophenol (C)

10.924min (-0.006) 109498.82ng

response 798780

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	63.38
264.00	61.60	64.30
0.00	0.00	0.00