
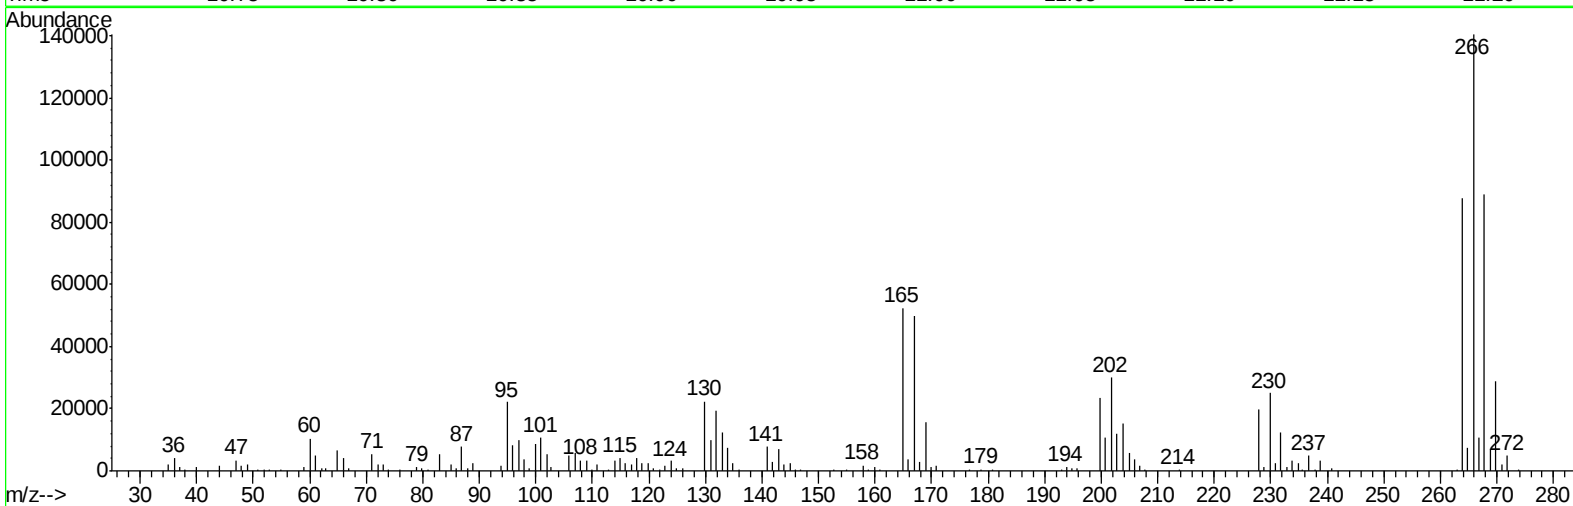


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062219\
Data File : BF115136.D
Acq On : 22 Jun 2019 23:29
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 07:51:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

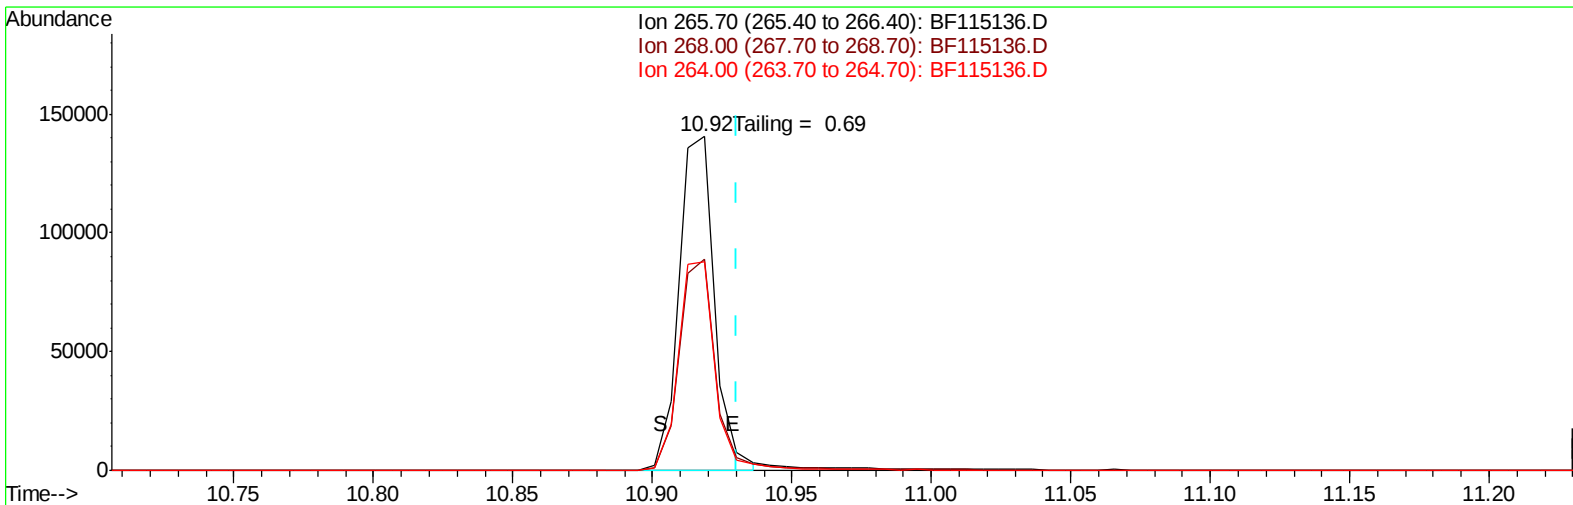

TIC: BF115136.D

(70) Pentachlorophenol (C)



10.919min (-0.012) 156908.60ng

response 129403

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	63.31
264.00	61.60	62.48
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062219\
Data File : BF115136.D
Acq On : 22 Jun 2019 23:29
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 07:51:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

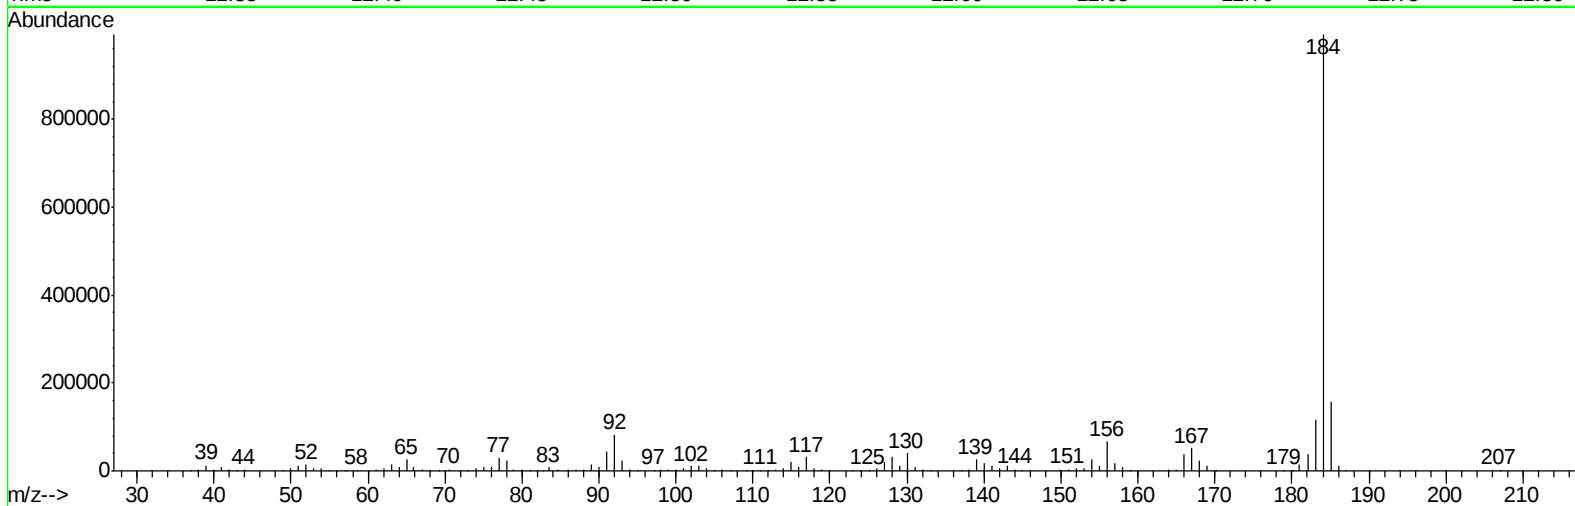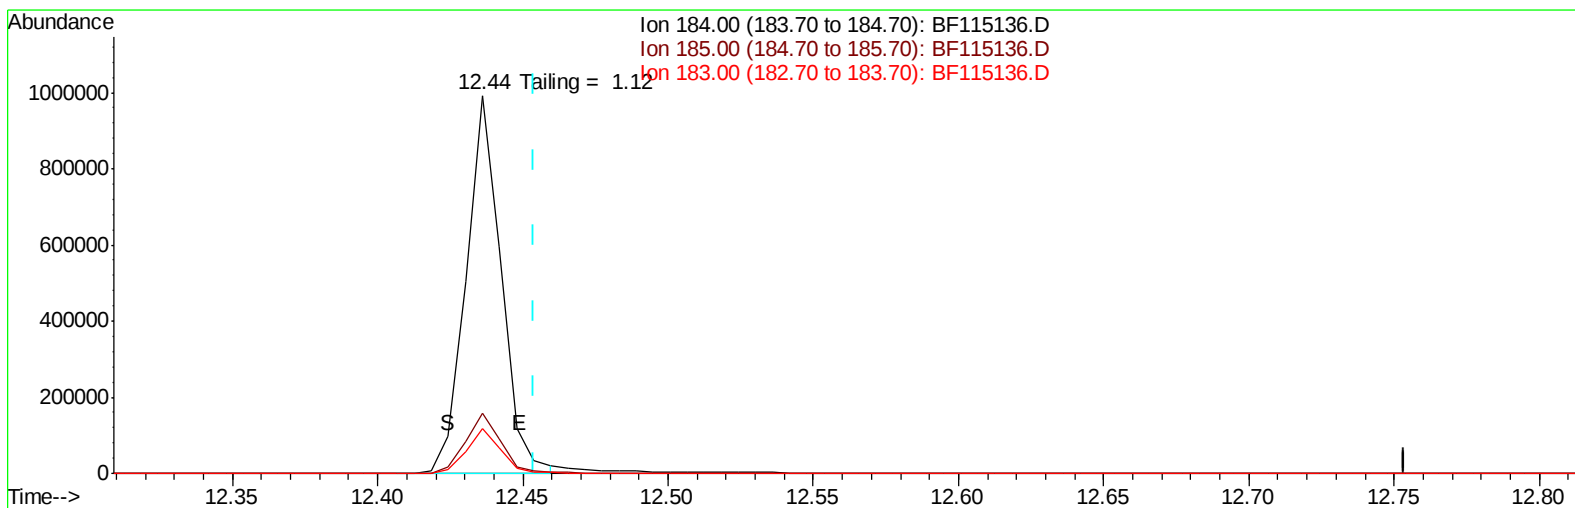

TIC: BF115136.D

(77) Benzidine

12.436min (-0.018) 17467.10ng

response 863253

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.91
183.00	12.00	11.73
0.00	0.00	0.00