


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062219\
 Data File : BF115106.D
 Acq On : 22 Jun 2019 8:23
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 24 04:21:29 2019

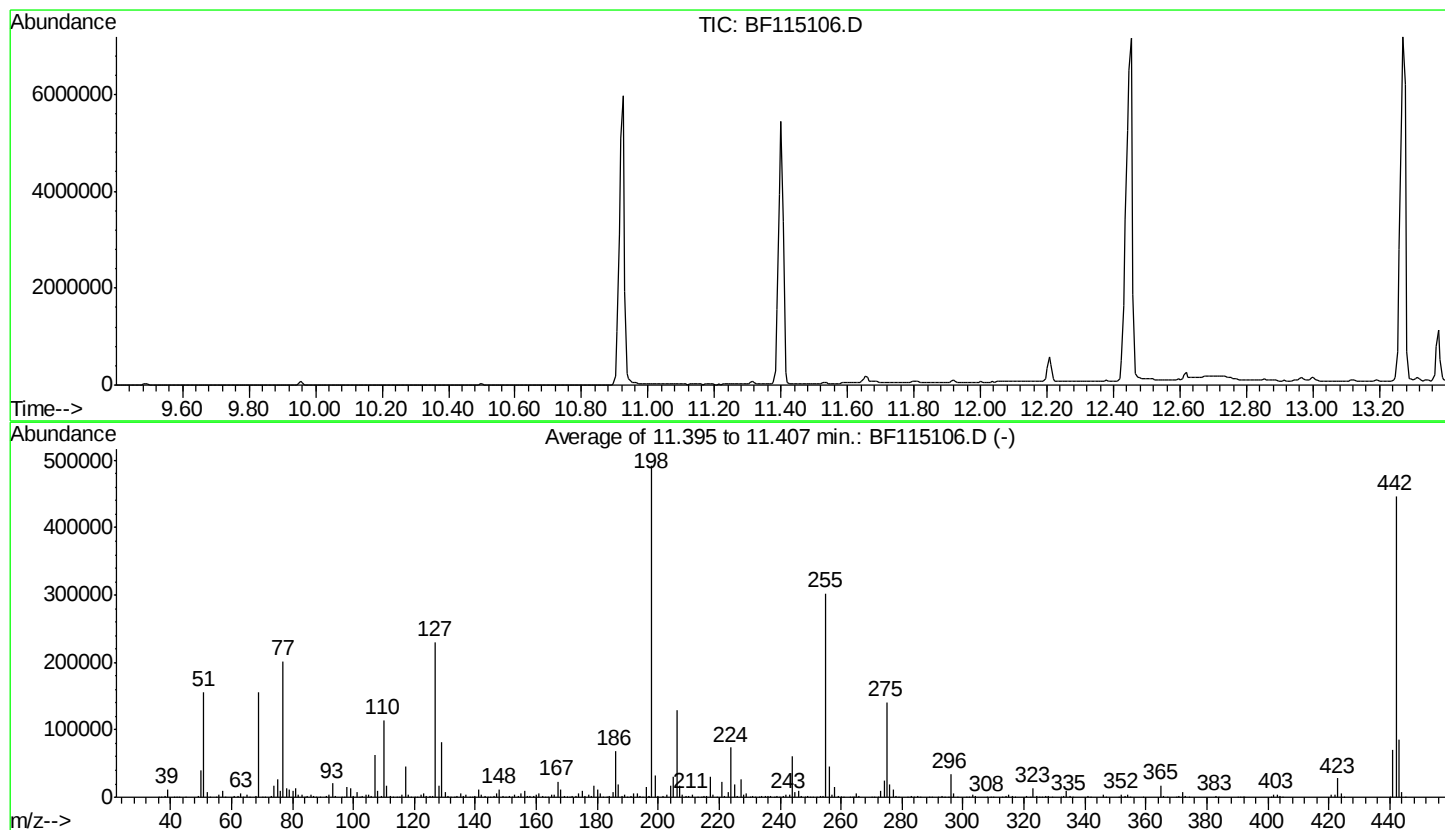

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	156680	PASS
68	69	0.00	2	1.8	2793	PASS
69	198	0.00	100	31.8	156379	PASS
70	69	0.00	2	0.6	933	PASS
127	198	10	80	46.9	230570	PASS
197	198	0.00	2	0.5	2436	PASS
198	198	100	100	100.0	492053	PASS
199	198	5	9	6.5	31935	PASS
275	198	10	60	28.7	141178	PASS
365	198	1	100	3.5	17407	PASS
441	198	0.01	100	14.3	70173	PASS
442	198	50	100	90.8	446549	PASS
443	442	15	24	19.2	85848	PASS