
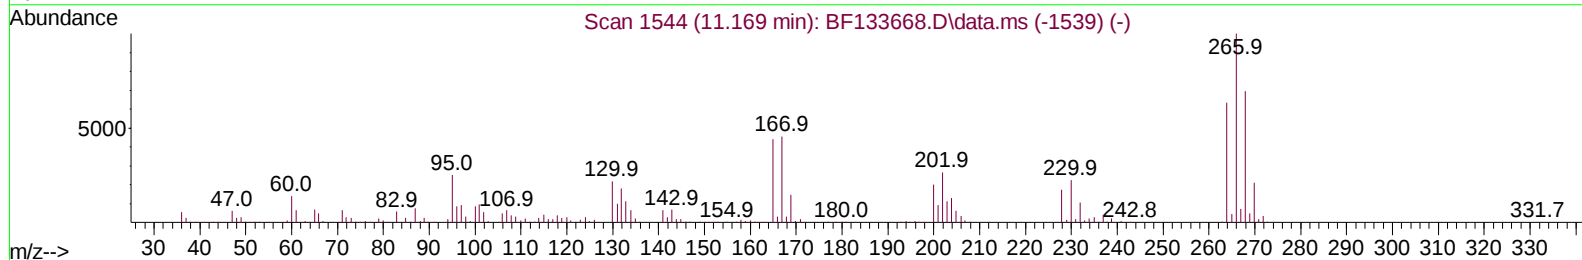
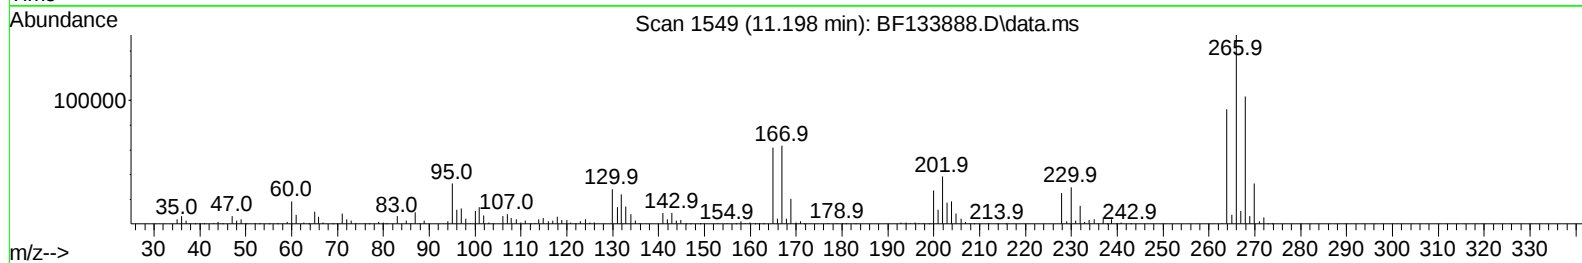


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062223\
Data File : BF133888.D
Acq On : 22 Jun 2023 07:58
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 23 04:15:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 02:21:26 2023
Response via : Initial Calibration

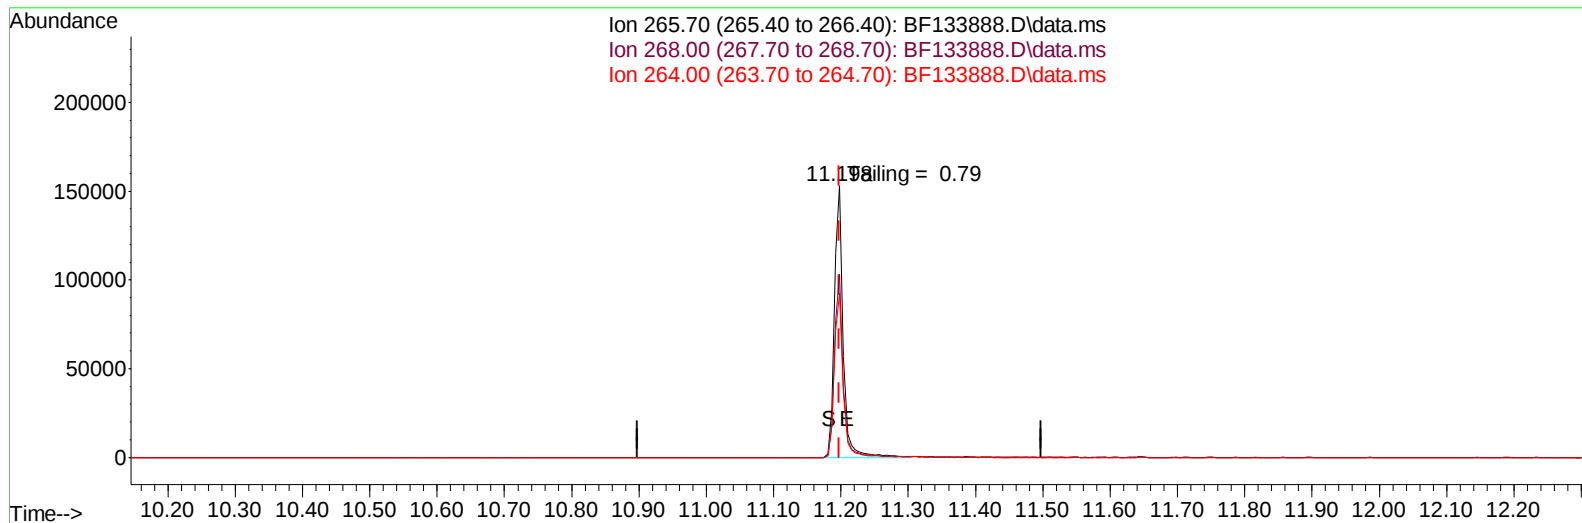

TIC: BF133888.D\data.ms




(70) Pentachlorophenol (C)

11.198min (+ 0.000) 34271.36 ng

response 139943

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	67.67
264.00	63.40	60.58
0.00	0.00	0.00

Quant Time: Jun 23 04:15:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 02:21:26 2023
Response via : Initial Calibration

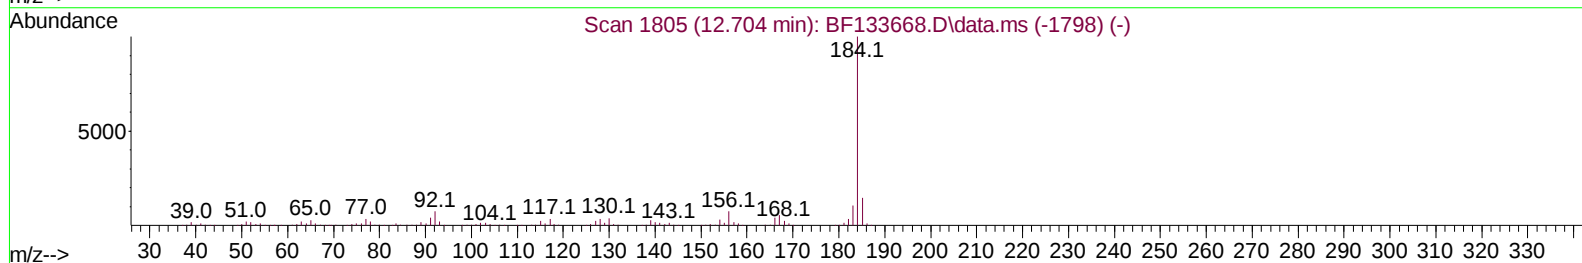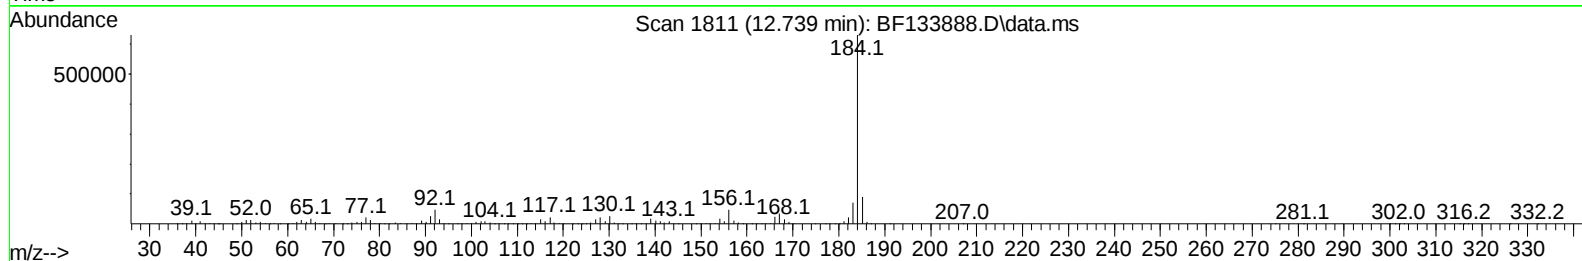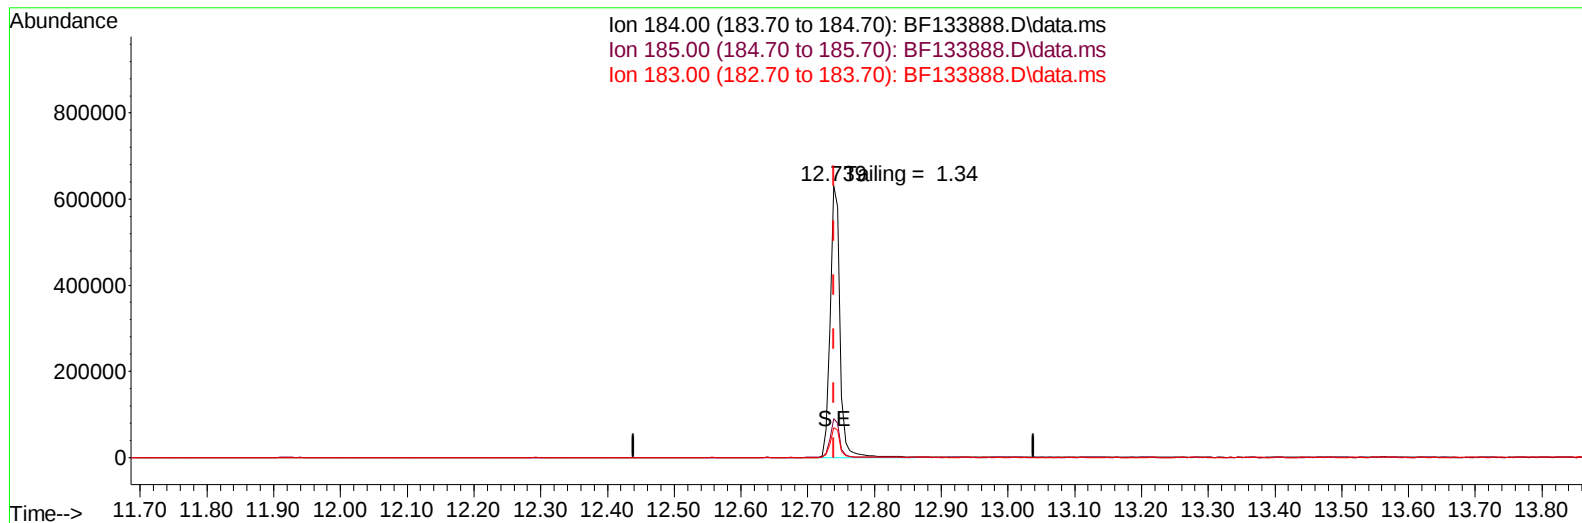

TIC: BF133888.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 66135.69 ng

response **645801**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.36
183.00	10.50	11.07
0.00	0.00	0.00