

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062223\
 Data File : BF133892.D
 Acq On : 22 Jun 2023 10:02
 Operator : CG\JU
 Sample : PB153433TB
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153433TB

Quant Time: Jun 23 02:25:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 23 02:21:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.857	152	111059	20.000	ng	0.00
21) Naphthalene-d8	8.139	136	426380	20.000	ng	0.00
39) Acenaphthene-d10	9.898	164	222173	20.000	ng	0.00
64) Phenanthrene-d10	11.392	188	446531	20.000	ng	0.00
76) Chrysene-d12	14.051	240	267083	20.000	ng	0.00
86) Perylene-d12	15.556	264	250842	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	872796	136.815	ng	0.01
7) Phenol-d6	6.498	99	1074973	129.455	ng	0.00
23) Nitrobenzene-d5	7.422	82	732574	93.581	ng	0.00
42) 2,4,6-Tribromophenol	10.692	330	355173	126.292	ng	0.00
45) 2-Fluorobiphenyl	9.222	172	1329061	85.036	ng	0.00
79) Terphenyl-d14	12.992	244	1565373	90.690	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062223\
Data File : BF133892.D
Acq On : 22 Jun 2023 10:02
Operator : CG\JU
Sample : PB153433TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153433TB


Quant Time: Jun 23 02:25:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 02:21:26 2023
Response via : Initial Calibration

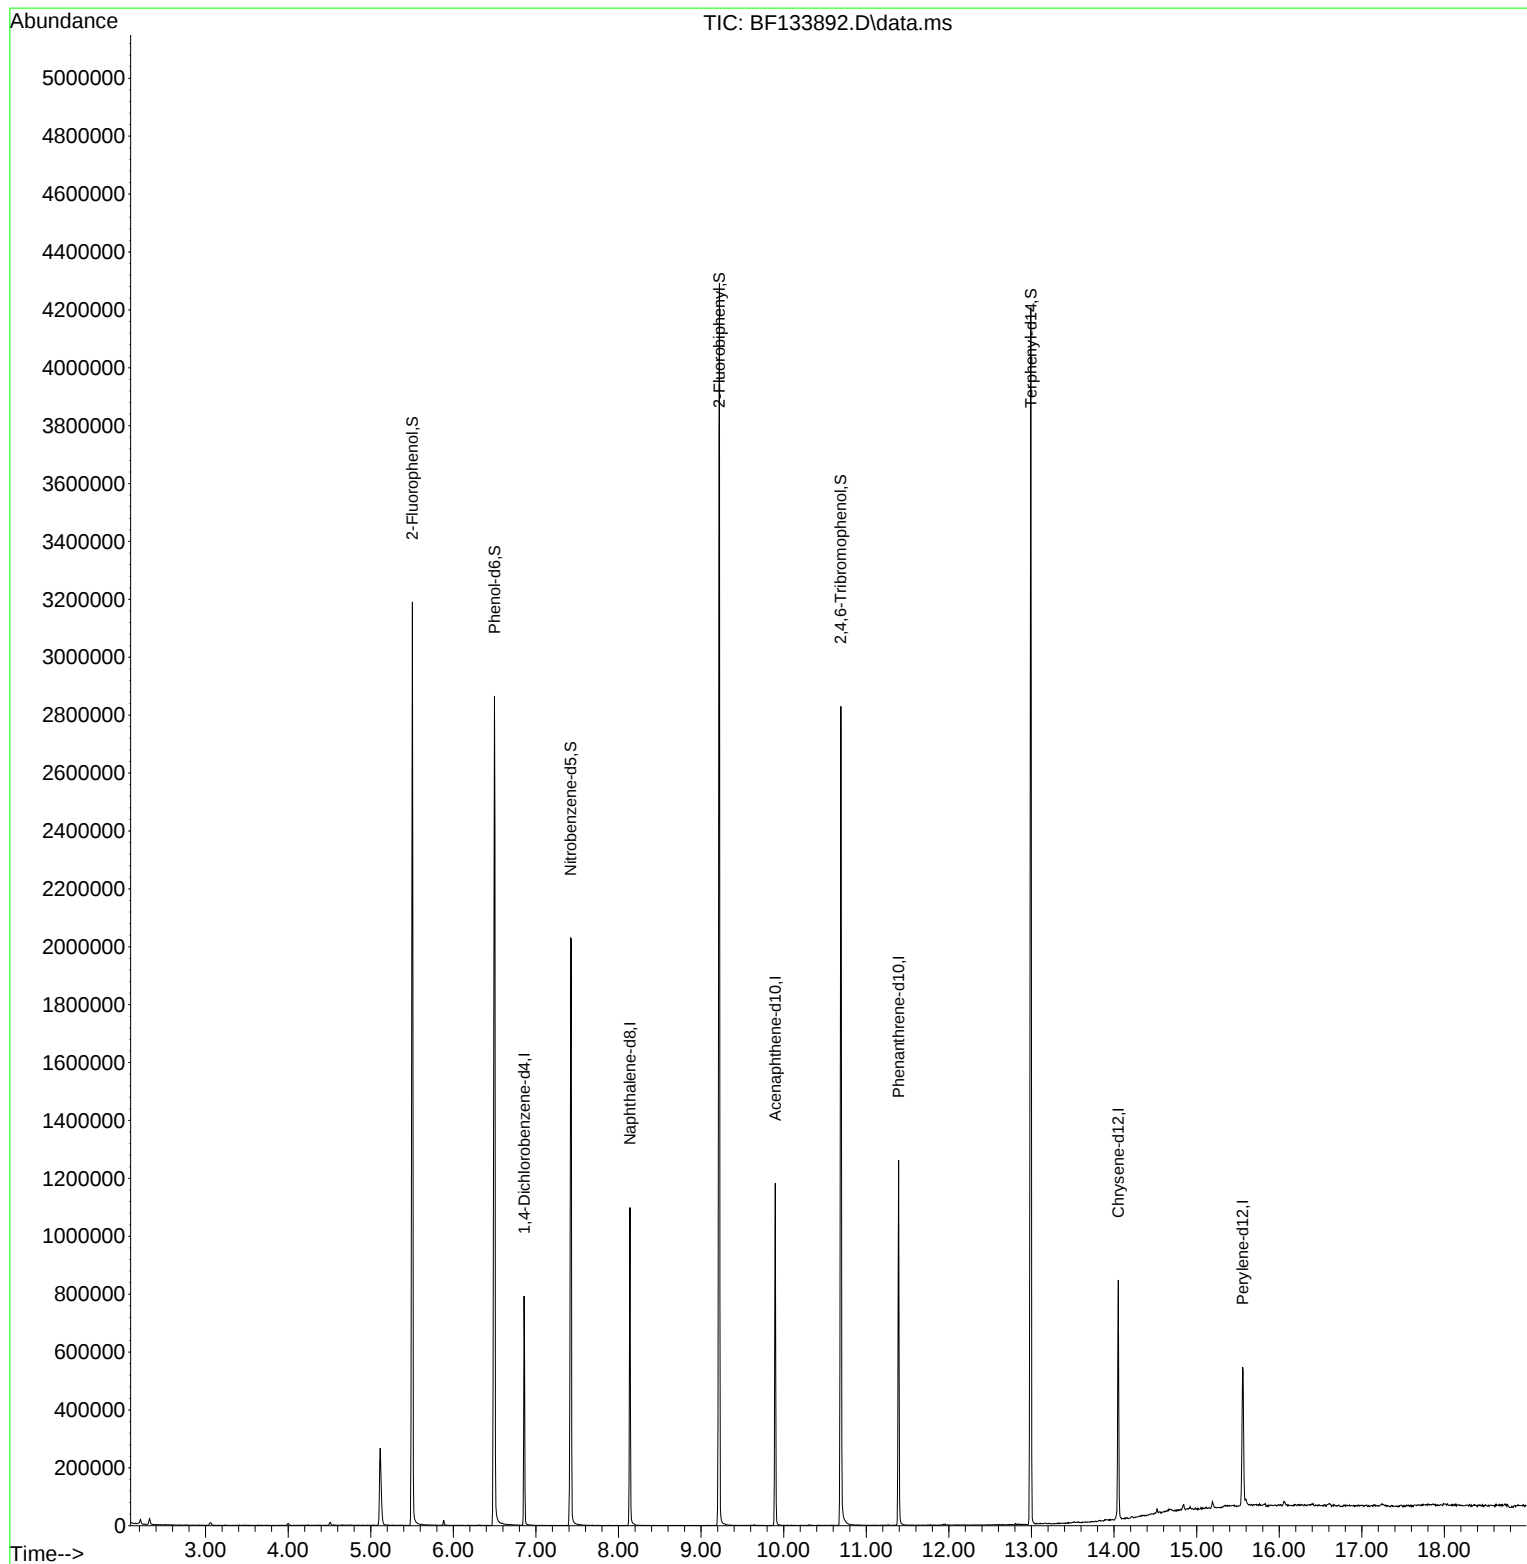



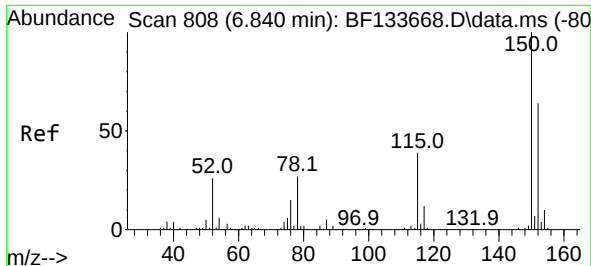


#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.857 min Scan# 811
Delta R.T. -0.006 min
Lab File: BF133892.D
Acq: 22 Jun 2023 10:02

Instrument :
BNA_F
ClientSampleId :
PB153433TB



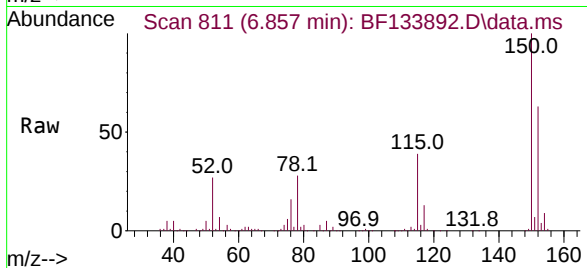


Tgt Ion:152 Resp: 111059
Ion Ratio Lower Upper
152 100
150 157.8 124.3 186.5
115 61.9 48.5 72.7

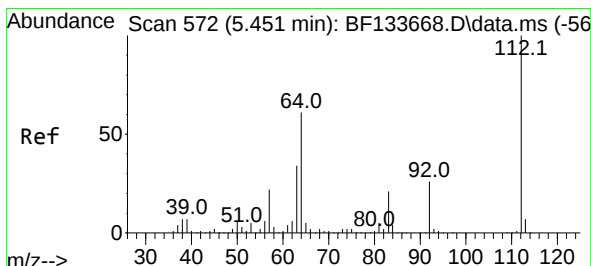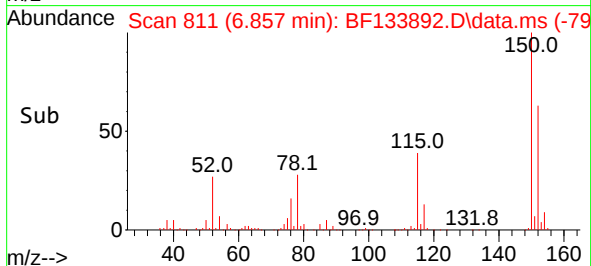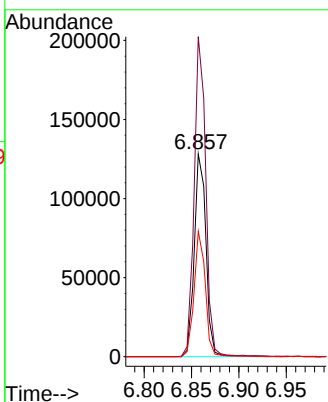

#5
2-Fluorophenol
Concen: 136.815 ng
RT: 5.504 min Scan# 581
Delta R.T. 0.012 min
Lab File: BF133892.D
Acq: 22 Jun 2023 10:02

Tgt Ion:112 Resp: 872796
Ion Ratio Lower Upper
112 100
64 66.0 49.0 73.4
63 37.2 26.8 40.2


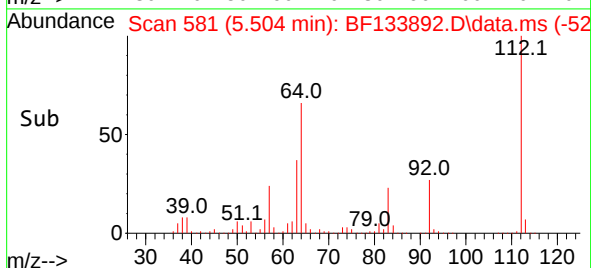
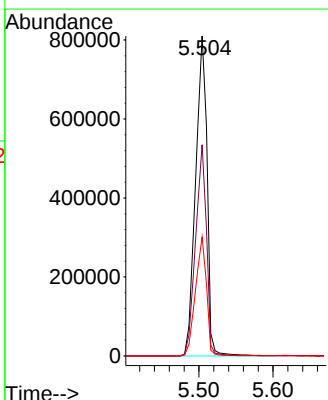
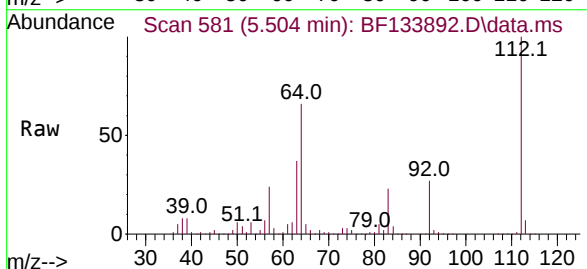




#7
Phenol-d6
Concen: 129.455 ng
RT: 6.498 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF133892.D
Acq: 22 Jun 2023 10:02




Instrument :
BNA_F
ClientSampleId :
PB153433TB


Tgt Ion: 99 Resp: 1074973
Ion Ratio Lower Upper
99 100
42 26.0 19.9 29.9
71 41.3 32.2 48.4

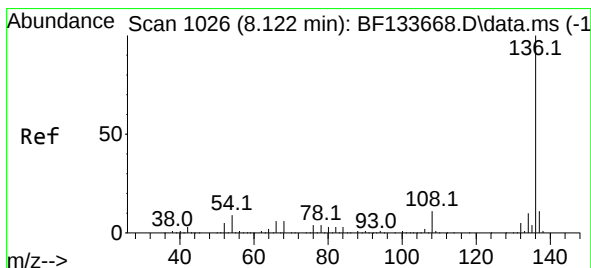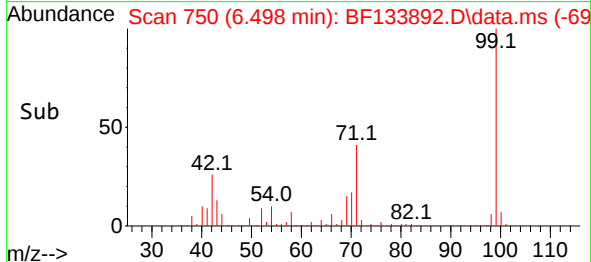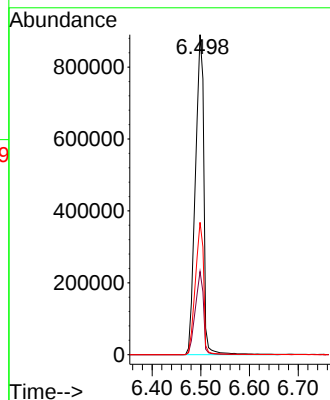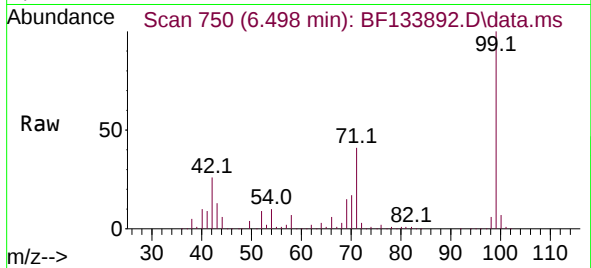

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.139 min Scan# 1029
Delta R.T. 0.000 min
Lab File: BF133892.D
Acq: 22 Jun 2023 10:02

Tgt Ion: 136 Resp: 426380
Ion Ratio Lower Upper
136 100
137 10.6 8.8 13.2
54 8.6 7.4 11.0
68 5.0 4.4 6.6

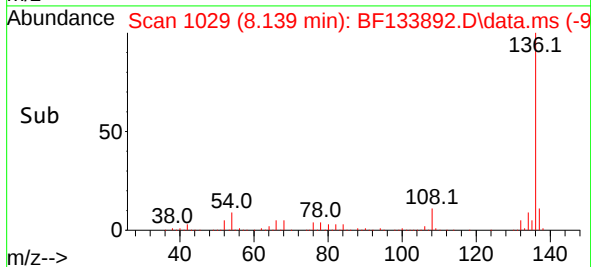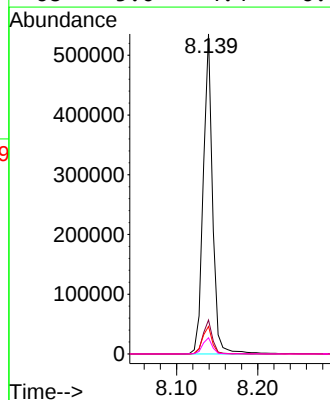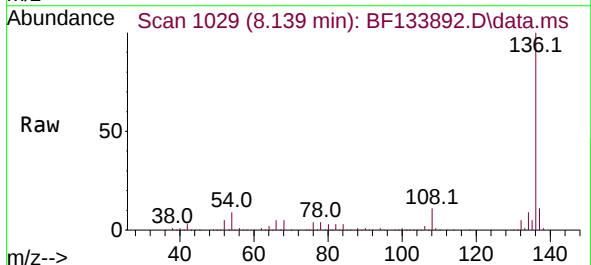

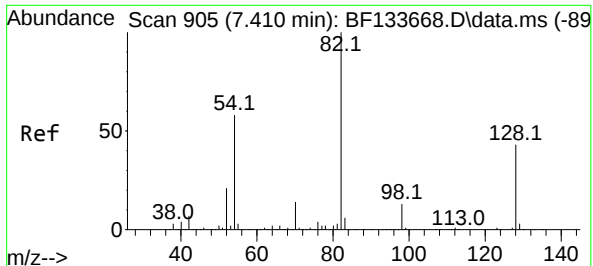

#23

Nitrobenzene-d5

Concen: 93.581 ng

RT: 7.422 min Scan# 905

Delta R.T. -0.006 min

Lab File: BF133892.D

Acq: 22 Jun 2023 10:02

Instrument :





BNA_F

ClientSampleId :

PB153433TB

Tgt Ion: 82 Resp: 732574

Ion	Ratio	Lower	Upper
82	100		
128	40.0	34.2	51.2
54	60.9	46.5	69.7

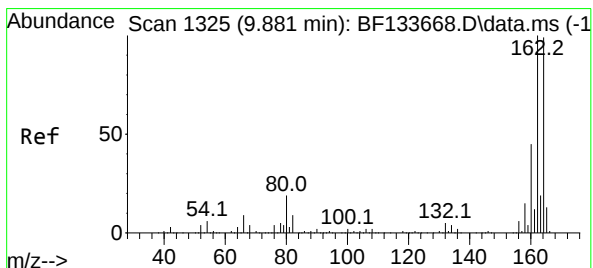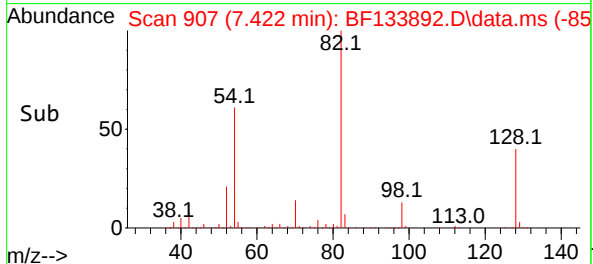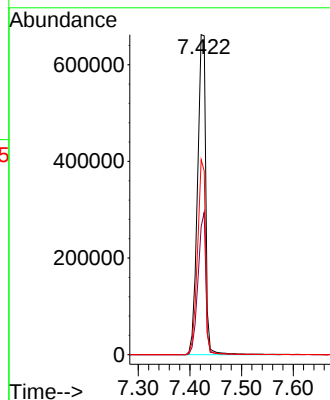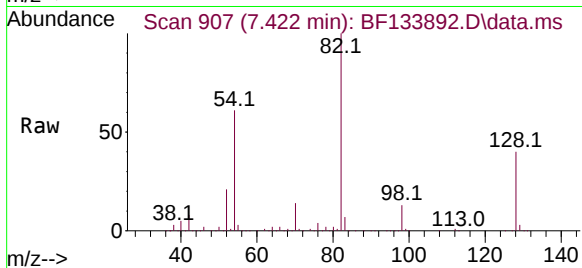

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.898 min Scan# 1328




Delta R.T. 0.000 min


Lab File: BF133892.D

Acq: 22 Jun 2023 10:02

Tgt Ion:164 Resp: 222173

Ion	Ratio	Lower	Upper
164	100		
162	99.0	80.8	121.2
160	45.6	36.7	55.1

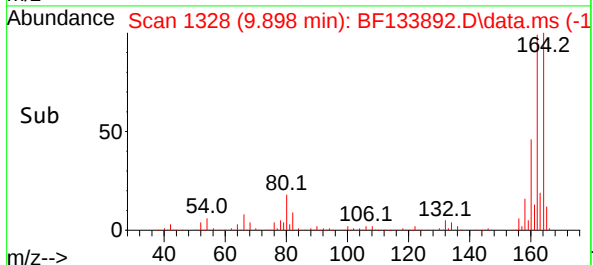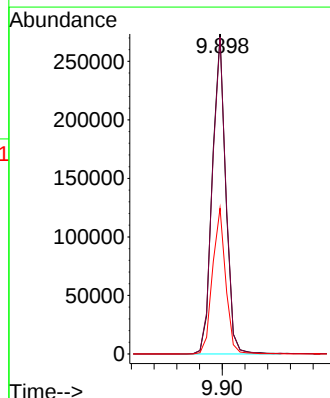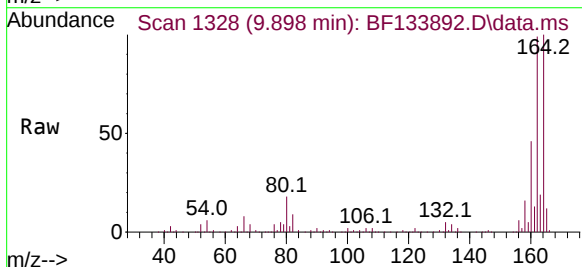

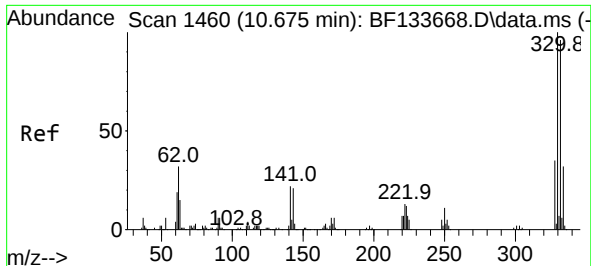

#42

2,4,6-Tribromophenol

Concen: 126.292 ng

RT: 10.692 min Scan# 1463

Delta R.T. -0.006 min

Lab File: BF133892.D


Acq: 22 Jun 2023 10:02

Instrument :

BNA_F

ClientSampleId :

PB153433TB

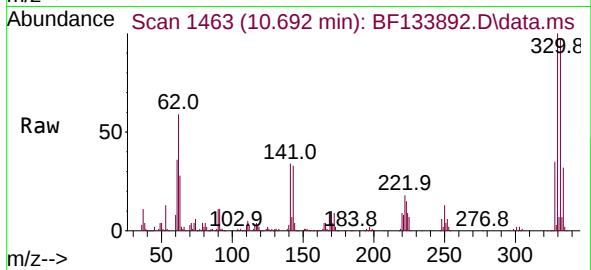




Tgt Ion:330 Resp: 355173

Ion Ratio Lower Upper

330 100

332 97.6 77.2 115.8

141 32.3 24.9 37.3

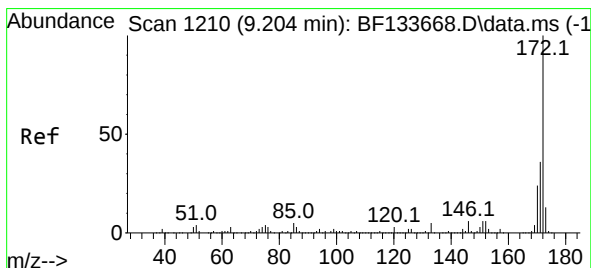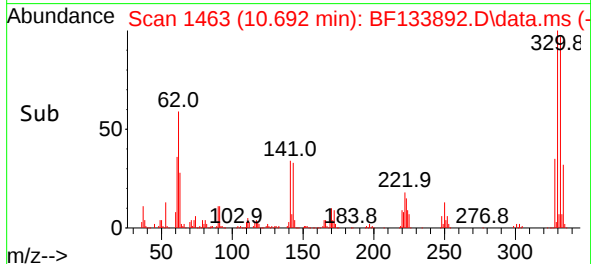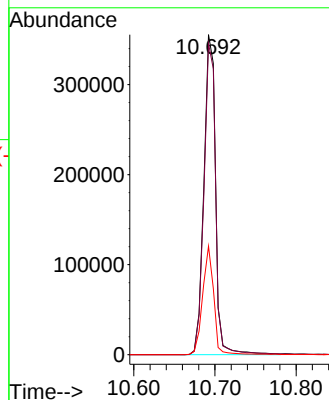

#45

2-Fluorobiphenyl

Concen: 85.036 ng

RT: 9.222 min Scan# 1213

Delta R.T. 0.000 min

Lab File: BF133892.D

Acq: 22 Jun 2023 10:02




Tgt Ion:172 Resp: 1329061

Ion Ratio Lower Upper

172 100

171 35.4 28.6 43.0

170 23.9 19.1 28.7


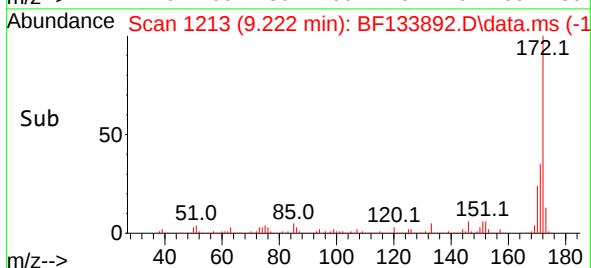
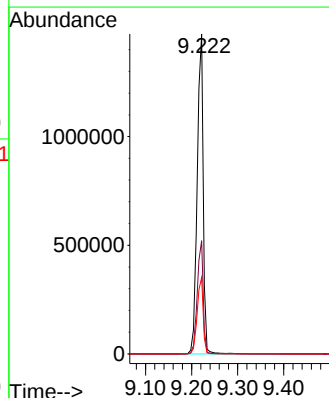
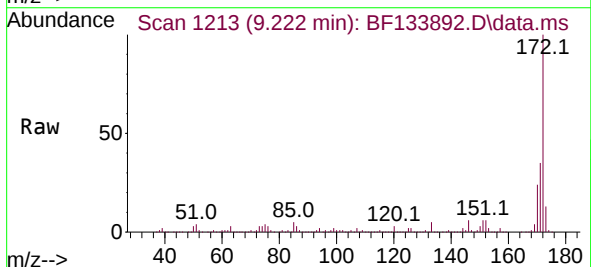




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.392 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF133892.D
Acq: 22 Jun 2023 10:02




Instrument :
BNA_F
ClientSampleId :
PB153433TB

Tgt Ion:188 Resp: 446531
Ion Ratio Lower Upper
188 100
94 8.9 6.8 10.2
80 9.0 7.8 11.6

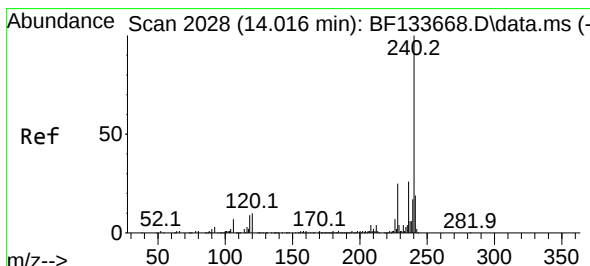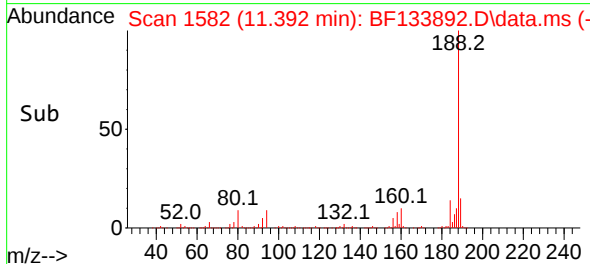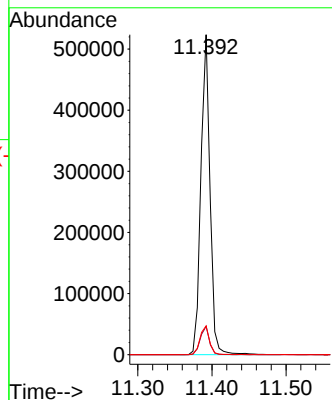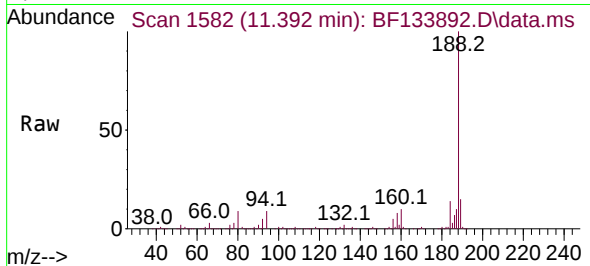

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.051 min Scan# 2034
Delta R.T. -0.006 min
Lab File: BF133892.D
Acq: 22 Jun 2023 10:02


Tgt Ion:240 Resp: 267083
Ion Ratio Lower Upper
240 100
120 9.8 8.1 12.1
236 26.6 20.5 30.7

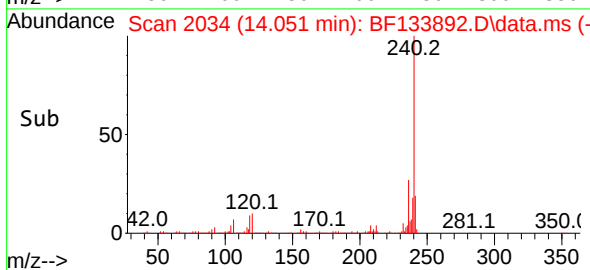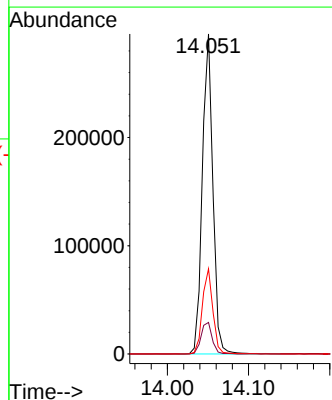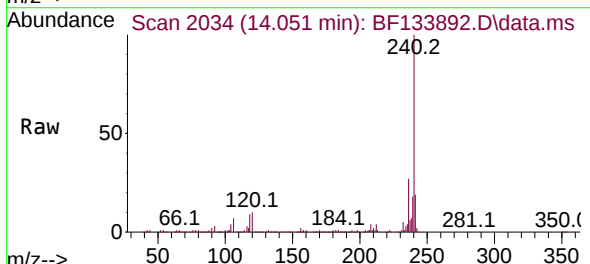






#79
 Terphenyl-d14
 Concen: 90.690 ng
 RT: 12.992 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BF133892.D
 Acq: 22 Jun 2023 10:02

Instrument :
 BNA_F
 ClientSampleId :
 PB153433TB

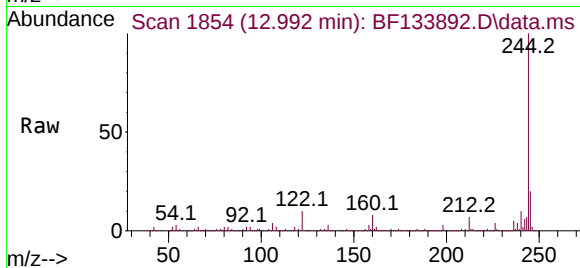

Tgt Ion:244 Resp: 1565373
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.4 8.2
 122 9.8 8.1 12.1

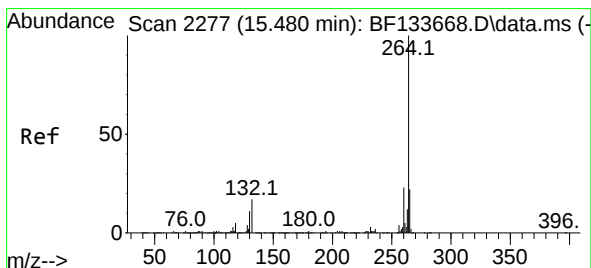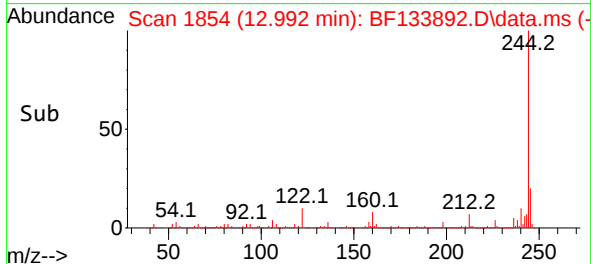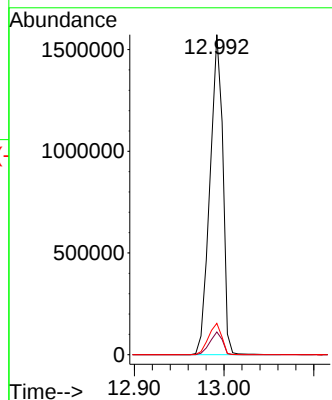

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.556 min Scan# 2290
 Delta R.T. -0.006 min
 Lab File: BF133892.D
 Acq: 22 Jun 2023 10:02

Tgt Ion:264 Resp: 250842
 Ion Ratio Lower Upper
 264 100
 260 24.0 18.2 27.2
 265 21.7 17.8 26.6

