

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062223\
 Data File : BF133909.D
 Acq On : 22 Jun 2023 19:27
 Operator : CG\JU
 Sample : PB153649BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153649BL

Quant Time: Jun 23 05:04:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 23 02:21:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.857	152	115159	20.000	ng	0.00
21) Naphthalene-d8	8.140	136	452358	20.000	ng	0.00
39) Acenaphthene-d10	9.898	164	229608	20.000	ng	0.00
64) Phenanthrene-d10	11.392	188	475216	20.000	ng	0.00
76) Chrysene-d12	14.051	240	312147	20.000	ng	0.00
86) Perylene-d12	15.557	264	226691	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	815202	123.237	ng	0.01
7) Phenol-d6	6.498	99	983362	114.207	ng	0.00
23) Nitrobenzene-d5	7.422	82	661969	79.705	ng	0.00
42) 2,4,6-Tribromophenol	10.692	330	332384	114.362	ng	0.00
45) 2-Fluorobiphenyl	9.216	172	1163403	72.027	ng	0.00
79) Terphenyl-d14	12.992	244	1573987	78.024	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062223\
Data File : BF133909.D
Acq On : 22 Jun 2023 19:27
Operator : CG\JU
Sample : PB153649BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153649BL

Quant Time: Jun 23 05:04:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 02:21:26 2023
Response via : Initial Calibration




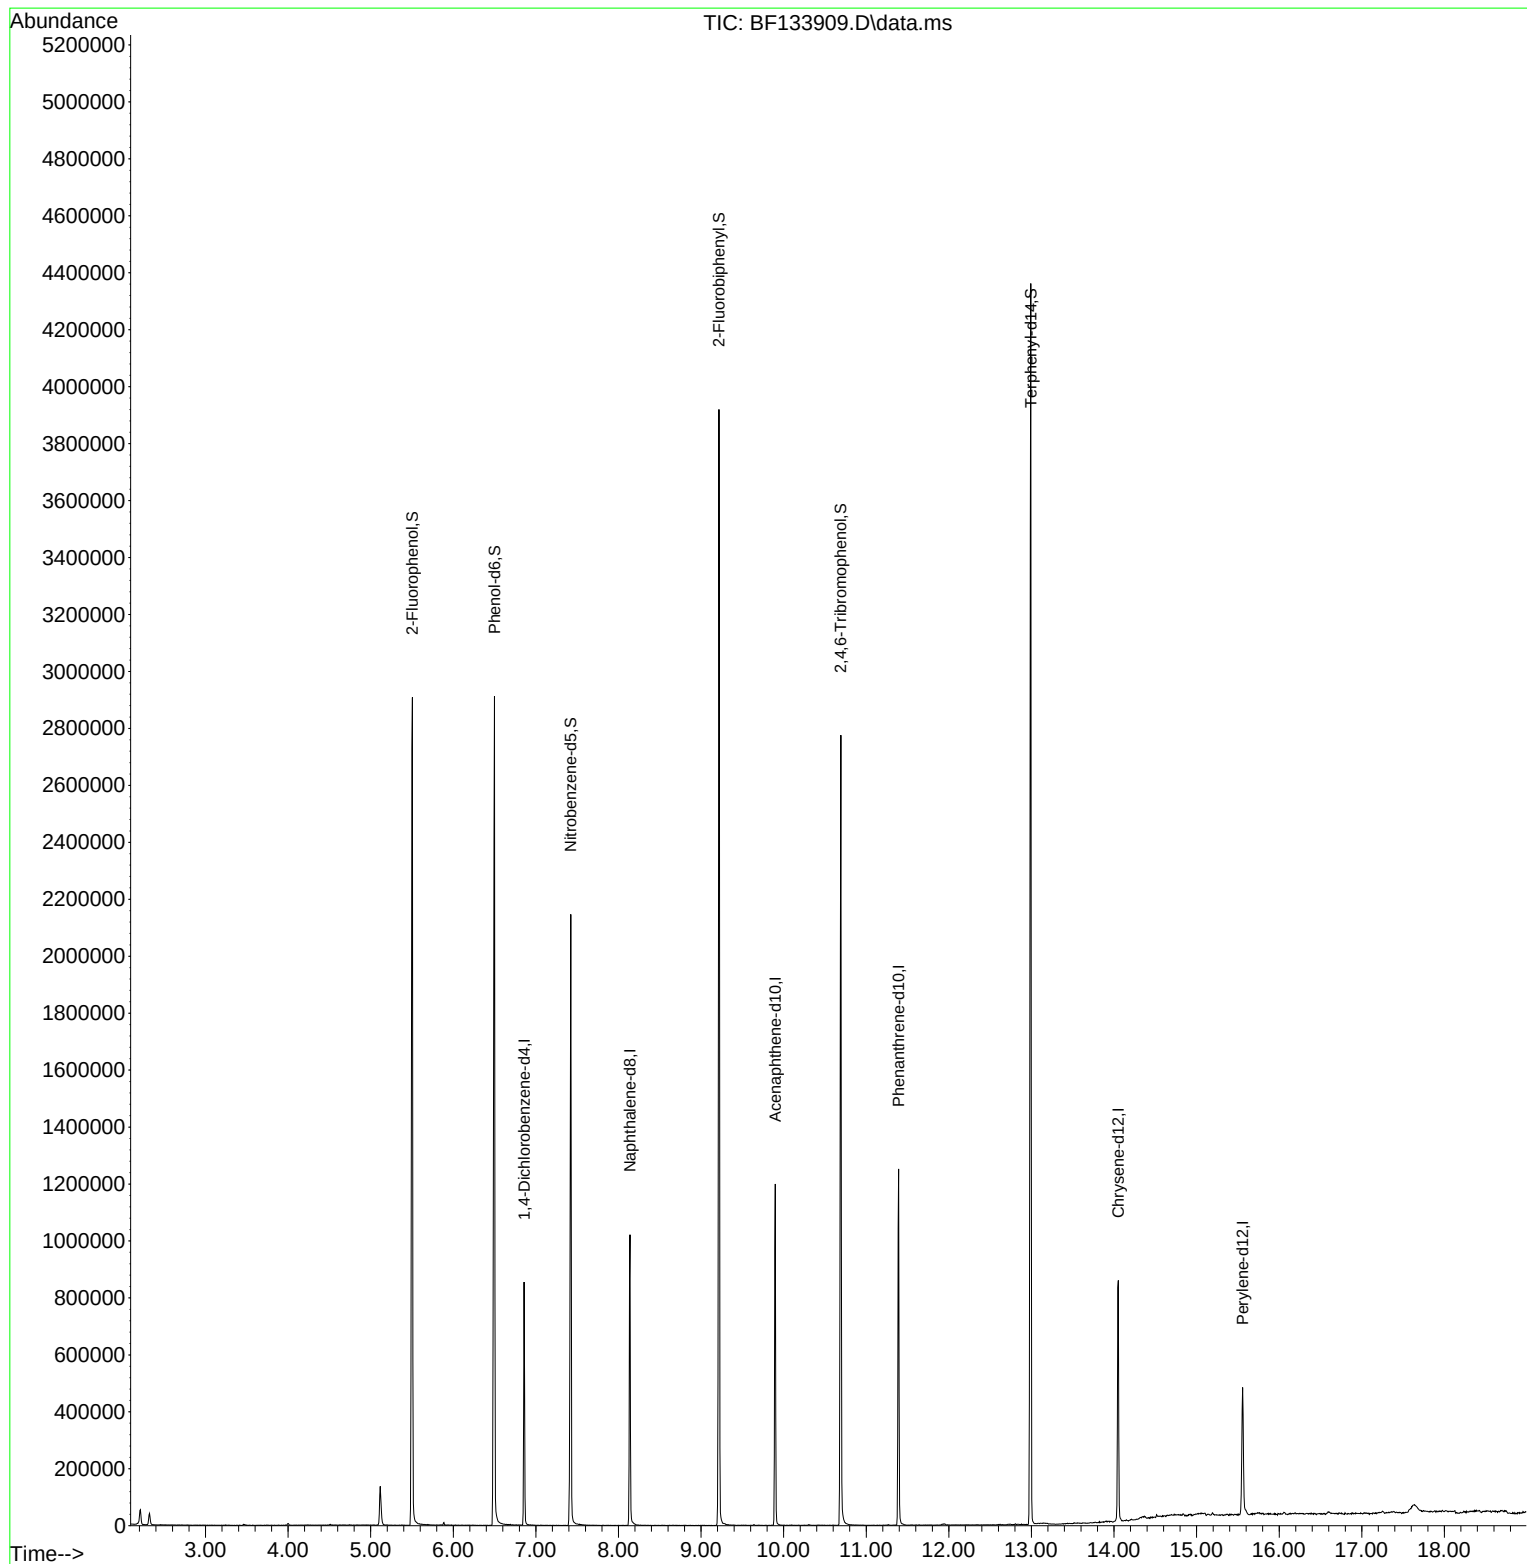


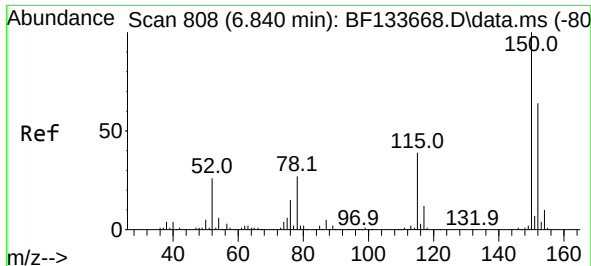

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.857 min Scan# 811
Delta R.T. -0.006 min
Lab File: BF133909.D
Acq: 22 Jun 2023 19:27




Instrument :
BNA_F
ClientSampleId :
PB153649BL


Tgt Ion:152 Resp: 115159
Ion Ratio Lower Upper
152 100
150 156.8 124.3 186.5
115 60.1 48.5 72.7

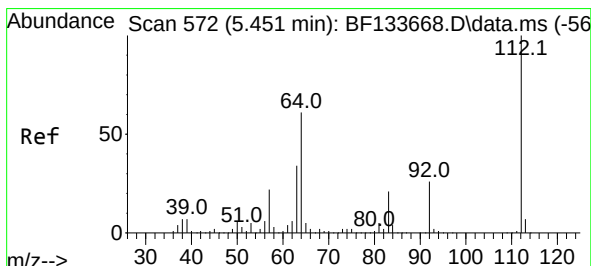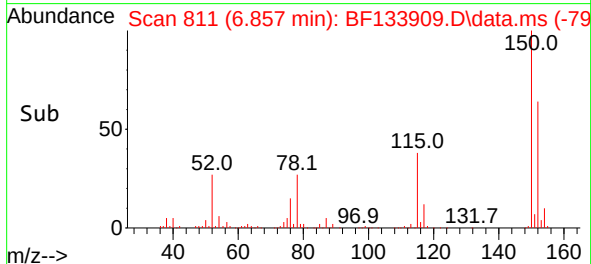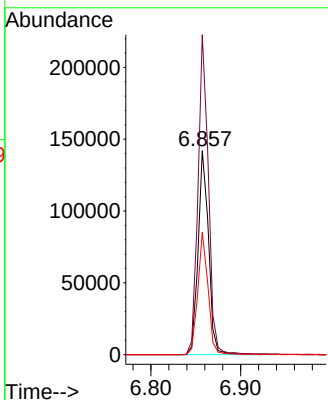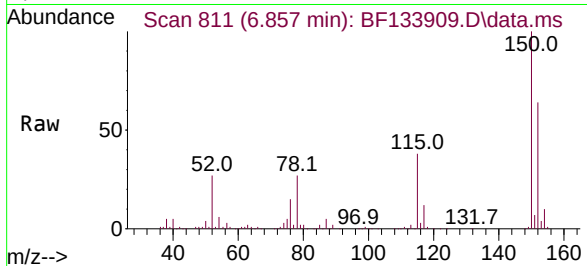

#5
2-Fluorophenol
Concen: 123.237 ng
RT: 5.504 min Scan# 581
Delta R.T. 0.012 min
Lab File: BF133909.D
Acq: 22 Jun 2023 19:27

Tgt Ion:112 Resp: 815202
Ion Ratio Lower Upper
112 100
64 61.4 49.0 73.4
63 34.0 26.8 40.2


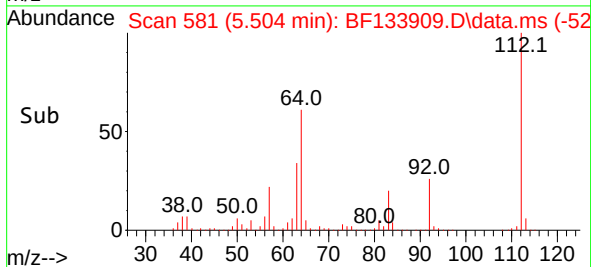
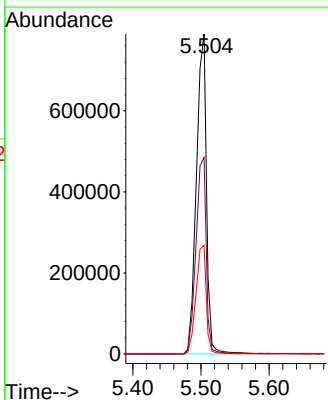
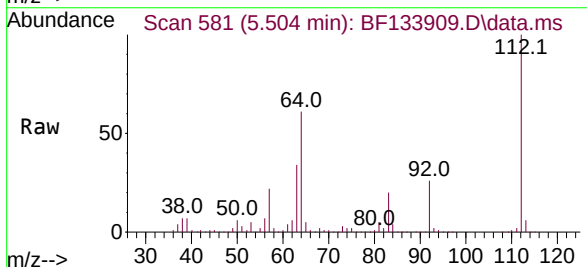


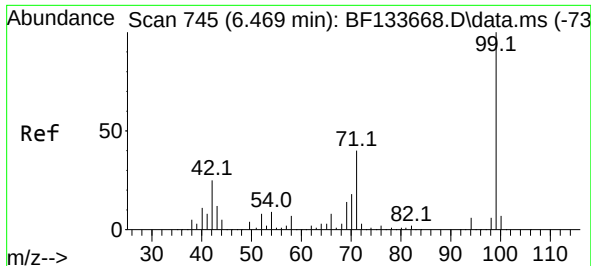

#7
Phenol-d6
Concen: 114.207 ng
RT: 6.498 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF133909.D
Acq: 22 Jun 2023 19:27




Instrument :
BNA_F
ClientSampleId :
PB153649BL


Tgt Ion: 99 Resp: 983362
Ion Ratio Lower Upper
99 100
42 24.1 19.9 29.9
71 38.9 32.2 48.4

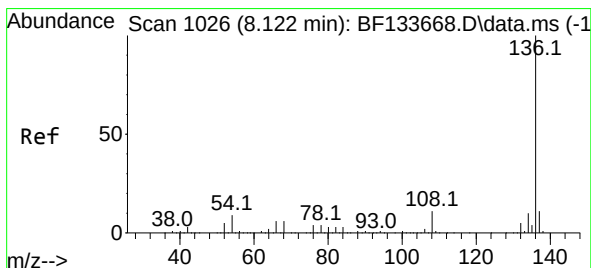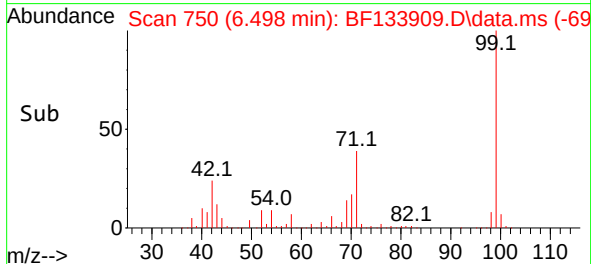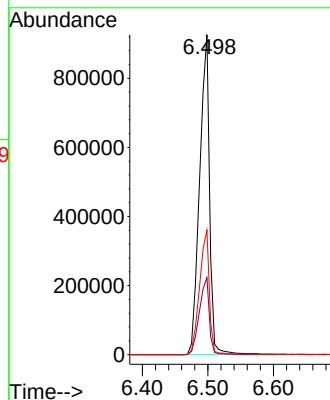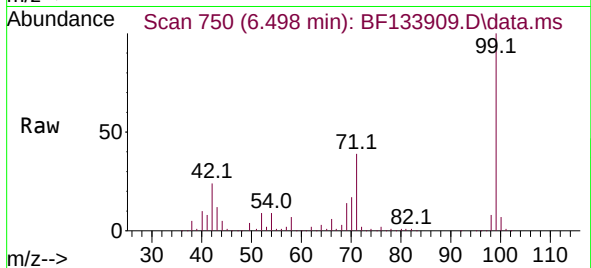

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.140 min Scan# 1029
Delta R.T. 0.000 min
Lab File: BF133909.D
Acq: 22 Jun 2023 19:27

Tgt Ion: 136 Resp: 452358
Ion Ratio Lower Upper
136 100
137 10.7 8.8 13.2
54 7.9 7.4 11.0
68 5.1 4.4 6.6

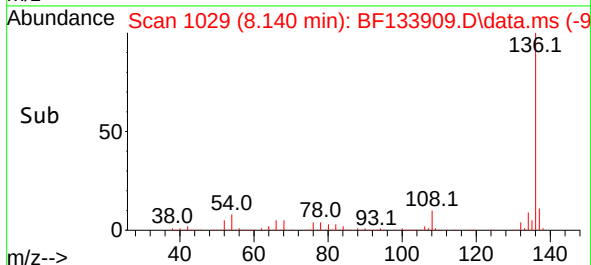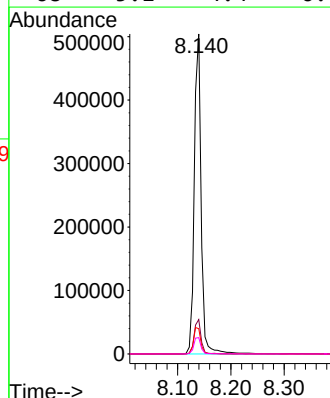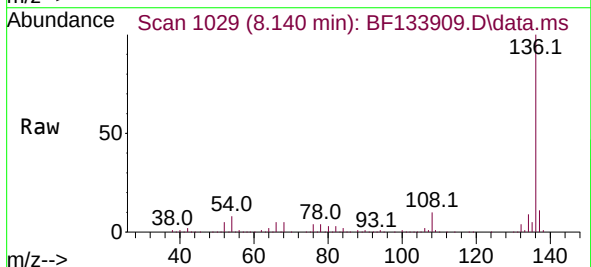

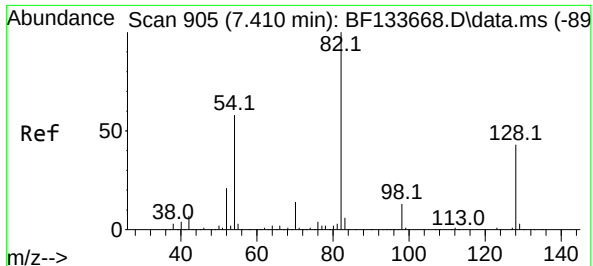

#23

Nitrobenzene-d5

Concen: 79.705 ng

RT: 7.422 min Scan# 905

Delta R.T. -0.006 min

Lab File: BF133909.D

Acq: 22 Jun 2023 19:27

Instrument :

BNA_F

ClientSampleId :

PB153649BL





Tgt Ion: 82 Resp: 661969

Ion Ratio Lower Upper

82 100

128 41.9 34.2 51.2

54 58.6 46.5 69.7

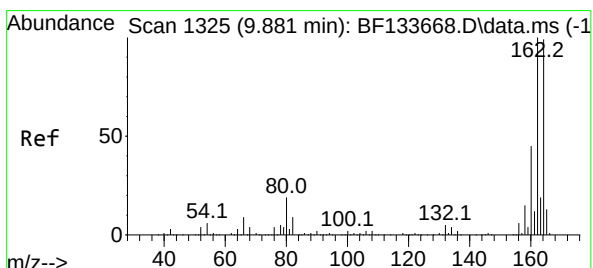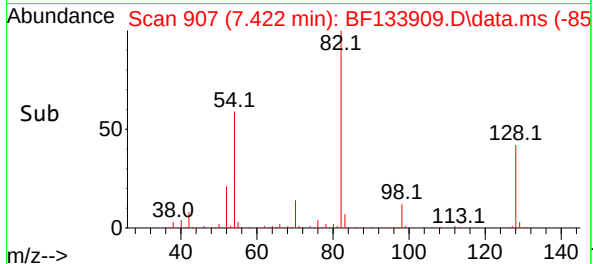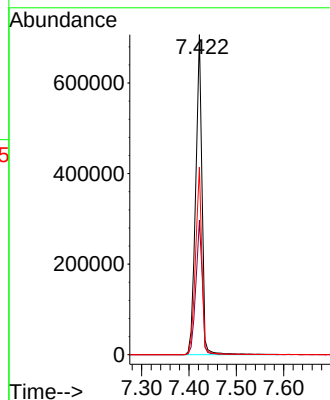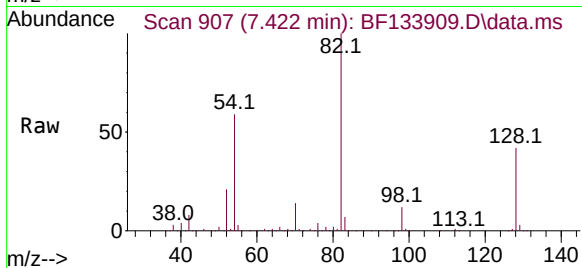

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.898 min Scan# 1328

Delta R.T. 0.000 min

Lab File: BF133909.D

Acq: 22 Jun 2023 19:27




Tgt Ion:164 Resp: 229608


Ion Ratio Lower Upper

164 100

162 101.6 80.8 121.2

160 45.5 36.7 55.1


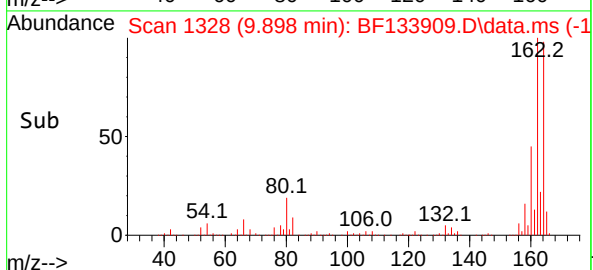
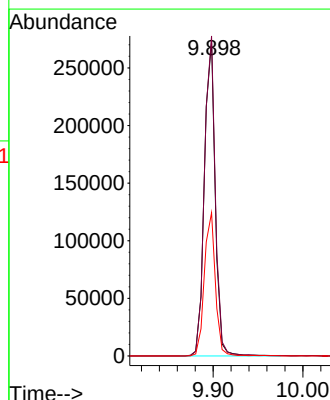
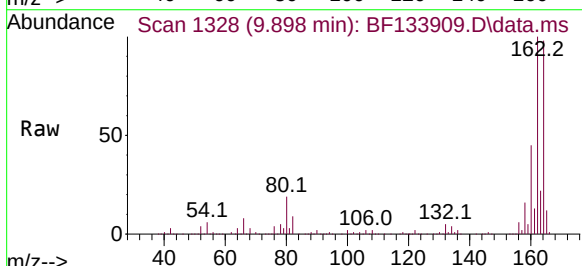


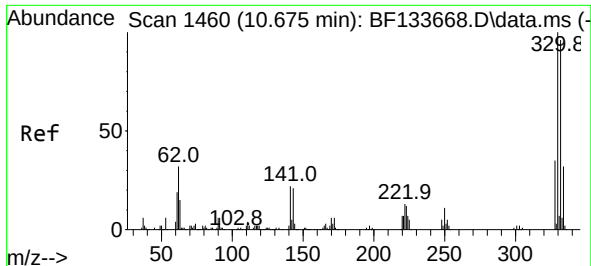

#42
2,4,6-Tribromophenol
Concen: 114.362 ng
RT: 10.692 min Scan# 1463
Delta R.T. -0.006 min
Lab File: BF133909.D
Acq: 22 Jun 2023 19:27




Instrument :
BNA_F
ClientSampleId :
PB153649BL


Tgt Ion:330 Resp: 332384
Ion Ratio Lower Upper
330 100
332 96.9 77.2 115.8
141 31.5 24.9 37.3

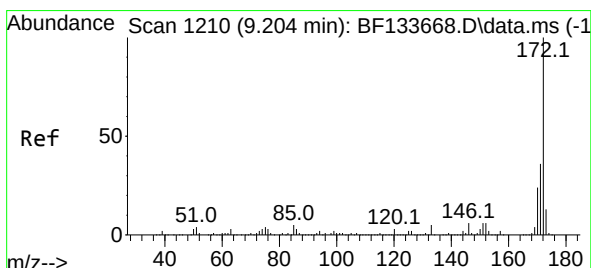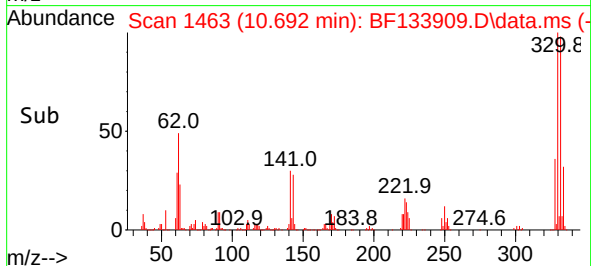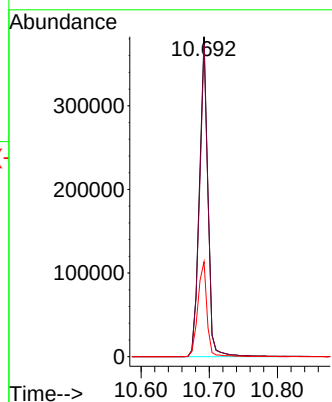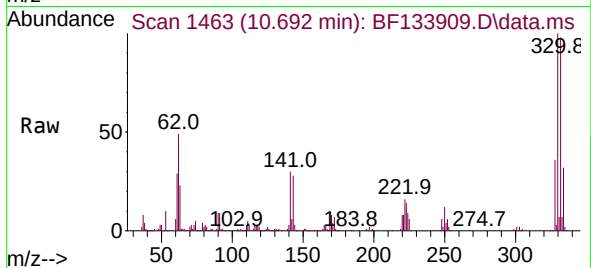

#45
2-Fluorobiphenyl
Concen: 72.027 ng
RT: 9.216 min Scan# 1212
Delta R.T. -0.006 min
Lab File: BF133909.D
Acq: 22 Jun 2023 19:27

Tgt Ion:172 Resp: 1163403
Ion Ratio Lower Upper
172 100
171 36.0 28.6 43.0
170 24.0 19.1 28.7

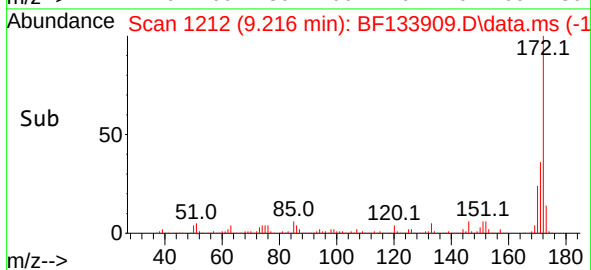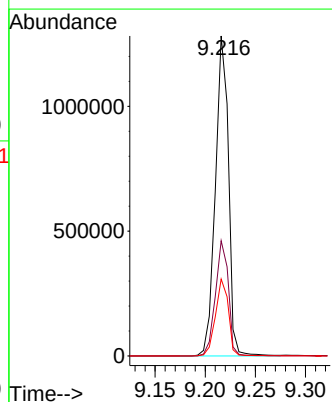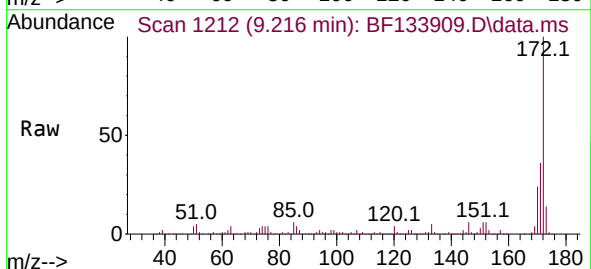

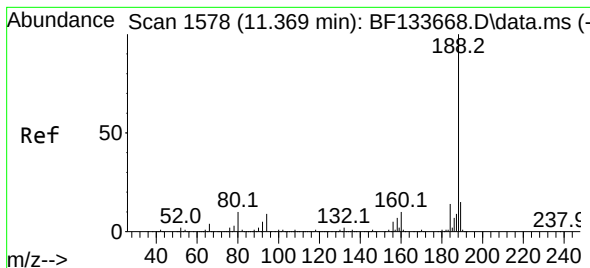

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.392 min Scan# 1

Delta R.T. 0.000 min

Lab File: BF133909.D

Acq: 22 Jun 2023 19:27

Instrument :

BNA_F

ClientSampleId :

PB153649BL





Tgt Ion:188 Resp: 475216

Ion Ratio Lower Upper

188 100

94 8.6 6.8 10.2

80 9.1 7.8 11.6

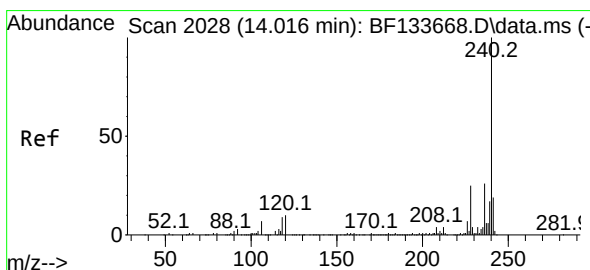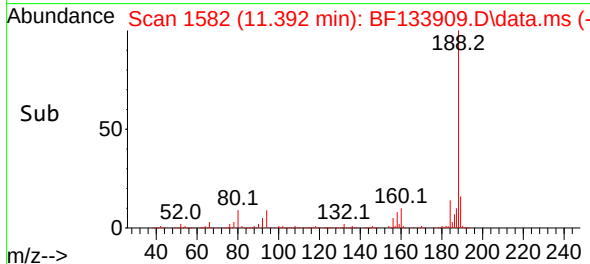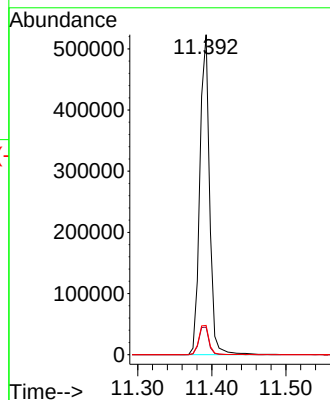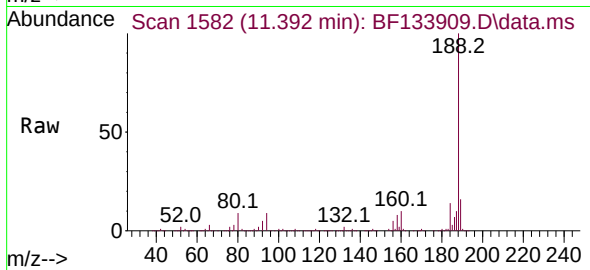

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.051 min Scan# 2034

Delta R.T. -0.006 min

Lab File: BF133909.D

Acq: 22 Jun 2023 19:27




Tgt Ion:240 Resp: 312147


Ion Ratio Lower Upper

240 100

120 9.1 8.1 12.1


236 26.1 20.5 30.7

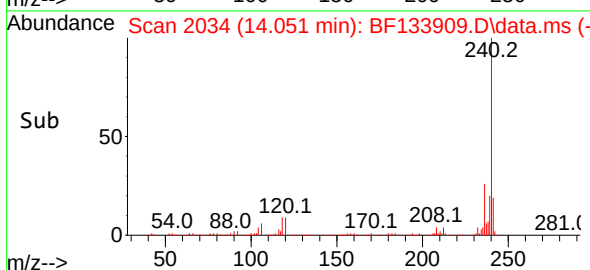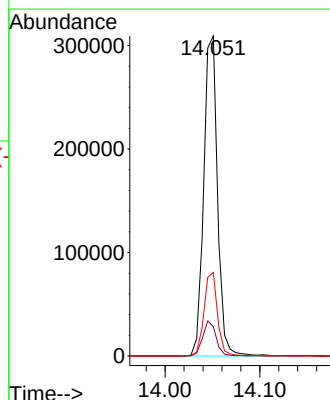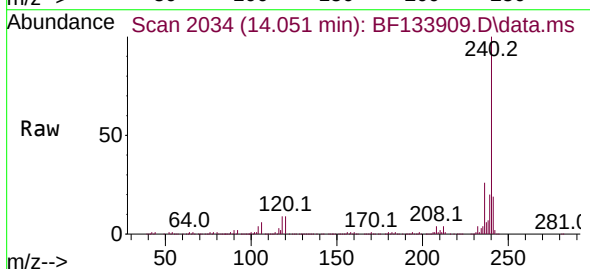



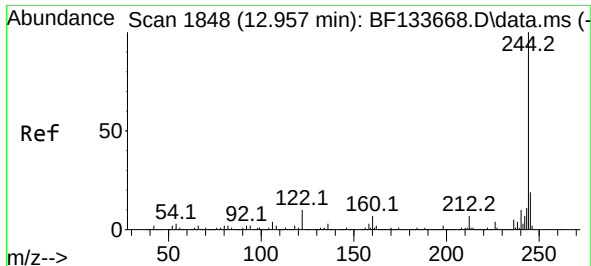


#79
 Terphenyl-d14
 Concen: 78.024 ng
 RT: 12.992 min Scan# 1848
 Delta R.T. 0.000 min
 Lab File: BF133909.D
 Acq: 22 Jun 2023 19:27


Instrument :
 BNA_F
 ClientSampleId :
 PB153649BL

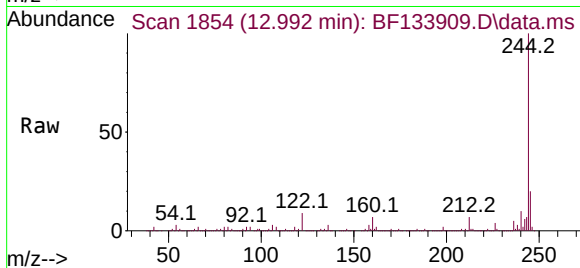

Tgt Ion:244 Resp: 1573987
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.4 8.2
 122 9.5 8.1 12.1

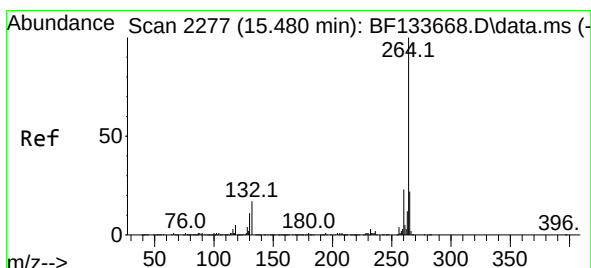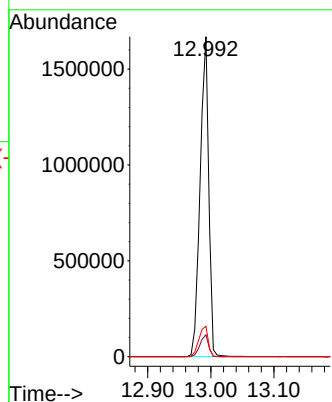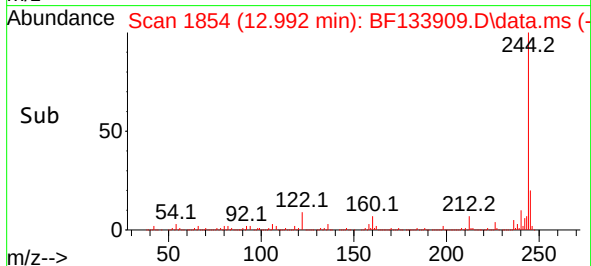

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.557 min Scan# 2290
 Delta R.T. -0.006 min
 Lab File: BF133909.D
 Acq: 22 Jun 2023 19:27

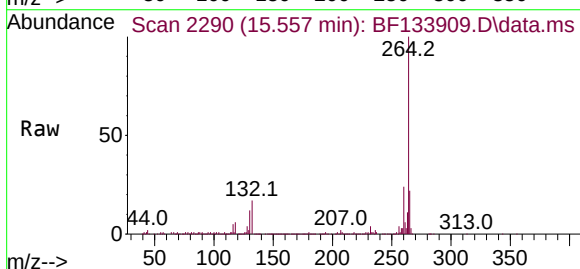

Tgt Ion:264 Resp: 226691
 Ion Ratio Lower Upper
 264 100
 260 24.1 18.2 27.2
 265 21.7 17.8 26.6

