

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062223\
 Data File : BF133919.D
 Acq On : 23 Jun 2023 00:57
 Operator : CG\JU
 Sample : 03321-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-22

Quant Time: Jun 23 05:06:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 23 02:21:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.857	152	99679	20.000	ng	0.00
21) Naphthalene-d8	8.133	136	387421	20.000	ng	0.00
39) Acenaphthene-d10	9.892	164	194566	20.000	ng	0.00
64) Phenanthrene-d10	11.386	188	407300	20.000	ng	0.00
76) Chrysene-d12	14.045	240	303335	20.000	ng	-0.01
86) Perylene-d12	15.551	264	142750	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	771315	134.711	ng	0.02
7) Phenol-d6	6.498	99	884725	118.708	ng	0.00
23) Nitrobenzene-d5	7.422	82	695599	97.793	ng	0.00
42) 2,4,6-Tribromophenol	10.692	330	366326	148.740	ng	0.00
45) 2-Fluorobiphenyl	9.216	172	1264112	92.357	ng	0.00
79) Terphenyl-d14	12.992	244	1677837	85.588	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062223\
Data File : BF133919.D
Acq On : 23 Jun 2023 00:57
Operator : CG\JU
Sample : 03321-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-22

Quant Time: Jun 23 05:06:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 02:21:26 2023
Response via : Initial Calibration




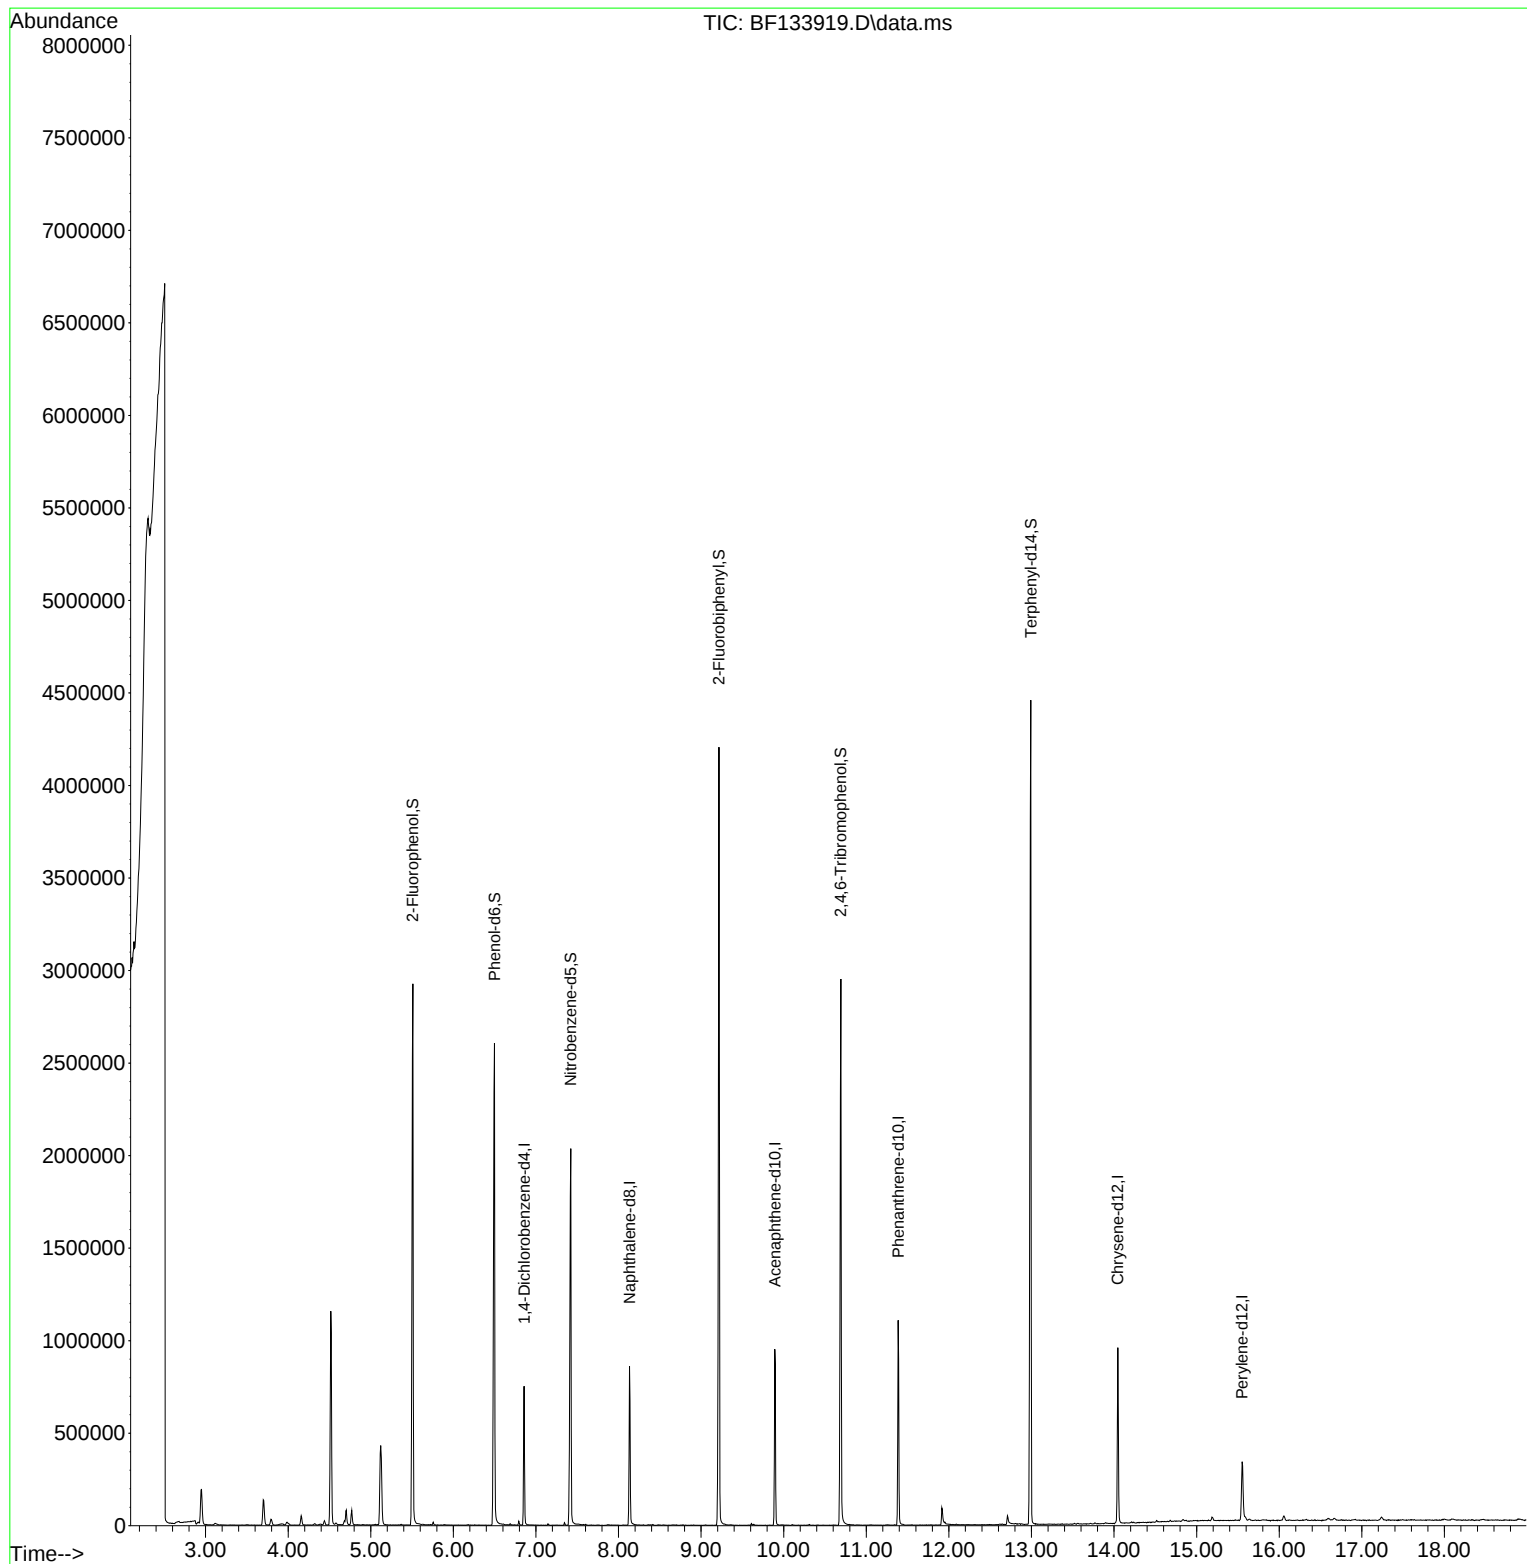




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.857 min Scan# 811
Delta R.T. -0.006 min
Lab File: BF133919.D
Acq: 23 Jun 2023 00:57




Instrument :
BNA_F
ClientSampleId :
WC-22

Tgt Ion:152 Resp: 99679
Ion Ratio Lower Upper
152 100
150 155.6 124.3 186.5
115 59.4 48.5 72.7

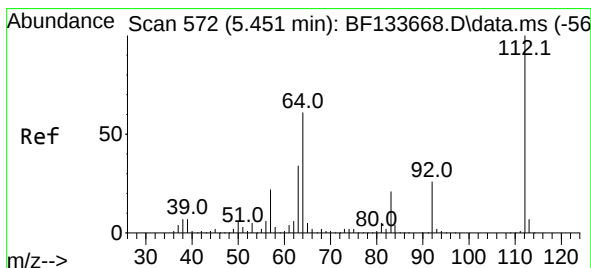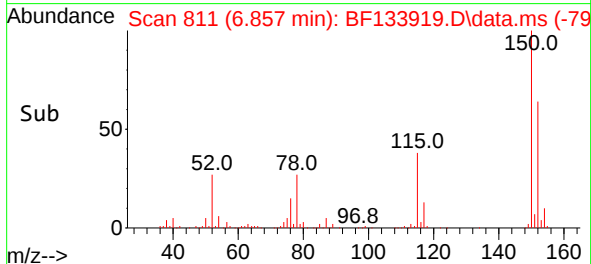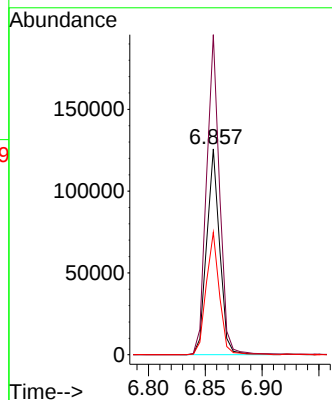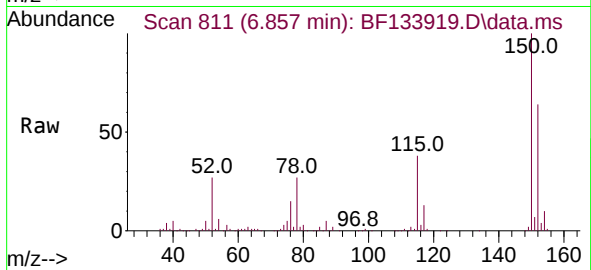

#5
2-Fluorophenol
Concen: 134.711 ng
RT: 5.510 min Scan# 582
Delta R.T. 0.018 min
Lab File: BF133919.D
Acq: 23 Jun 2023 00:57

Tgt Ion:112 Resp: 771315
Ion Ratio Lower Upper
112 100
64 62.7 49.0 73.4
63 35.7 26.8 40.2


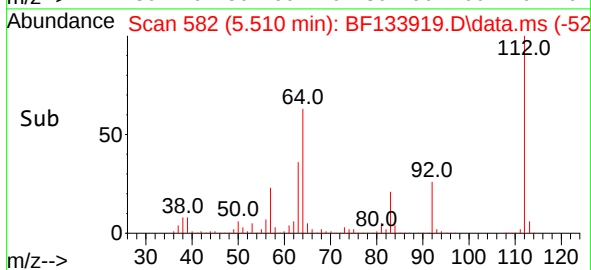
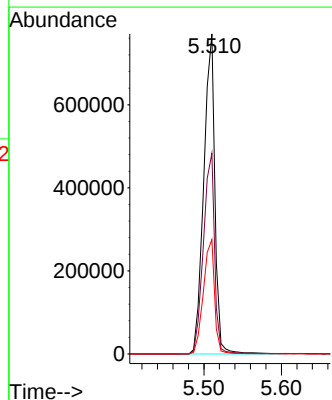
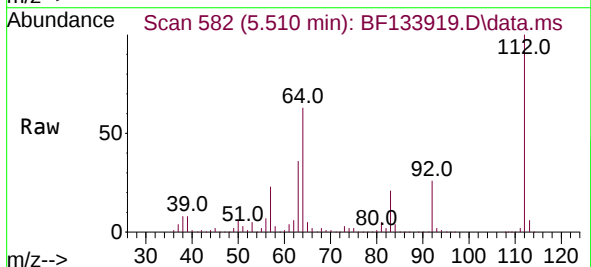




#7
Phenol-d6
Concen: 118.708 ng
RT: 6.498 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF133919.D
Acq: 23 Jun 2023 00:57




Instrument :
BNA_F
ClientSampleId :
WC-22

Tgt Ion: 99 Resp: 884725
Ion Ratio Lower Upper
99 100
42 24.5 19.9 29.9
71 40.5 32.2 48.4

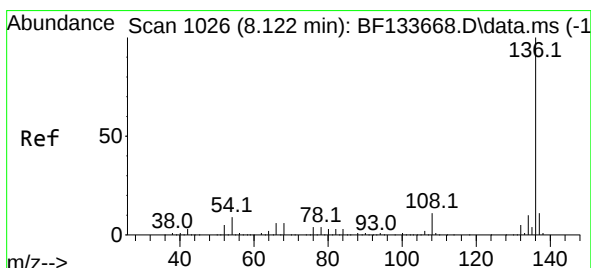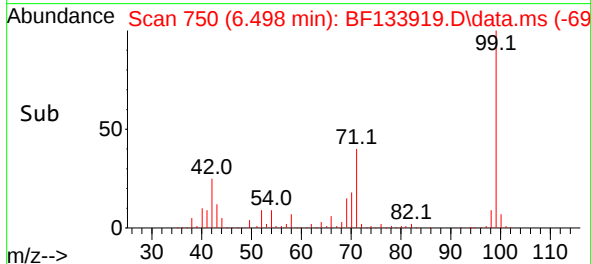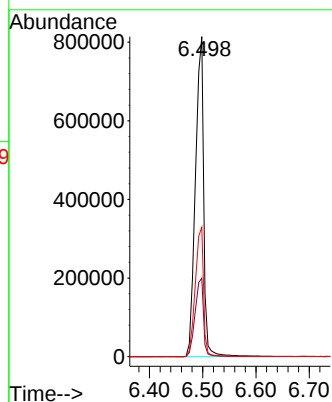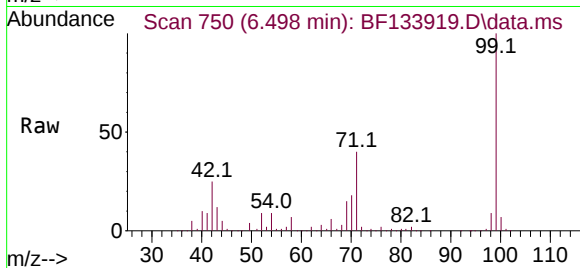

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.133 min Scan# 1028
Delta R.T. -0.006 min
Lab File: BF133919.D
Acq: 23 Jun 2023 00:57

Tgt Ion: 136 Resp: 387421
Ion Ratio Lower Upper
136 100
137 11.2 8.8 13.2
54 9.4 7.4 11.0
68 5.6 4.4 6.6

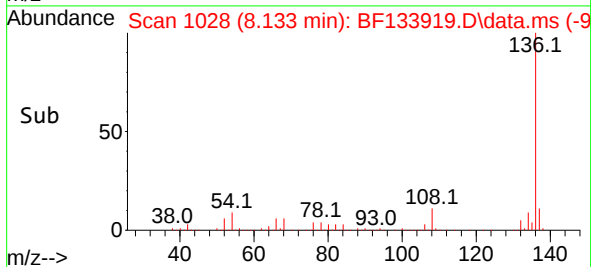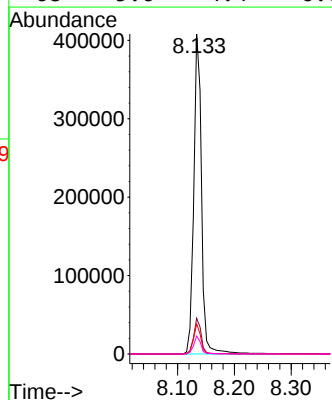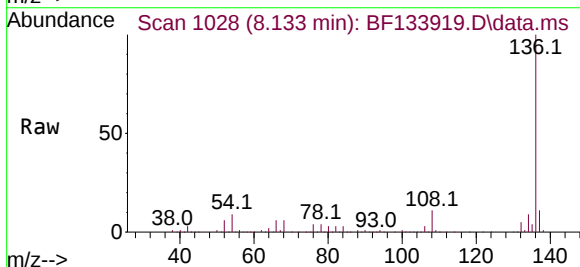



#23

Nitrobenzene-d5

Concen: 97.793 ng

RT: 7.422 min Scan# 90

Delta R.T. -0.006 min

Lab File: BF133919.D

Acq: 23 Jun 2023 00:57

Instrument :

BNA_F

ClientSampleId :

WC-22





Tgt Ion: 82 Resp: 695599

Ion Ratio Lower Upper

82 100

128 41.8 34.2 51.2

54 59.2 46.5 69.7

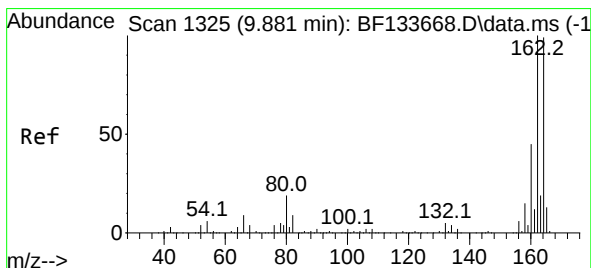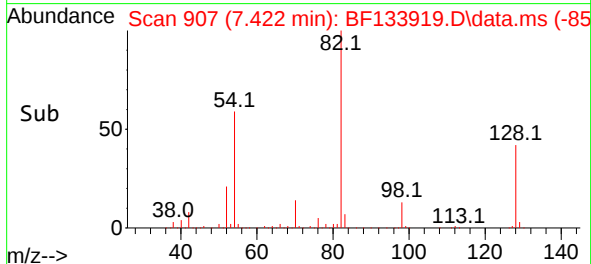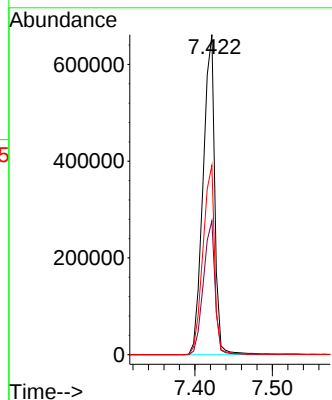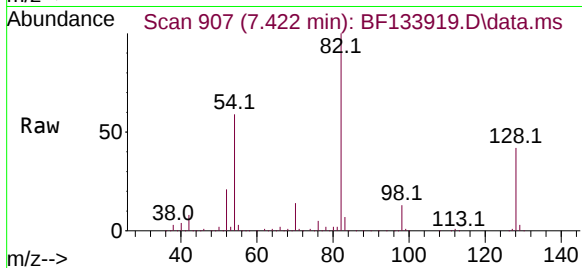

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.892 min Scan# 1327

Delta R.T. -0.006 min

Lab File: BF133919.D

Acq: 23 Jun 2023 00:57




Tgt Ion:164 Resp: 194566


Ion Ratio Lower Upper

164 100

162 101.2 80.8 121.2

160 46.4 36.7 55.1


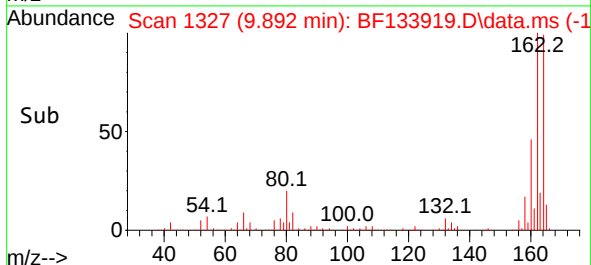
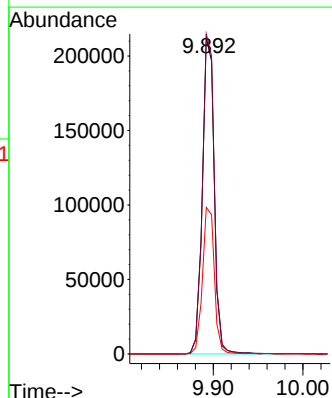
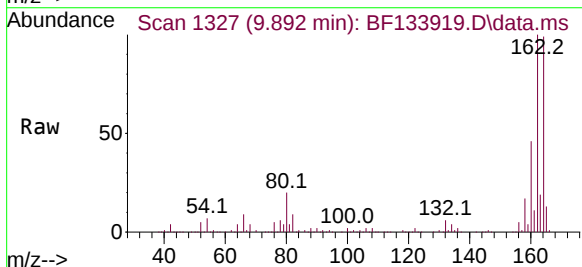


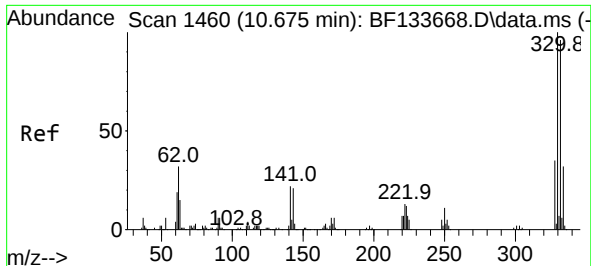

#42
2,4,6-Tribromophenol
Concen: 148.740 ng
RT: 10.692 min Scan# 1463
Delta R.T. -0.006 min
Lab File: BF133919.D
Acq: 23 Jun 2023 00:57




Instrument :
BNA_F
ClientSampleId :
WC-22

Tgt Ion:330 Resp: 366326
Ion Ratio Lower Upper
330 100
332 96.6 77.2 115.8
141 32.0 24.9 37.3

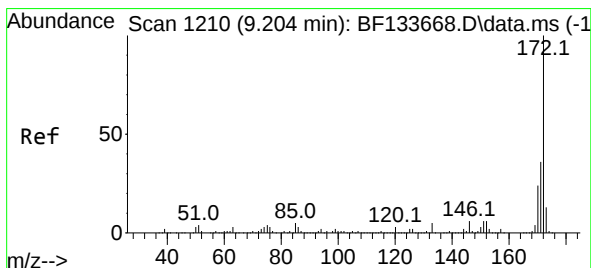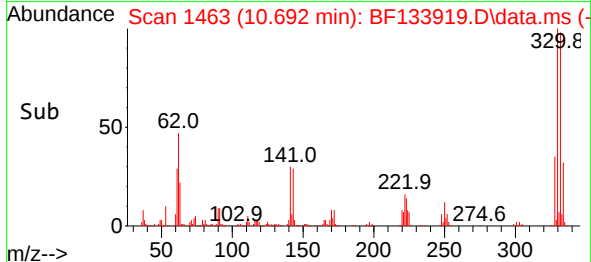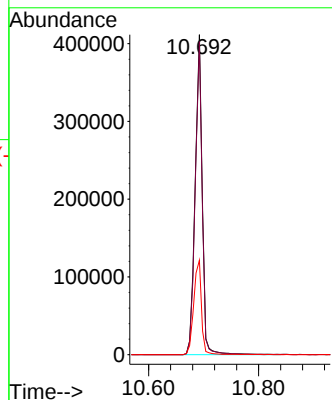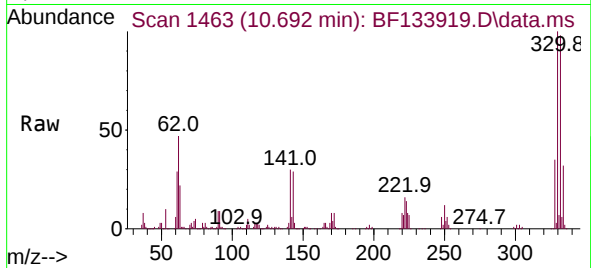

#45
2-Fluorobiphenyl
Concen: 92.357 ng
RT: 9.216 min Scan# 1212
Delta R.T. -0.006 min
Lab File: BF133919.D
Acq: 23 Jun 2023 00:57

Tgt Ion:172 Resp: 1264112
Ion Ratio Lower Upper
172 100
171 35.5 28.6 43.0
170 24.0 19.1 28.7


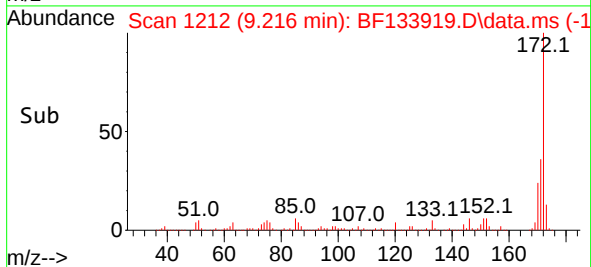
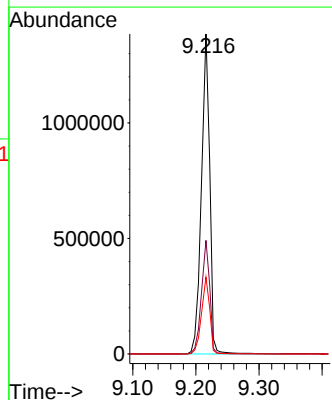
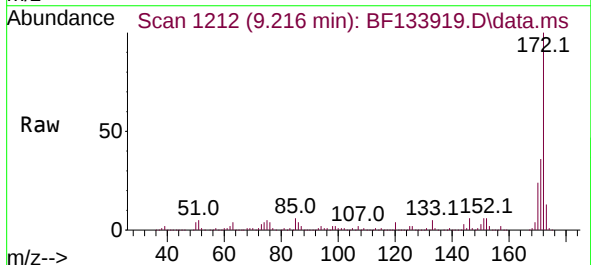




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.386 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF133919.D
Acq: 23 Jun 2023 00:57




Instrument :
BNA_F
ClientSampleId :
WC-22

Tgt Ion:188 Resp: 407300
Ion Ratio Lower Upper
188 100
94 8.8 6.8 10.2
80 10.1 7.8 11.6

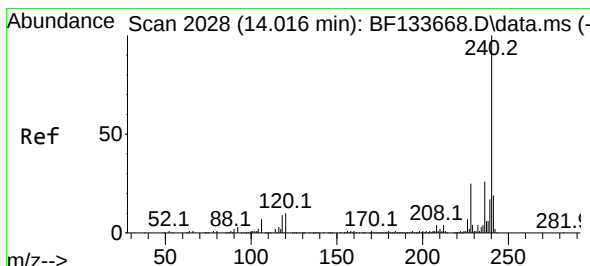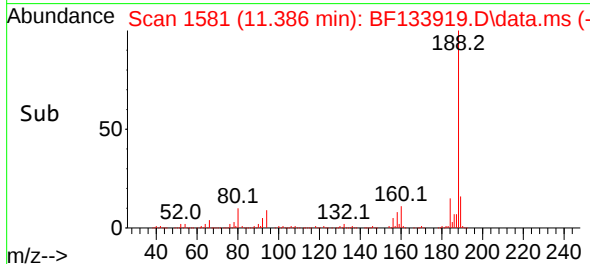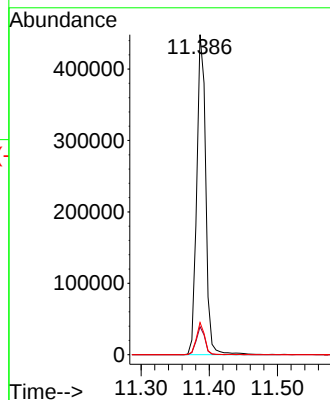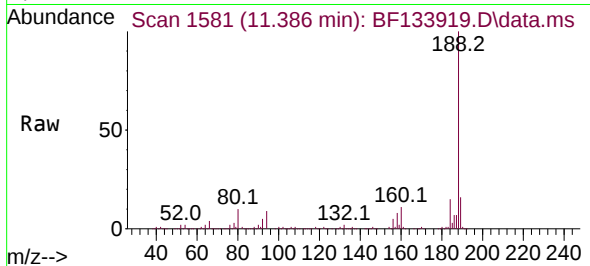

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.045 min Scan# 2033
Delta R.T. -0.012 min
Lab File: BF133919.D
Acq: 23 Jun 2023 00:57

Tgt Ion:240 Resp: 303335
Ion Ratio Lower Upper
240 100
120 10.3 8.1 12.1
236 26.3 20.5 30.7


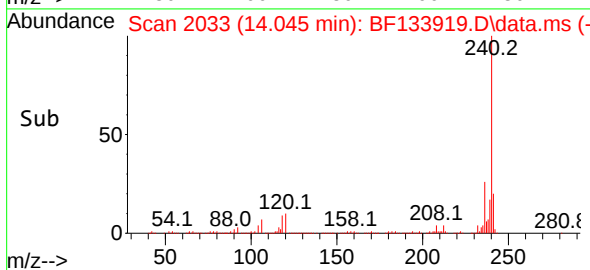
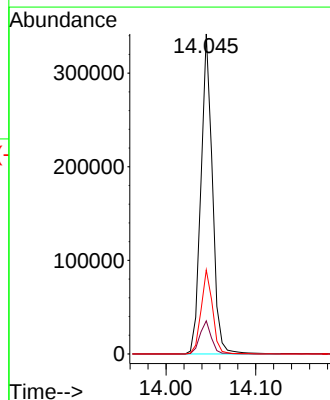
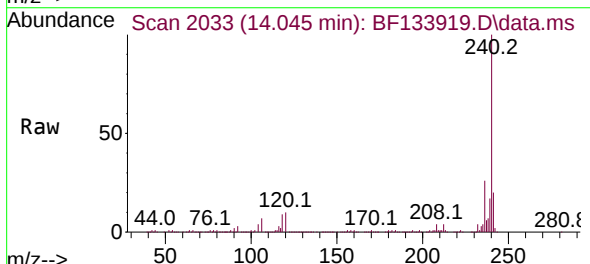




#79
 Terphenyl-d14
 Concen: 85.588 ng
 RT: 12.992 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: BF133919.D
 Acq: 23 Jun 2023 00:57

Instrument :
 BNA_F
 ClientSampleId :
 WC-22

Tgt Ion:244 Resp: 1677837
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.4 8.2
 122 9.2 8.1 12.1

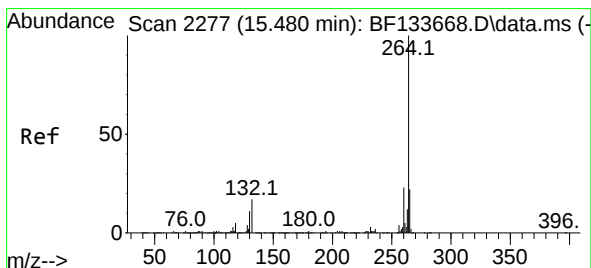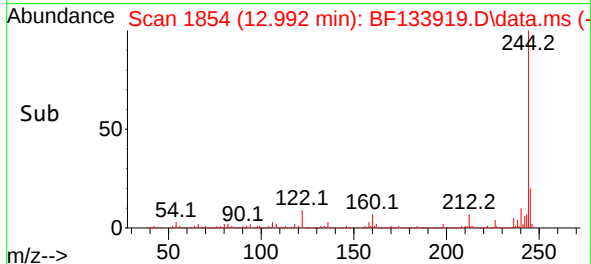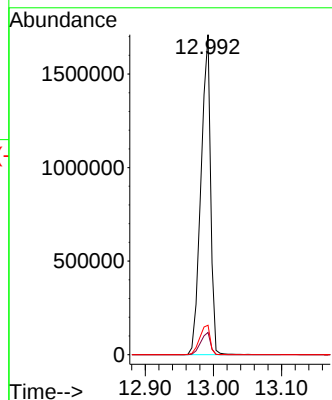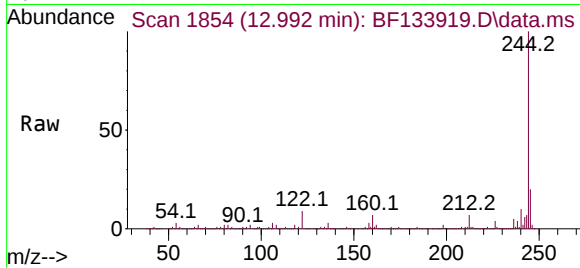

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.551 min Scan# 2289
 Delta R.T. -0.012 min
 Lab File: BF133919.D
 Acq: 23 Jun 2023 00:57

Tgt Ion:264 Resp: 142750
 Ion Ratio Lower Upper
 264 100
 260 24.0 18.2 27.2
 265 20.8 17.8 26.6

