
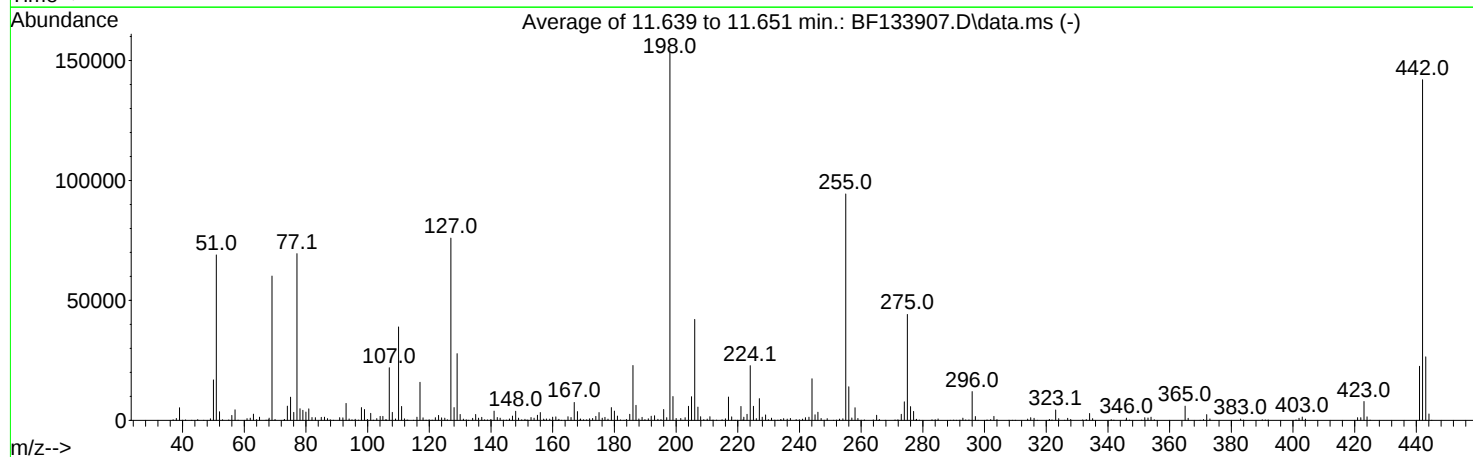


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062223\
 Data File : BF133907.D
 Acq On : 22 Jun 2023 18:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 23 02:21:26 2023

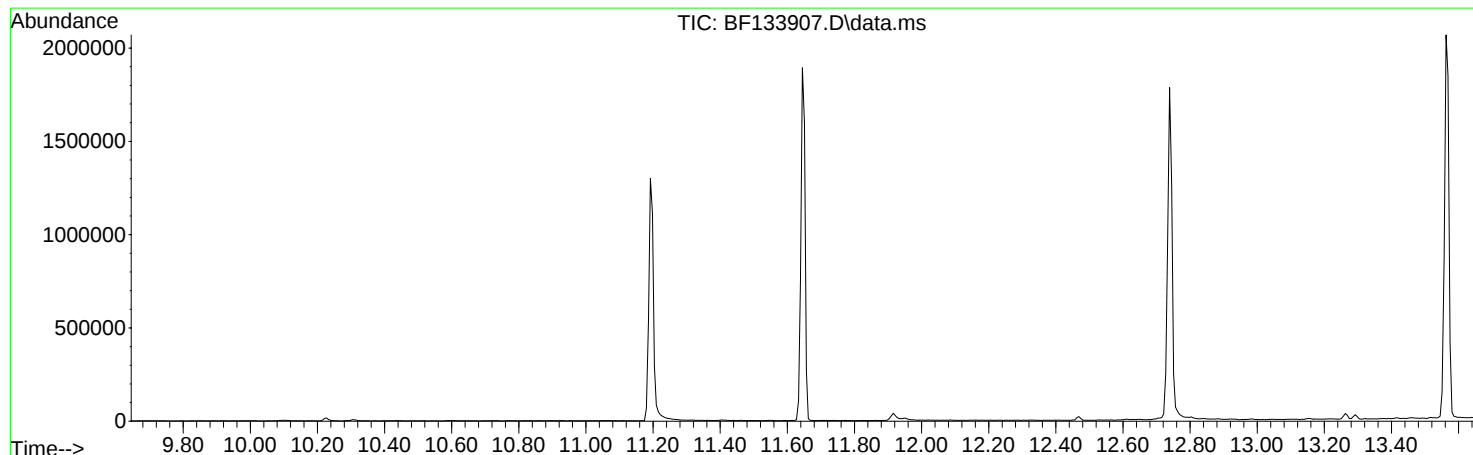

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	68981	PASS
68	69	0.00	2	1.6	933	PASS
69	198	0.00	100	39.2	60128	PASS
70	69	0.00	2	0.7	404	PASS
127	198	10	80	49.6	75989	PASS
197	198	0.00	2	0.7	1143	PASS
198	198	100	100	100.0	153333	PASS
199	198	5	9	6.5	9921	PASS
275	198	10	60	28.8	44157	PASS
365	198	1	100	3.9	5949	PASS
441	198	0.01	100	14.7	22579	PASS
442	442	50	100	100.0	141979	PASS
443	442	15	24	18.7	26501	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/22/2023	BNA_F	<u>BF133907.D</u>
Compound Name	Response	Retention Time
DDT	372974	13.563
DDD	8583	13.263
DDE	513	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9096	382070	2.38

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062223\
Data File : BF133907.D
Acq On : 22 Jun 2023 18:23
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 23 04:16:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 02:21:26 2023
Response via : Initial Calibration

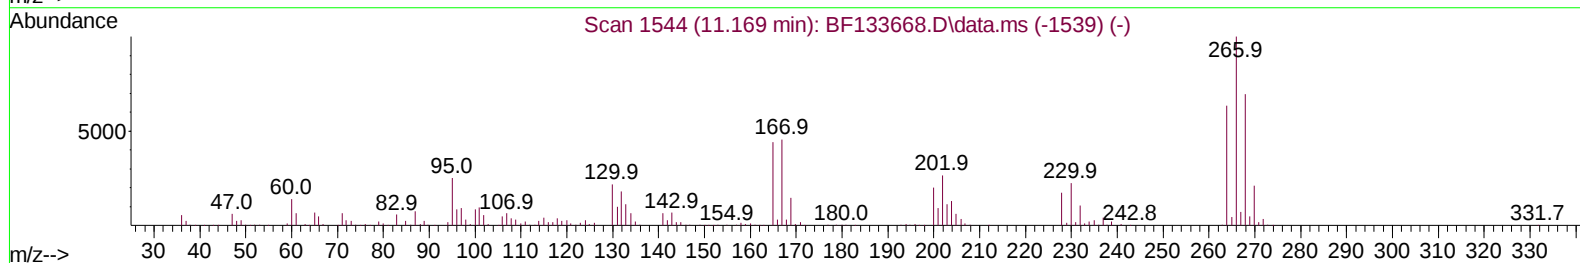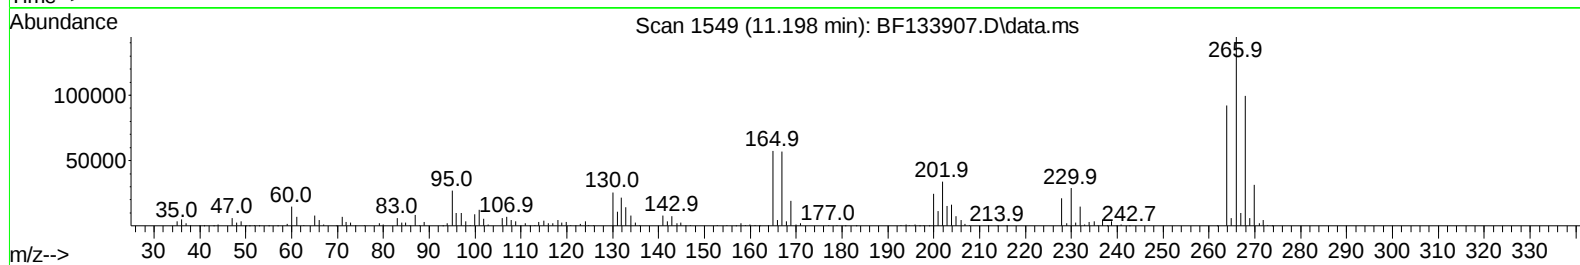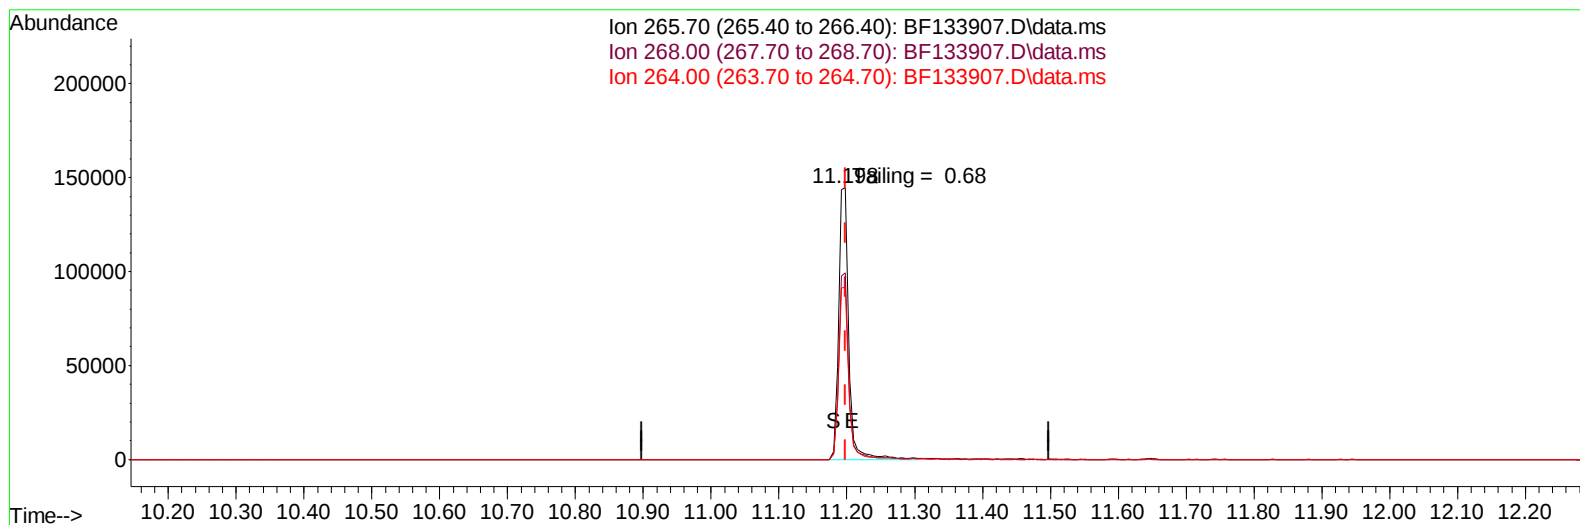

TIC: BF133907.D\data.ms

(70) Pentachlorophenol (C)

11.198min (+ 0.000) 37567.30 ng




response 148385

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	68.73
264.00	63.40	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062223\
 Data File : BF133907.D
 Acq On : 22 Jun 2023 18:23
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 23 04:16:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 23 02:21:26 2023
 Response via : Initial Calibration

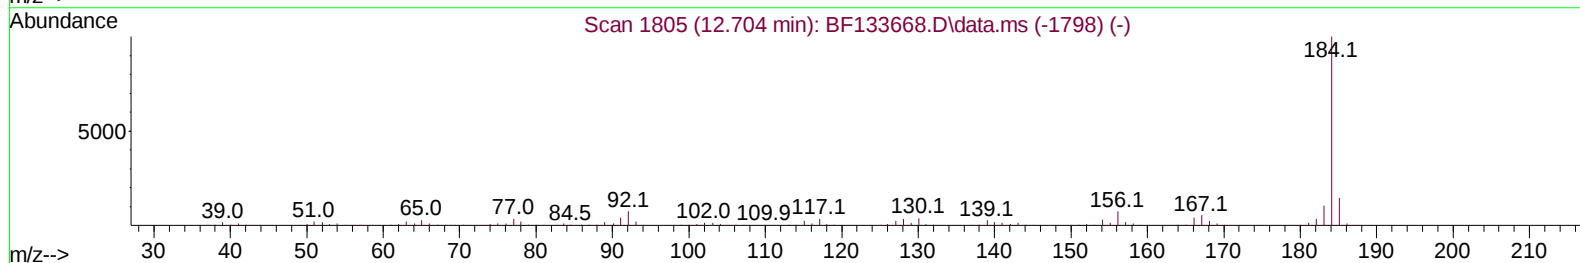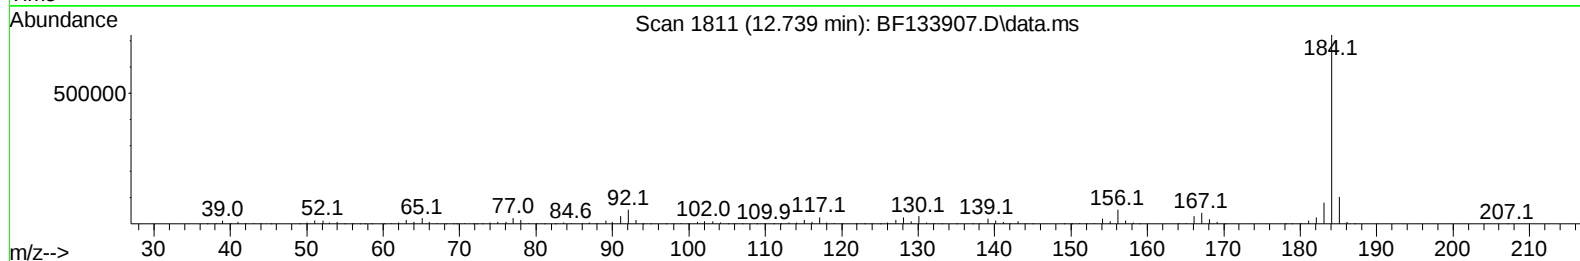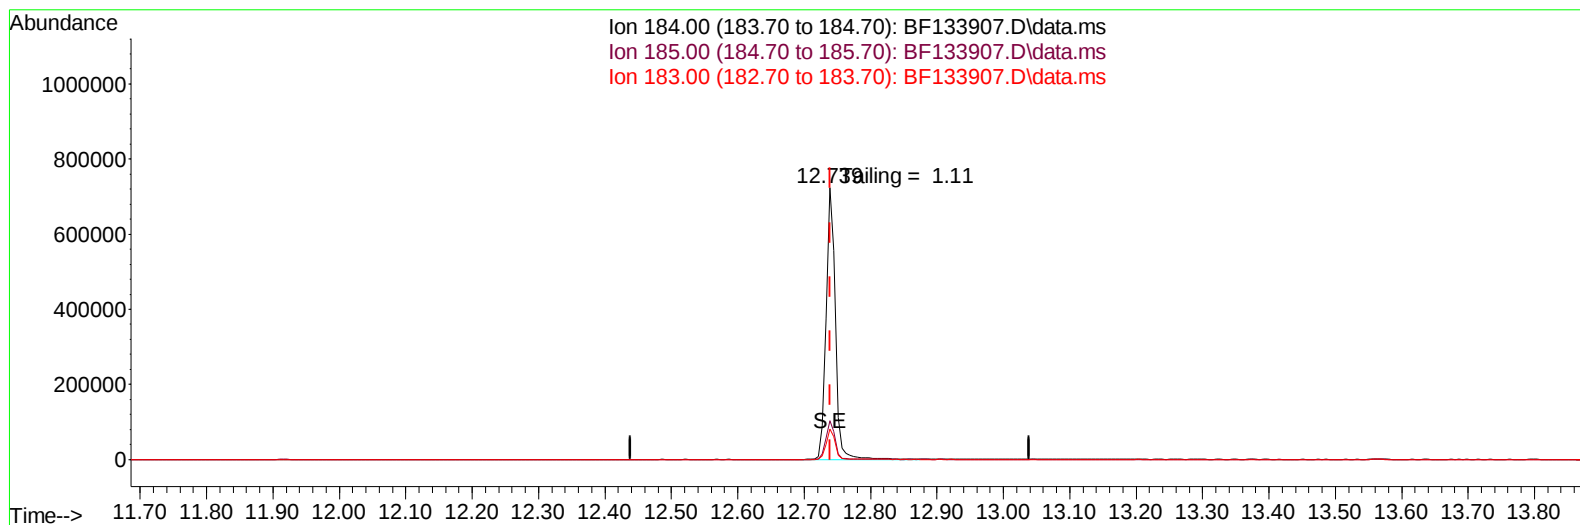

TIC: BF133907.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 120039.97 ng

response 696854

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.33
183.00	10.50	11.20
0.00	0.00	0.00