

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062323\
 Data File : BF133946.D
 Acq On : 23 Jun 2023 16:48
 Operator : CG\JU
 Sample : 03331-08 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMPOSITE-SB17

Quant Time: Jun 23 18:35:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 23 02:21:26 2023
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :mohammad ahmed 06/27/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.863	152	93853	20.000	ng	0.00
21) Naphthalene-d8	8.139	136	316370	20.000	ng	0.00
39) Acenaphthene-d10	9.898	164	132327	20.000	ng	0.00
64) Phenanthrene-d10	11.392	188	236777	20.000	ng	0.00
76) Chrysene-d12	14.062	240	143755	20.000	ng	0.00
86) Perylene-d12	15.574	264	127918	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.498	112	332259	61.631	ng	0.00
7) Phenol-d6	6.498	99	382063	54.446	ng	0.00
23) Nitrobenzene-d5	7.422	82	243623	41.943	ng	0.00
42) 2,4,6-Tribromophenol	10.692	330	87628	52.314	ng	0.00
45) 2-Fluorobiphenyl	9.216	172	436000	46.837	ng	0.00
79) Terphenyl-d14	12.992	244	424866	45.732	ng	0.00
Target Compounds						
						Qvalue
31) Naphthalene	8.163	128	30894	2.004	ng	99
49) Acenaphthylene	9.757	152	76082	5.710	ng	97
52) Acenaphthene	9.933	154	57692	7.397	ng	96
55) Dibenzofuran	10.104	168	44803	3.765	ng	97
58) Fluorene	10.451	166	87178	9.579	ng	100
71) Phenanthrene	11.421	178	1082144	90.082	ng	99
72) Anthracene	11.469	178	339098	27.072	ng	100
73) Carbazole	11.627	167	69202	5.932	ng	97
74) Di-n-butylphthalate	11.957	149	81840	5.472	ng	100
75) Fluoranthene	12.627	202	1876179	147.072	ng	99
78) Pyrene	12.857	202	1766397	131.906	ng	98
80) Butylbenzylphthalate	13.486	149	1693260	299.514	ng	94
81) Benzo(a)anthracene	14.057	228	725154	72.927	ng	96
83) Chrysene	14.092	228	722801	76.854	ng	98
84) Bis(2-ethylhexyl)phtha...	14.045	149	2163855	310.858	ng	# 98
87) Indeno(1,2,3-cd)pyrene	17.133	276	275284	31.281	ng	94
88) Benzo(b)fluoranthene	15.133	252	726389m	93.481	ng	
89) Benzo(k)fluoranthene	15.156	252	276781m	36.566	ng	
90) Benzo(a)pyrene	15.515	252	532111	73.785	ng	98
91) Dibenzo(a,h)anthracene	17.145	278	74192	10.183	ng	97
92) Benzo(g,h,i)perylene	17.603	276	247180	34.218	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062323\
Data File : BF133946.D
Acq On : 23 Jun 2023 16:48
Operator : CG\JU
Sample : 03331-08 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
COMPOSITE-SB17

Quant Time: Jun 23 18:35:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 02:21:26 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023



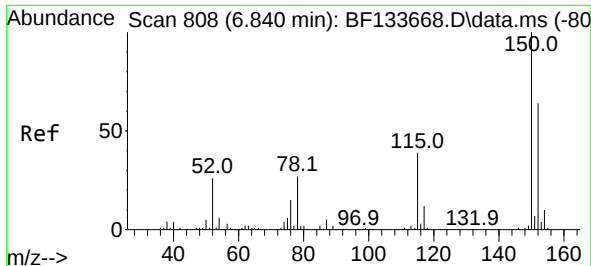

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.863 min Scan# 812
Delta R.T. -0.000 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Instrument :
BNA_F
ClientSampleId :
COMPOSITE-SB17



Tgt Ion:152 Resp: 9385
Ion Ratio Lower Upper
152 100
150 151.7 124.3 186.5
115 56.8 48.5 72.7




Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023



#5
2-Fluorophenol
Concen: 61.631 ng
RT: 5.498 min Scan# 580
Delta R.T. 0.006 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48


Tgt Ion:112 Resp: 332259
Ion Ratio Lower Upper
112 100
64 60.1 49.0 73.4
63 34.1 26.8 40.2





#7
Phenol-d6
Concen: 54.446 ng
RT: 6.498 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Instrument :
BNA_F
ClientSampleId :
COMPOSITE-SB17




Tgt Ion: 99 Resp: 38206
Ion Ratio Lower Upper
99 100
42 24.1 19.9 29.9
71 39.2 32.2 48.4

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.139 min Scan# 1029
Delta R.T. 0.000 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48



Tgt Ion:136 Resp: 316370
Ion Ratio Lower Upper
136 100
137 11.0 8.8 13.2
54 8.2 7.4 11.0
68 5.3 4.4 6.6



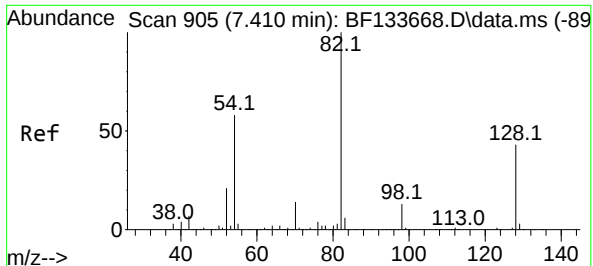

#23

Nitrobenzene-d5

Concen: 41.943 ng

RT: 7.422 min Scan# 905

Delta R.T. -0.006 min

Lab File: BF133946.D

Acq: 23 Jun 2023 16:48

Instrument :

BNA_F

ClientSampleId :

COMPOSITE-SB17

Tgt Ion: 82 Resp: 24362

Ion Ratio Lower Upper

82 100

128 43.5 34.2 51.2





54 56.7 46.5 69.7

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/26/2023

Supervised By :mohammad ahmed 06/27/2023



#31

Naphthalene

Concen: 2.004 ng

RT: 8.163 min Scan# 1033

Delta R.T. 0.000 min

Lab File: BF133946.D

Acq: 23 Jun 2023 16:48




Tgt Ion:128 Resp: 30894


Ion Ratio Lower Upper

128 100

129 12.0 8.9 13.3


127 13.4 10.5 15.7





#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.898 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Instrument :
BNA_F
ClientSampleId :
COMPOSITE-SB17




Tgt Ion:164 Resp: 13232
Ion Ratio Lower Upper
164 100
162 101.2 80.8 121.2
160 45.3 36.7 55.1

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023




#42
2,4,6-Tribromophenol
Concen: 52.314 ng
RT: 10.692 min Scan# 1463
Delta R.T. -0.006 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48



Tgt Ion:330 Resp: 87628
Ion Ratio Lower Upper
330 100
332 96.2 77.2 115.8
141 35.6 24.9 37.3





#45

2-Fluorobiphenyl

Concen: 46.837 ng

RT: 9.216 min Scan# 11

Delta R.T. -0.006 min

Lab File: BF133946.D


Acq: 23 Jun 2023 16:48

Instrument :

BNA_F

ClientSampleId :

COMPOSITE-SB17



Tgt Ion:172 Resp: 436000

Ion Ratio Lower Upper

172 100

171 35.4 28.6 43.0




170 23.6 19.1 28.7

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/26/2023

Supervised By :mohammad ahmed 06/27/2023



#49

Acenaphthylene

Concen: 5.710 ng

RT: 9.757 min Scan# 1304

Delta R.T. -0.006 min

Lab File: BF133946.D

Acq: 23 Jun 2023 16:48




Tgt Ion:152 Resp: 76082


Ion Ratio Lower Upper

152 100

151 18.7 16.2 24.4


153 13.5 10.4 15.6





#52
Acenaphthene
Concen: 7.397 ng
RT: 9.933 min Scan# 1334
Delta R.T. 0.000 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Instrument :
BNA_F
ClientSampleId :
COMPOSITE-SB17




Tgt Ion:154 Resp: 57692
Ion Ratio Lower Upper
154 100
153 117.4 89.8 134.8
152 56.1 43.4 65.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023




#55
Dibenzofuran
Concen: 3.765 ng
RT: 10.104 min Scan# 1363
Delta R.T. -0.006 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Tgt Ion:168 Resp: 44803
Ion Ratio Lower Upper
168 100
139 39.5 30.9 46.3
169 16.3 10.9 16.3





#58
Fluorene
Concen: 9.579 ng
RT: 10.451 min Scan# 1419
Delta R.T. 0.000 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Instrument :
BNA_F
ClientSampleId :
COMPOSITE-SB17



Tgt Ion:166 Resp: 87178
Ion Ratio Lower Upper
166 100
165 91.8 73.1 109.7
167 13.0 10.5 15.7




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.392 min Scan# 1582
Delta R.T. 0.000 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48


Tgt Ion:188 Resp: 236777
Ion Ratio Lower Upper
188 100
94 8.8 6.8 10.2
80 9.5 7.8 11.6





#71
Phenanthrene
Concen: 90.082 ng
RT: 11.421 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Instrument :
BNA_F
ClientSampleId :
COMPOSITE-SB17



Tgt Ion:178 Resp: 108214
Ion Ratio Lower Upper
178 100
176 19.9 15.6 23.4
179 16.0 12.4 18.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023



#72
Anthracene
Concen: 27.072 ng
RT: 11.469 min Scan# 1595
Delta R.T. -0.006 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48


Tgt Ion:178 Resp: 339098
Ion Ratio Lower Upper
178 100
176 18.8 15.1 22.7
179 16.0 12.6 18.8





#73
 Carbazole
 Concen: 5.932 ng
 RT: 11.627 min Scan# 1622
 Delta R.T. 0.000 min
 Lab File: BF133946.D
 Acq: 23 Jun 2023 16:48




Instrument :
 BNA_F
 ClientSampleId :
 COMPOSITE-SB17




Tgt Ion:167 Resp: 6920
 Ion Ratio Lower Upper
 167 100
 166 22.0 17.0 25.6
 139 12.0 11.2 16.8

Manual Integrations
 APPROVED



Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :mohammad ahmed 06/27/2023




#74
 Di-n-butylphthalate
 Concen: 5.472 ng
 RT: 11.957 min Scan# 1678
 Delta R.T. 0.000 min
 Lab File: BF133946.D
 Acq: 23 Jun 2023 16:48




Tgt Ion:149 Resp: 81840
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.4 11.0
 104 5.0 3.8 5.8





#75
Fluoranthene
Concen: 147.072 ng
RT: 12.627 min Scan# 11
Delta R.T. 0.012 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Instrument :
BNA_F
ClientSampleId :
COMPOSITE-SB17




Tgt Ion:202 Resp: 1876179
Ion Ratio Lower Upper
202 100
101 9.8 0.0 29.6
203 18.2 0.0 37.4

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023




#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.062 min Scan# 2036
Delta R.T. 0.006 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Tgt Ion:240 Resp: 143755
Ion Ratio Lower Upper
240 100
120 9.7 8.1 12.1
236 25.6 20.5 30.7





#78
Pyrene
Concen: 131.906 ng
RT: 12.857 min Scan# 1831
Delta R.T. 0.012 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Instrument :
BNA_F
ClientSampleId :
COMPOSITE-SB17




Tgt Ion:202 Resp: 176639
Ion Ratio Lower Upper
202 100
200 20.8 16.2 24.2
203 18.8 13.9 20.9

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023




#79
Terphenyl-d14
Concen: 45.732 ng
RT: 12.992 min Scan# 1854
Delta R.T. 0.000 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Tgt Ion:244 Resp: 424866
Ion Ratio Lower Upper
244 100
212 7.1 5.4 8.2
122 9.7 8.1 12.1





#80
Butylbenzylphthalate
Concen: 299.514 ng
RT: 13.486 min Scan# 1929
Delta R.T. 0.018 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Instrument :
BNA_F
ClientSampleId :
COMPOSITE-SB17



Tgt Ion:149 Resp: 1693260
Ion Ratio Lower Upper
149 100
91 73.0 54.0 81.0
206 20.7 15.6 23.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023



#81
Benzo(a)anthracene
Concen: 72.927 ng
RT: 14.057 min Scan# 2035
Delta R.T. 0.012 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48

Tgt Ion:228 Resp: 725154
Ion Ratio Lower Upper
228 100
226 29.1 21.7 32.5
229 21.6 15.4 23.2





#83

Chrysene

Concen: 76.854 ng

RT: 14.092 min Scan# 2032

Delta R.T. 0.012 min

Lab File: BF133946.D

Acq: 23 Jun 2023 16:48

Instrument :

BNA_F

ClientSampleId :

COMPOSITE-SB17





Tgt Ion:228 Resp: 722800
 Ion Ratio Lower Upper
 228 100
 226 31.4 25.0 37.6
 229 22.6 15.8 23.8

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/26/2023

Supervised By :mohammad ahmed 06/27/2023



#84

Bis(2-ethylhexyl)phthalate

Concen: 310.858 ng




RT: 14.045 min Scan# 2033


Delta R.T. 0.018 min

Lab File: BF133946.D

Acq: 23 Jun 2023 16:48

Tgt Ion:149 Resp: 2163855
 Ion Ratio Lower Upper
 149 100
 167 28.0 21.8 32.8
 279 5.2 3.3 4.9#





#86

Perylene-d12

Concen: 20.000 ng

RT: 15.574 min Scan# 21

Delta R.T. 0.012 min

Lab File: BF133946.D

Acq: 23 Jun 2023 16:48

Instrument :

BNA_F

ClientSampleId :





COMPOSITE-SB17

Tgt Ion:264	Resp:	127918
Ion Ratio	Lower	Upper
264	100	
260	23.8	18.2 27.2
265	25.4	17.8 26.6

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023



#87

Indeno(1,2,3-cd)pyrene

Concen: 31.281 ng




RT: 17.133 min Scan# 2558


Delta R.T. 0.012 min

Lab File: BF133946.D

Acq: 23 Jun 2023 16:48


Tgt Ion:276	Resp:	275284
Ion Ratio	Lower	Upper
276	100	
138	18.6	17.9 26.9
277	23.6	20.3 30.5





#88
Benzo(b)fluoranthene
Concen: 93.481 ng m
RT: 15.133 min Scan# 2118
Delta R.T. 0.018 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48




Instrument :
BNA_F
ClientSampleId :
COMPOSITE-SB17



Tgt Ion:252 Resp: 726389
Ion Ratio Lower Upper
252 100
253 22.8 17.0 25.6
125 10.4 7.3 10.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 06/26/2023
Supervised By :mohammad ahmed 06/27/2023



#89
Benzo(k)fluoranthene
Concen: 36.566 ng m
RT: 15.156 min Scan# 2222
Delta R.T. 0.012 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48

Tgt Ion:252 Resp: 276781
Ion Ratio Lower Upper
252 100
253 23.3 17.0 25.4
125 8.3 7.8 11.6





#90

Benzo(a)pyrene

Concen: 73.785 ng

RT: 15.515 min Scan# 21

Delta R.T. 0.018 min

Lab File: BF133946.D

Acq: 23 Jun 2023 16:48

Instrument :

BNA_F

ClientSampleId :





COMPOSITE-SB17

Tgt Ion:252 Resp: 53211
 Ion Ratio Lower Upper
 252 100
 253 22.2 17.1 25.7
 125 9.4 8.6 13.0

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :mohammad ahmed 06/27/2023



#91

Dibenzo(a,h)anthracene

Concen: 10.183 ng




RT: 17.145 min Scan# 2560


Delta R.T. 0.006 min

Lab File: BF133946.D

Acq: 23 Jun 2023 16:48

Tgt Ion:278 Resp: 74192
 Ion Ratio Lower Upper
 278 100
 139 13.9 11.4 17.2
 279 25.9 19.0 28.4






#92
Benzo(g,h,i)perylene
Concen: 34.218 ng
RT: 17.603 min Scan# 20
Delta R.T. 0.012 min
Lab File: BF133946.D
Acq: 23 Jun 2023 16:48

Instrument :

BNA_F

ClientSampleId :

COMPOSITE-SB17



Tgt Ion:276 Resp: 247180
Ion Ratio Lower Upper
276 100
277 25.2 19.8 29.8
138 18.9 15.0 22.4

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/26/2023

Supervised By :mohammad ahmed 06/27/2023

