

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062323\
 Data File : BF133932.D
 Acq On : 23 Jun 2023 09:12
 Operator : CG\JU
 Sample : PB153615BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB153615BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.140	515	519	525	rBV	41624	60305	1.26%	0.225%
2	5.504	576	581	584	rBV	3482565	3676308	76.76%	13.712%
3	6.504	744	751	754	rBV	3042484	3737539	78.04%	13.940%
4	6.857	808	811	815	rBV	734330	614737	12.84%	2.293%
5	7.428	902	908	911	rBV	2441622	2472143	51.62%	9.221%
6	8.139	1025	1029	1034	rBV	963676	811841	16.95%	3.028%
7	9.222	1207	1213	1216	rBV	4968022	4371000	91.27%	16.303%
8	9.898	1324	1328	1331	rBV	1151211	918175	19.17%	3.425%
9	10.692	1458	1463	1467	rBV	2850033	3050715	63.70%	11.378%
10	11.392	1578	1582	1589	rBV	1211375	1027499	21.45%	3.832%
11	12.998	1849	1855	1858	rBV	4565915	4789274	100.00%	17.863%
12	14.051	2030	2034	2042	rVB	761346	700751	14.63%	2.614%
13	15.562	2285	2291	2302	rBV	417791	580999	12.13%	2.167%




Sum of corrected areas: 26811286

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062323\
Data File : BF133932.D
Acq On : 23 Jun 2023 09:12
Operator : CG\JU
Sample : PB153615BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153615BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

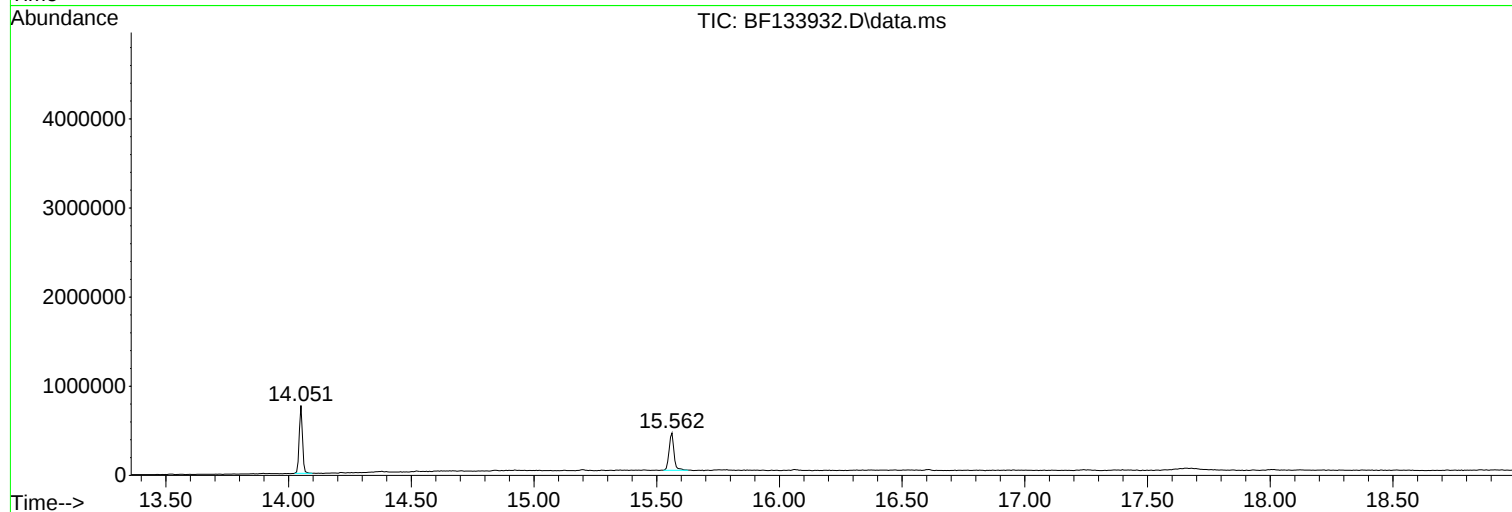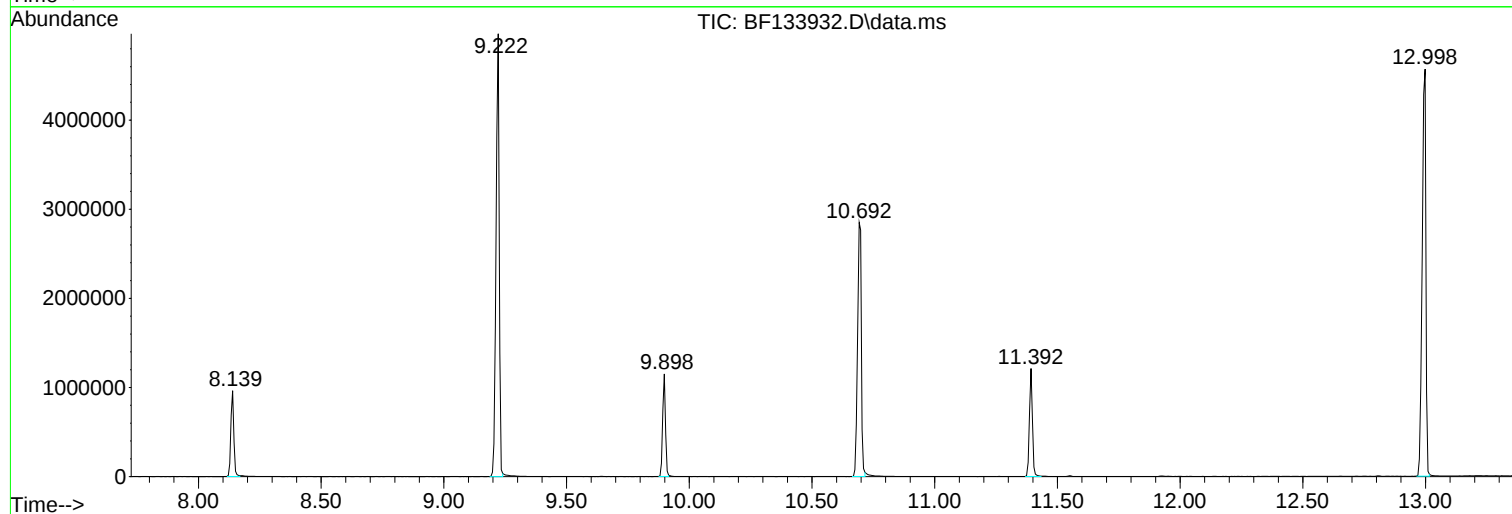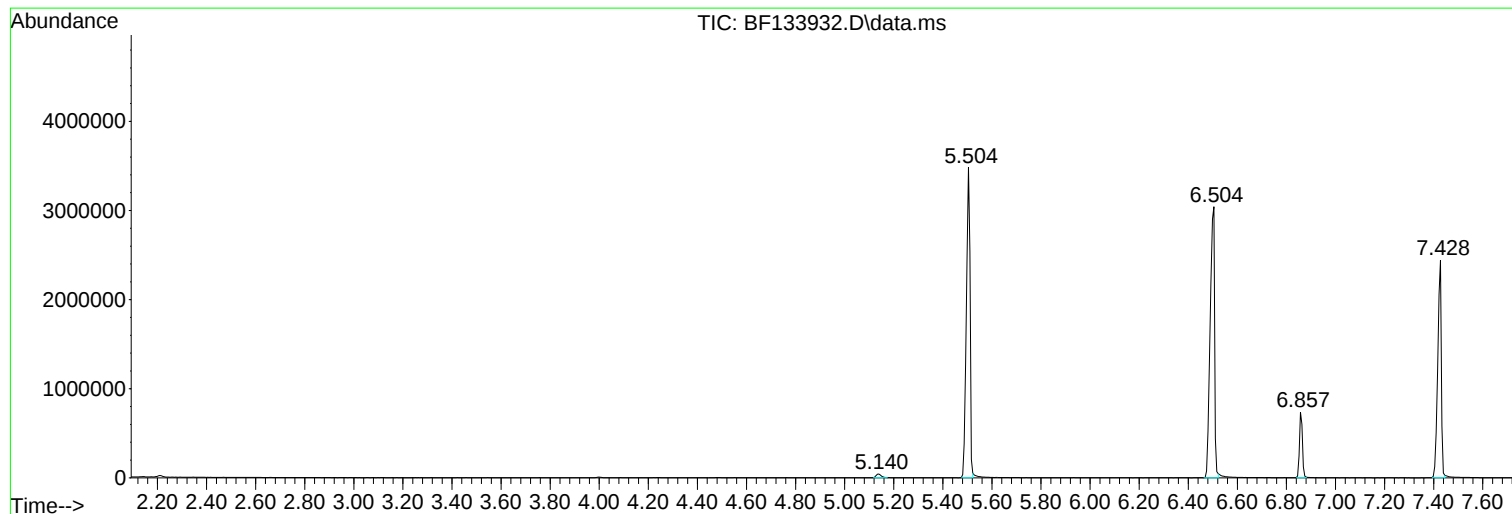

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062323\
Data File : BF133932.D
Acq On : 23 Jun 2023 09:12
Operator : CG\JU
Sample : PB153615BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153615BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062323\
Data File : BF133932.D
Acq On : 23 Jun 2023 09:12
Operator : CG\JU
Sample : PB153615BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB153615BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------