
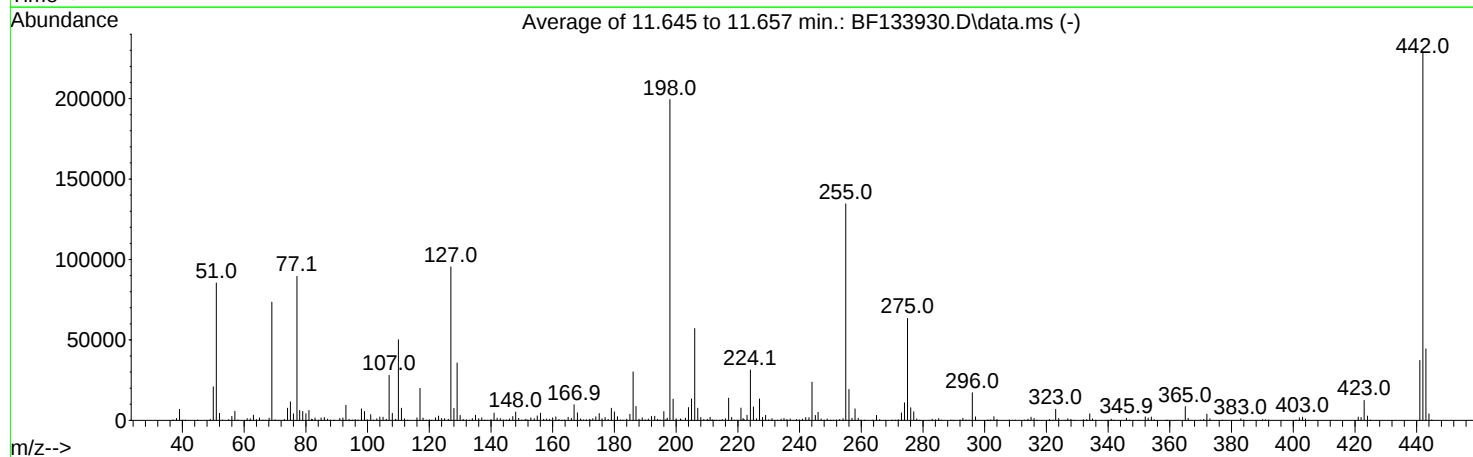


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062323\
Data File : BF133930.D
Acq On : 23 Jun 2023 08:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 23 02:21:26 2023

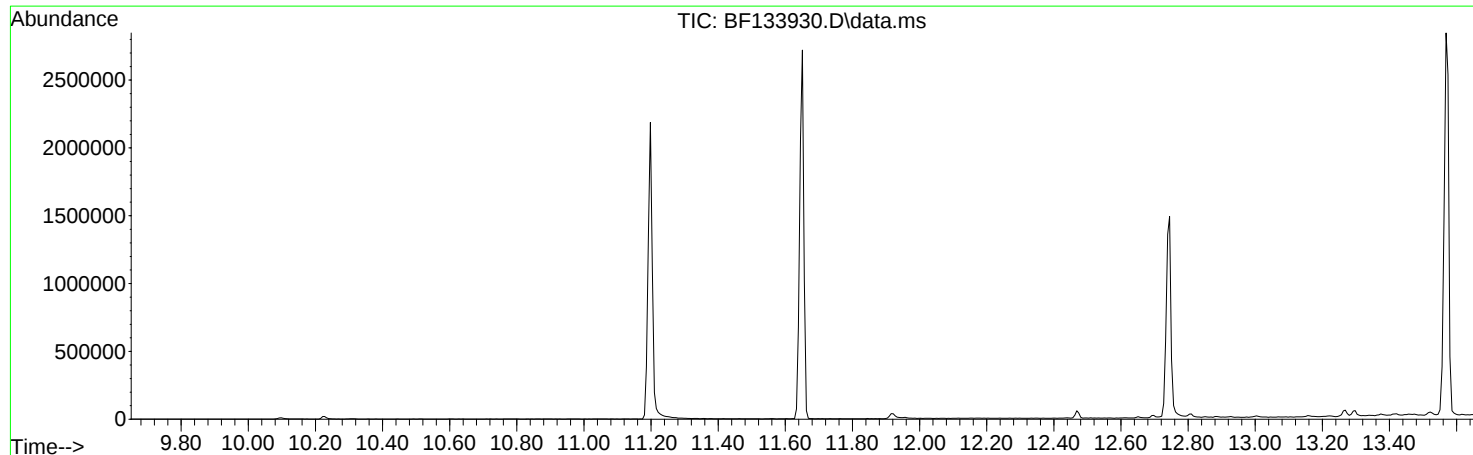

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	85443	PASS
68	69	0.00	2	1.9	1369	PASS
69	198	0.00	100	36.8	73462	PASS
70	69	0.00	2	0.5	397	PASS
127	198	10	80	47.8	95360	PASS
197	198	0.00	2	0.7	1429	PASS
198	198	100	100	100.0	199421	PASS
199	198	5	9	6.6	13229	PASS
275	198	10	60	31.8	63371	PASS
365	198	1	100	4.3	8562	PASS
441	198	0.01	100	18.7	37280	PASS
442	442	50	100	100.0	228651	PASS
443	442	15	24	19.4	44464	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/23/2023	BNA_F	<u>BF133930.D</u>
Compound Name	Response	Retention Time
DDT	522908	13.568
DDD	15124	13.268
DDE	633	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15757	538665	2.93

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062323\
Data File : BF133930.D
Acq On : 23 Jun 2023 08:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 25 04:46:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 02:21:26 2023
Response via : Initial Calibration

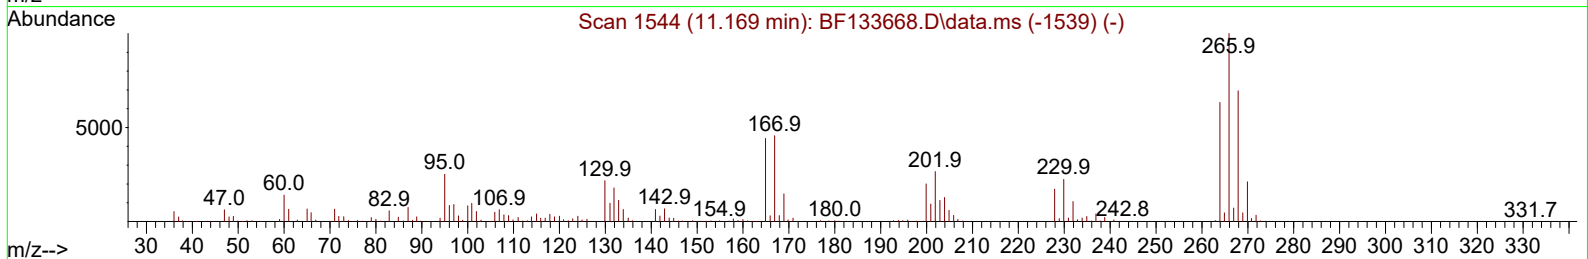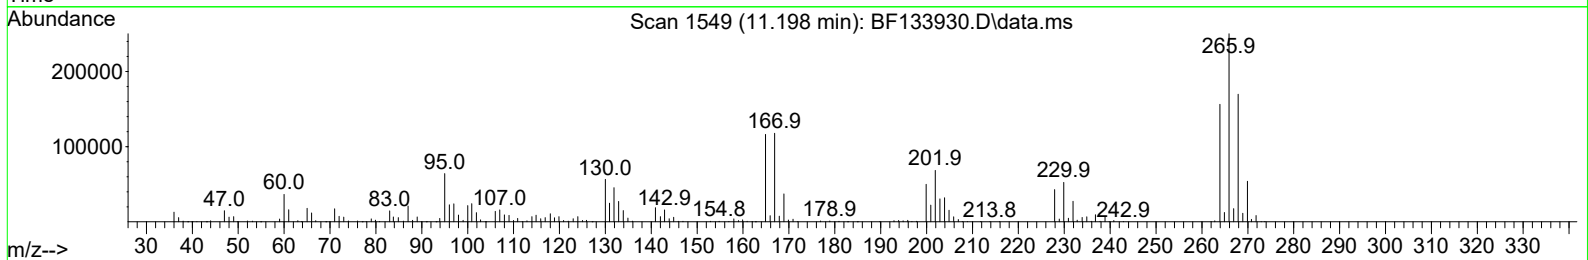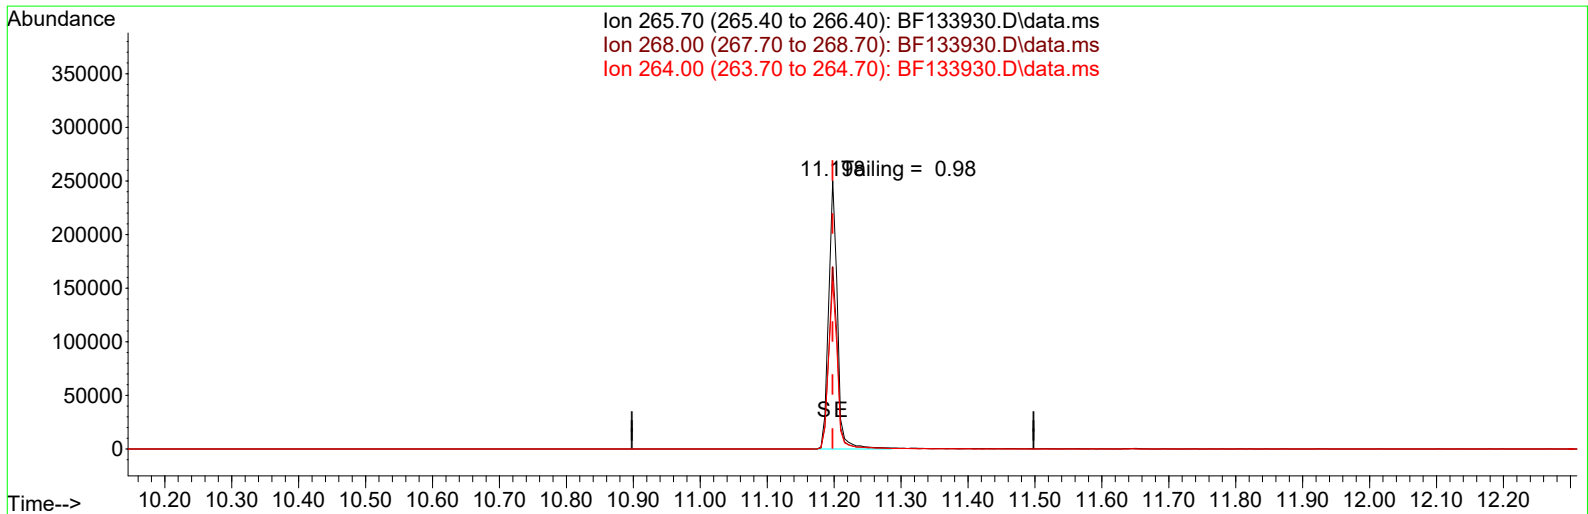

TIC: BF133930.D\data.ms

(70) Pentachlorophenol (C)

11.198min (+ 0.000) 232205.61 ng




response 230110

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.60	67.89
264.00	63.40	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062323\
Data File : BF133930.D
Acq On : 23 Jun 2023 08:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 25 04:46:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 23 02:21:26 2023
Response via : Initial Calibration

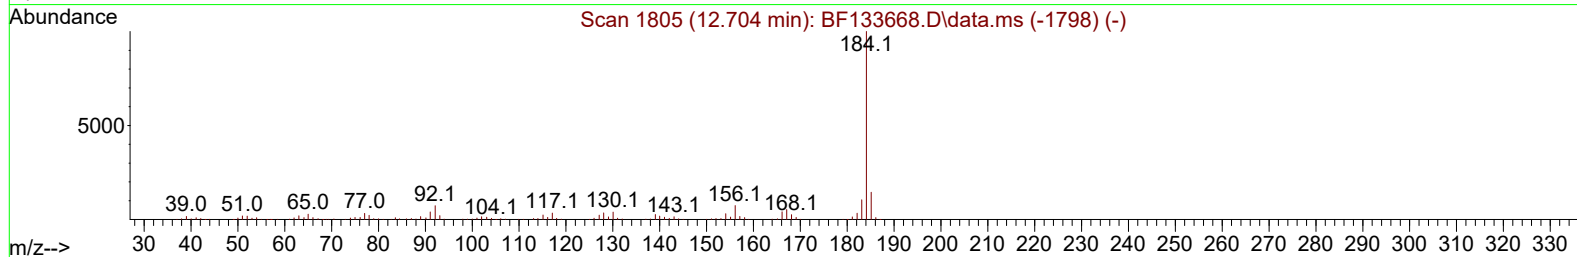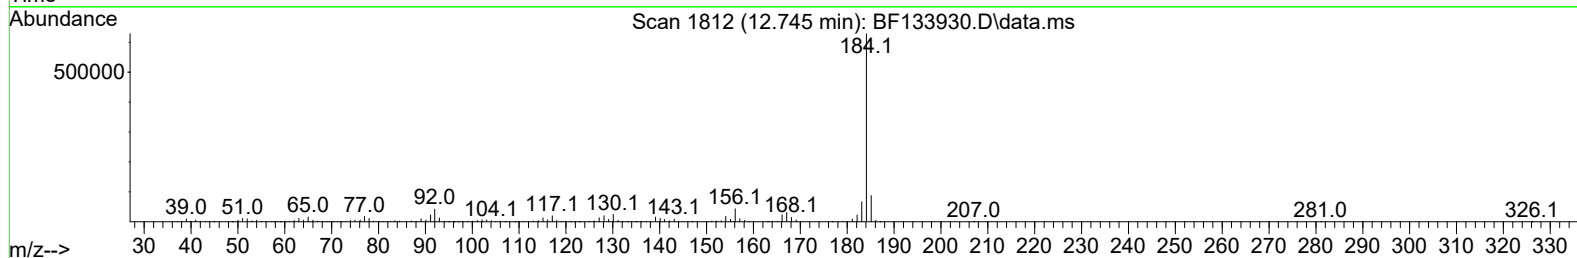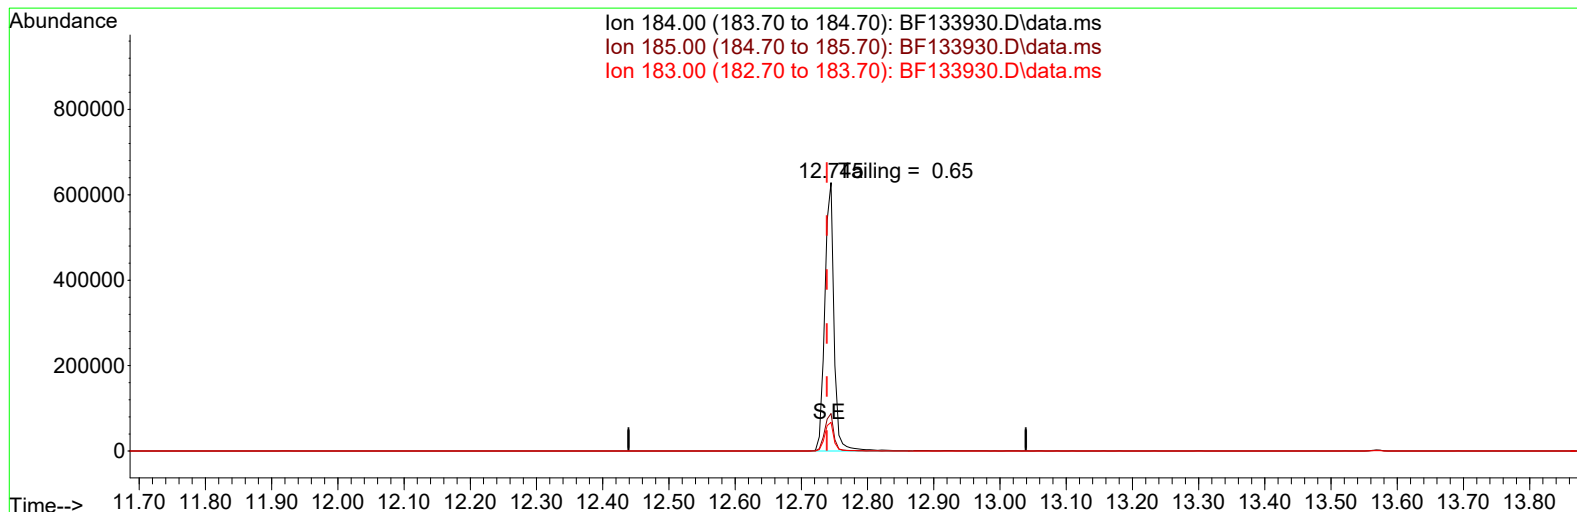

TIC: BF133930.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 46048.89 ng

response 610360

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.99
183.00	10.50	10.68
0.00	0.00	0.00