
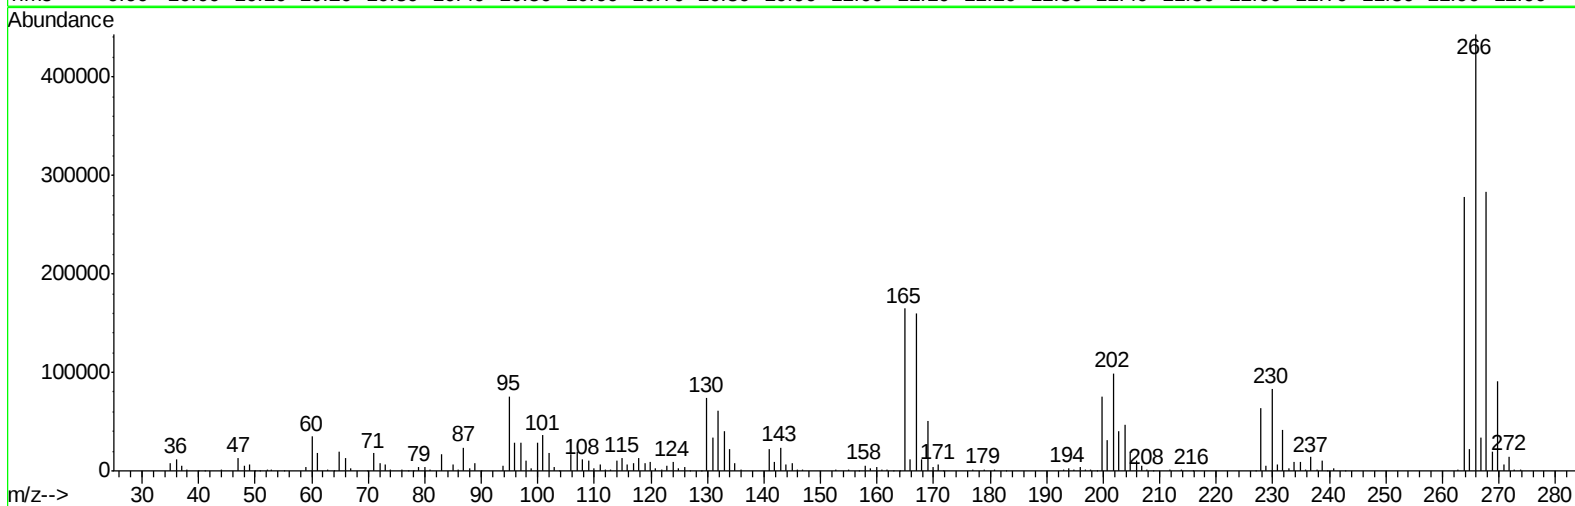


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062519\
Data File : BF115176.D
Acq On : 25 Jun 2019 8:27
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 09:47:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

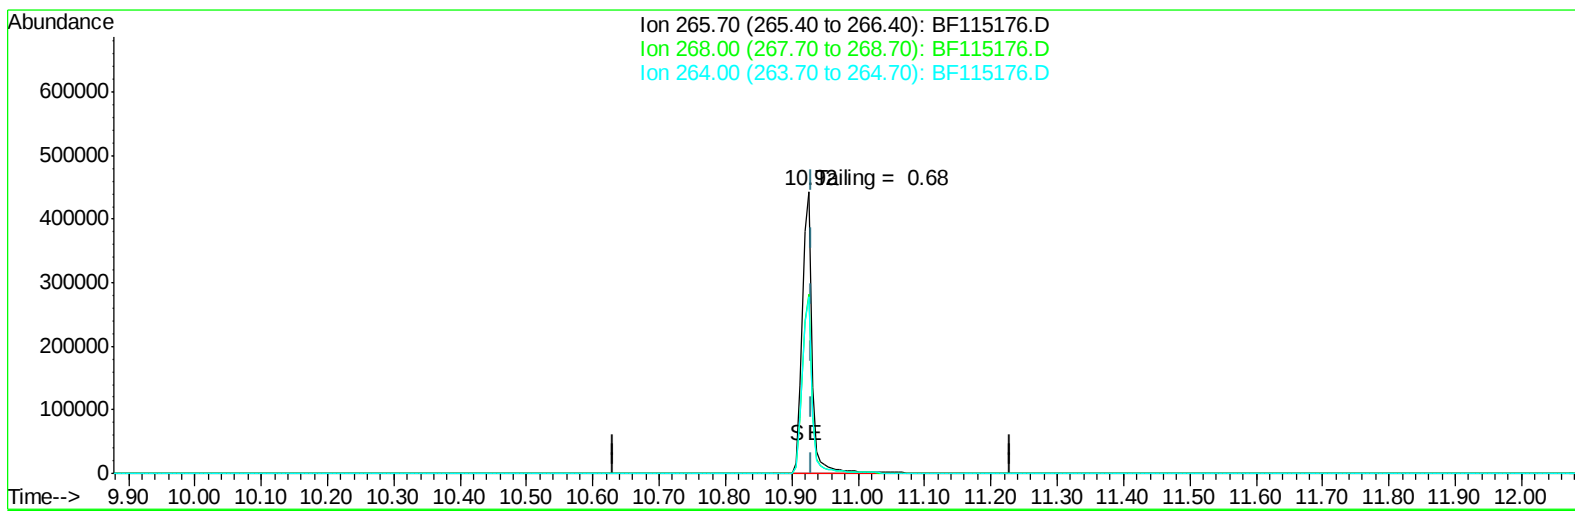

TIC: BF115176.D

(70) Pentachlorophenol (C)



10.925min (-0.006) 225742.56ng

response 441732

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	63.85
264.00	61.60	62.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062519\
Data File : BF115176.D
Acq On : 25 Jun 2019 8:27
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 09:47:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

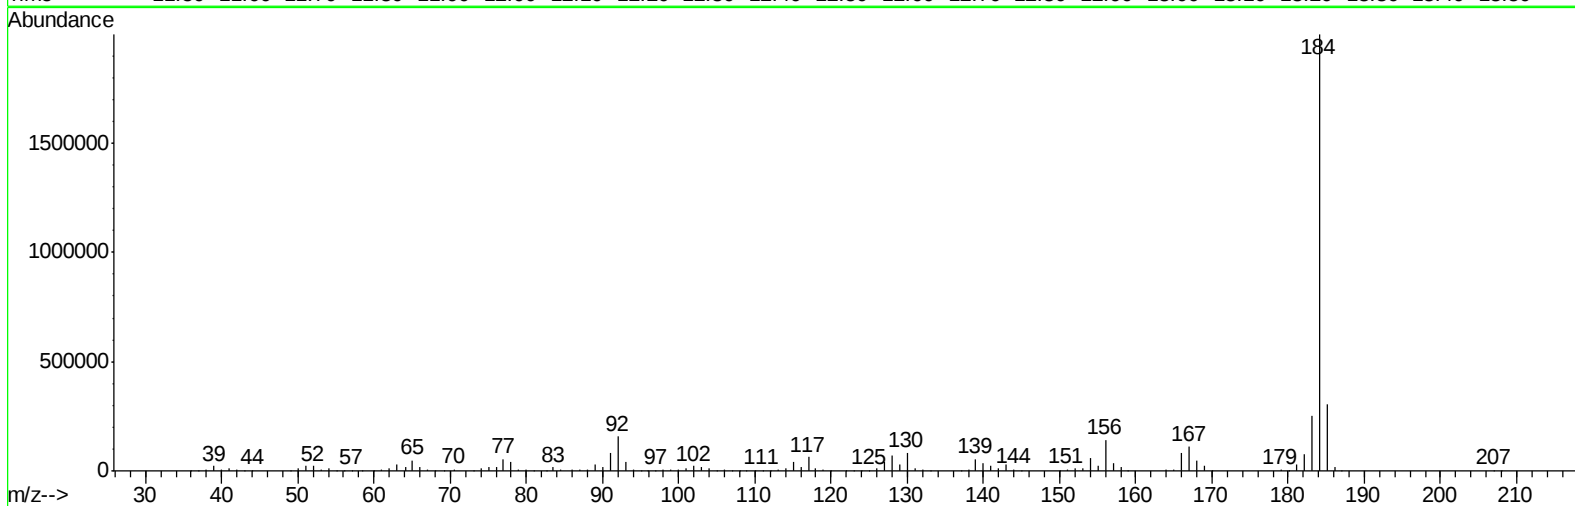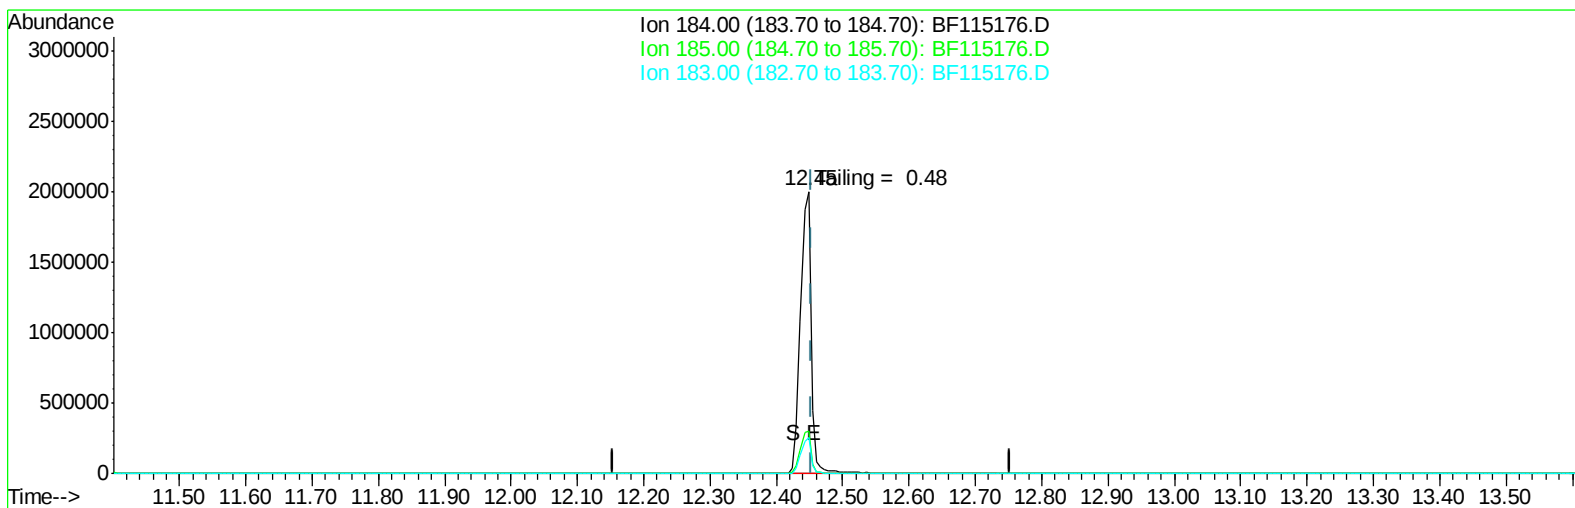

TIC: BF115176.D

(77) Benzidine

12.448min (-0.006) 155638.92ng

response 2142407

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.21
183.00	12.00	12.54
0.00	0.00	0.00