
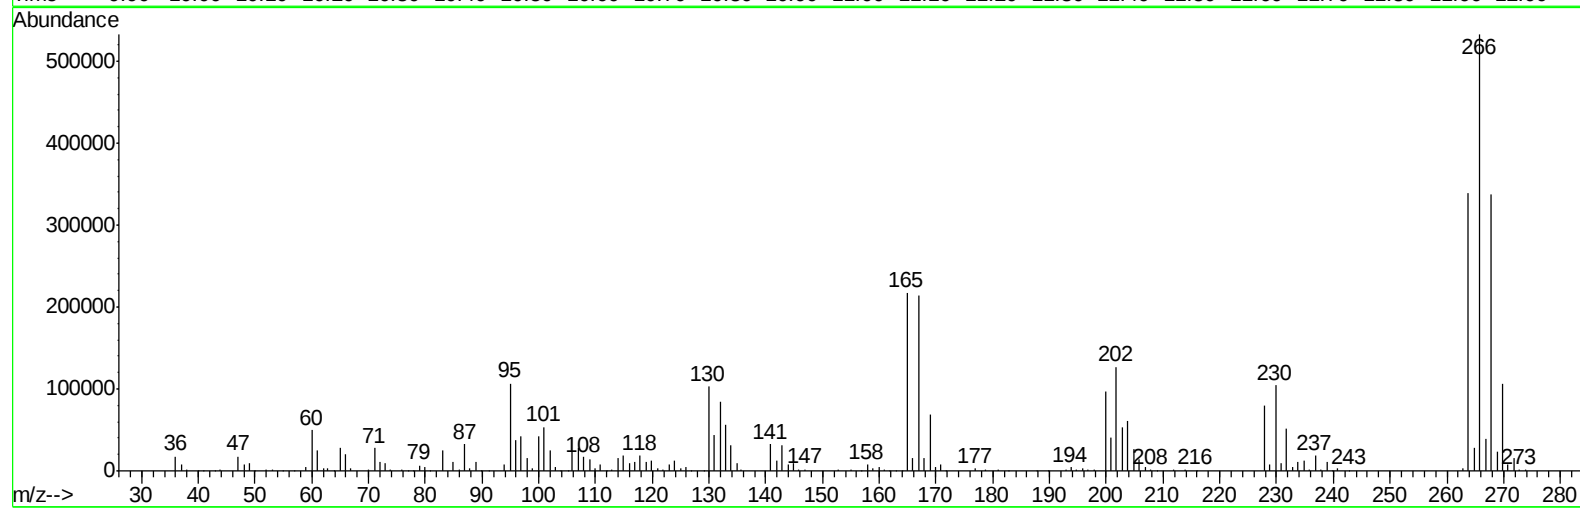


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062519\
Data File : BF115191.D
Acq On : 25 Jun 2019 17:00
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 07:57:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 04:21:29 2019
Response via : Initial Calibration

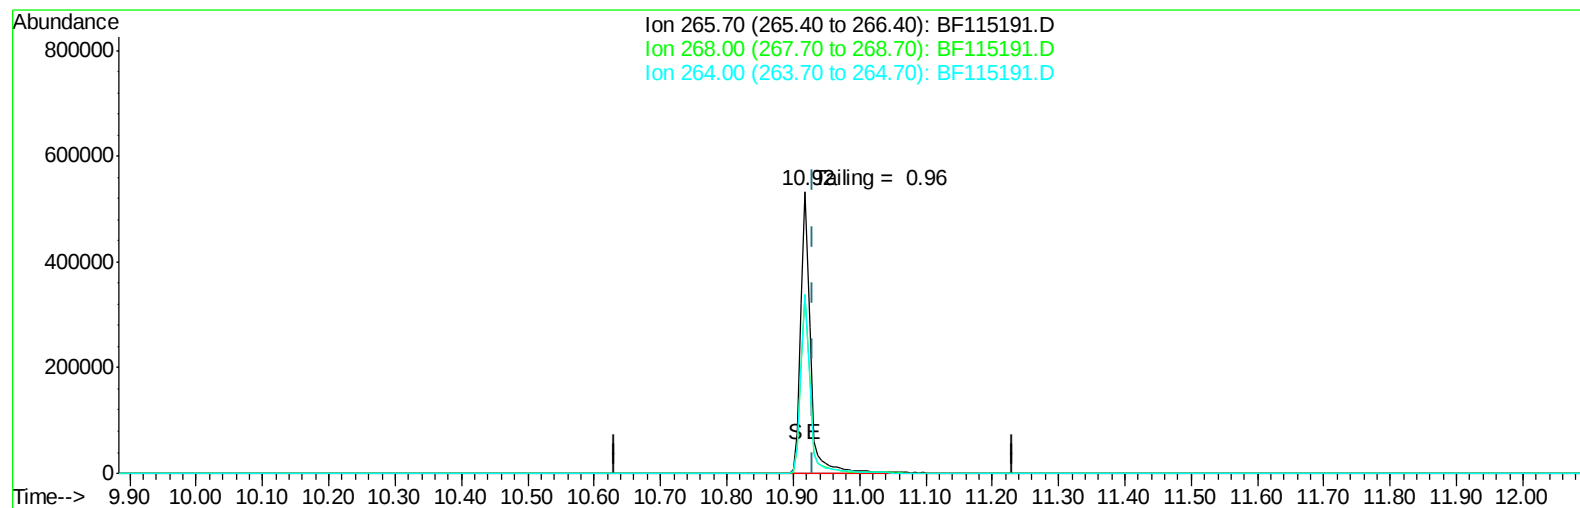

TIC: BF115191.D

(70) Pentachlorophenol (C)



10.918min (-0.012) 221640.34ng

response 516790

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	63.29
264.00	61.60	63.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062519\
 Data File : BF115191.D
 Acq On : 25 Jun 2019 17:00
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 07:57:56 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 24 04:21:29 2019
 Response via : Initial Calibration

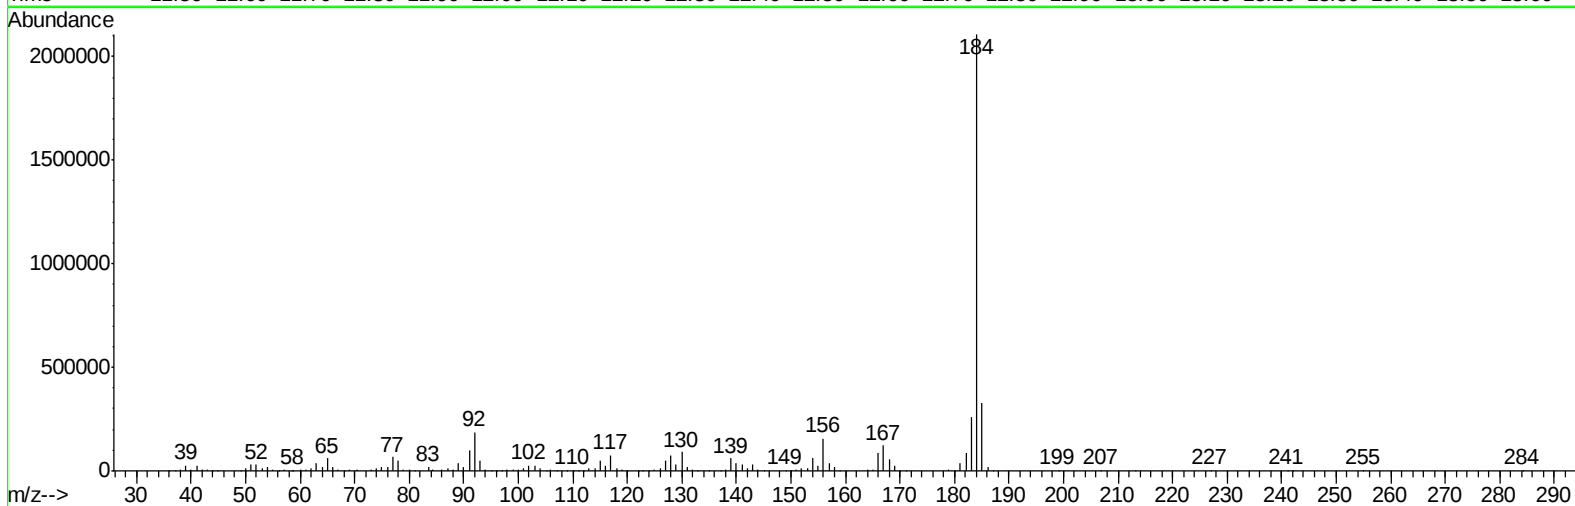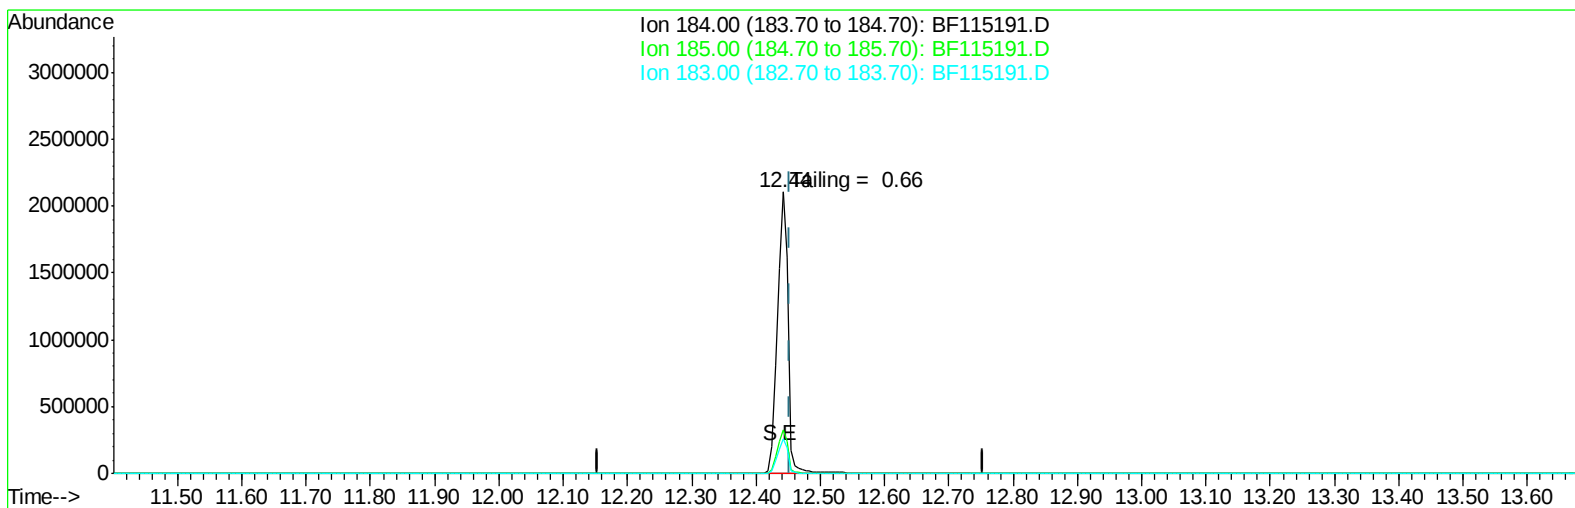

TIC: BF115191.D

(77) Benzidine

12.442min (-0.012) 128362.19ng

response 2382514

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.59
183.00	12.00	12.34
0.00	0.00	0.00