

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062519\
 Data File : BF115180.D
 Acq On : 25 Jun 2019 10:44
 Operator : HP/JU
 Sample : PB120877BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120877BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.219	552	558	561	rBV	5322412	5671381	72.10%	9.450%
2	6.254	727	734	737	rBV	5144446	5754095	73.15%	9.588%
3	6.384	750	756	759	rBV	5618916	6051514	76.94%	10.083%
4	6.613	791	795	798	rBV	1762674	1584263	20.14%	2.640%
5	6.766	817	821	825	rBV	5183745	4929293	62.67%	8.213%
6	7.172	884	890	893	rBV	3782773	3836250	48.77%	6.392%
7	7.889	1007	1012	1016	rBV	2325179	2068793	26.30%	3.447%
8	8.972	1190	1196	1199	rBV	6744013	7327814	93.16%	12.210%
9	9.636	1304	1309	1328	rBV	2558913	2453647	31.19%	4.088%
10	10.419	1436	1442	1445	rBV	4480816	4390781	55.82%	7.316%
11	11.107	1555	1559	1563	rBV	3090176	2656361	33.77%	4.426%
12	12.695	1824	1829	1832	rBV	7125908	7865697	100.00%	13.106%
13	13.724	2000	2004	2015	rBV	2463998	2458023	31.25%	4.096%
14	14.824	2188	2191	2197	rVB	103109	116193	1.48%	0.194%
15	15.089	2231	2236	2244	rBV	1664306	2237448	28.45%	3.728%
16	15.165	2245	2249	2256	rVB	151919	208312	2.65%	0.347%
17	15.542	2309	2313	2320	rVB	120165	172563	2.19%	0.288%
18	15.983	2384	2388	2399	rVB	89716	153803	1.96%	0.256%
19	16.507	2472	2477	2485	rVB3	40738	79667	1.01%	0.133%


Sum of corrected areas: 60015898

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062519\
Data File : BF115180.D
Acq On : 25 Jun 2019 10:44
Operator : HP/JU
Sample : PB120877BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120877BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

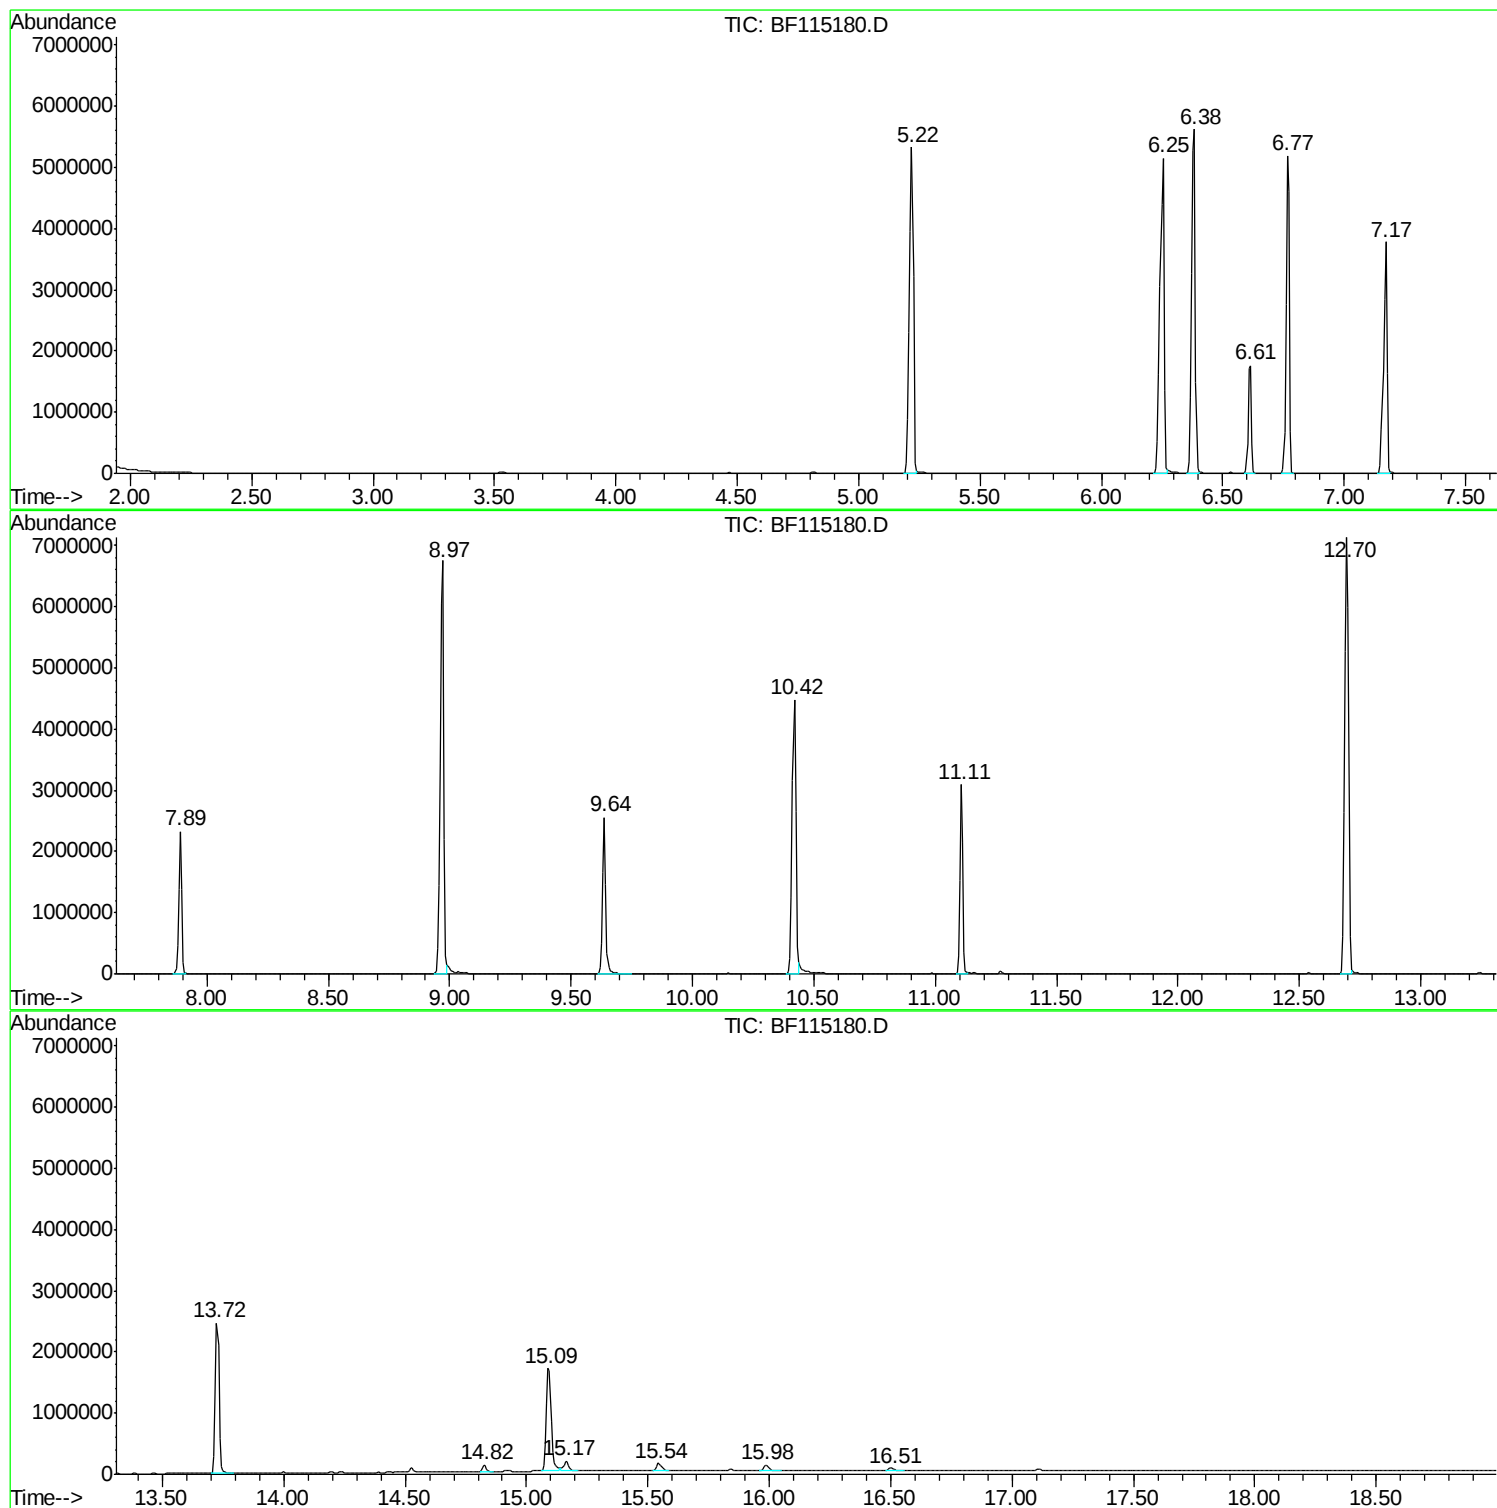

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062519\
Data File : BF115180.D
Acq On : 25 Jun 2019 10:44
Operator : HP/JU
Sample : PB120877BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120877BL









Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	76.40 ng	6051510	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	16
4		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9
5		Cyclopropanamine, 1-phenyl-	133	C9H11N	1000351-26-2	9

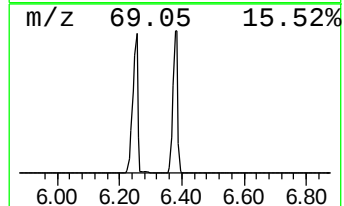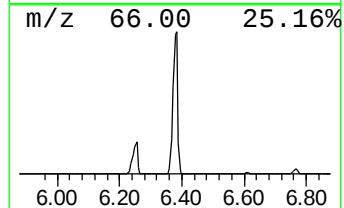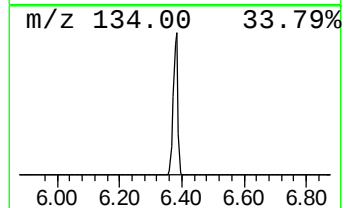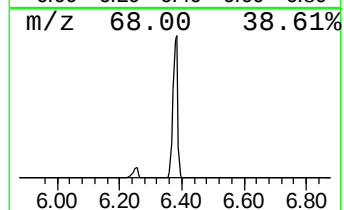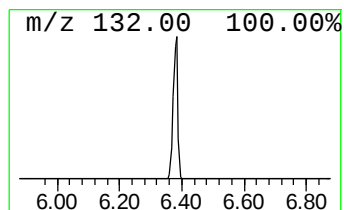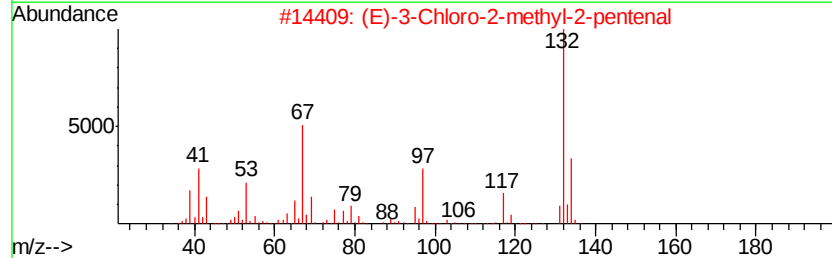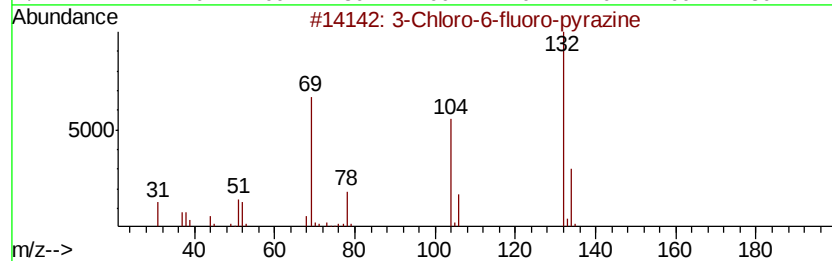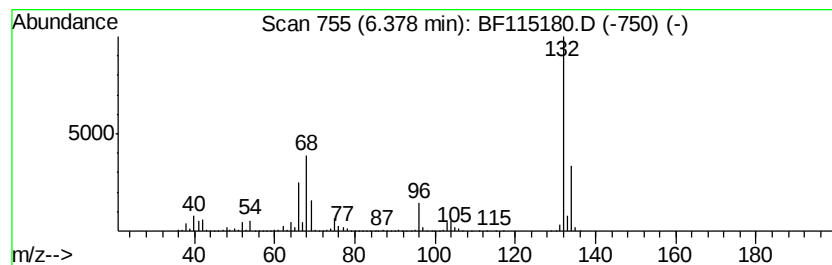

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062519\
Data File : BF115180.D
Acq On : 25 Jun 2019 10:44
Operator : HP/JU
Sample : PB120877BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120877BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.38	6.38	76.4	ng	6051510	1	6.61	1584260	20.0